

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111522\
 Data File : VU051861.D
 Acq On : 15 Nov 2022 15:58
 Operator : JC/MD
 Sample : VU1115MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK009

Quant Time: Nov 16 01:10:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 16 01:02:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	472409	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	466830	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	169822	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	110264	47.544	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	95.080%	
7) Chloroethane-d5	1.903	69	117995	50.780	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	101.560%	
11) 1,1-Dichloroethene-d2	2.565	63	134200	32.268	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	64.540%	
21) 2-Butanone-d5	4.616	46	255502	96.884	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	96.880%	
24) Chloroform-d	5.060	84	276848	47.620	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.240%	
26) 1,2-Dichloroethane-d4	5.700	65	175909	49.429	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.860%	
32) Benzene-d6	5.726	84	497750	51.137	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	102.280%	
36) 1,2-Dichloropropane-d6	6.687	67	187957	51.877	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	103.760%	
41) Toluene-d8	7.896	98	367613	46.013	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	92.020%	
43) trans-1,3-Dichloroprop...	8.179	79	66872	46.338	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	92.680%	
47) 2-Hexanone-d5	8.629	63	173105	94.009	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	94.010%	
56) 1,1,2,2-Tetrachloroeth...	10.754	84	335013	47.509	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	95.020%	
66) 1,2-Dichlorobenzene-d4	12.192	152	166243	55.626	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	111.260%	
Target Compounds						
13) Acetone	2.623	43	7297	2.586	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111522\
Data File : VU051861.D
Acq On : 15 Nov 2022 15:58
Operator : JC/MD
Sample : VU1115MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK009

Quant Time: Nov 16 01:10:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 16 01:02:23 2022
Response via : Initial Calibration

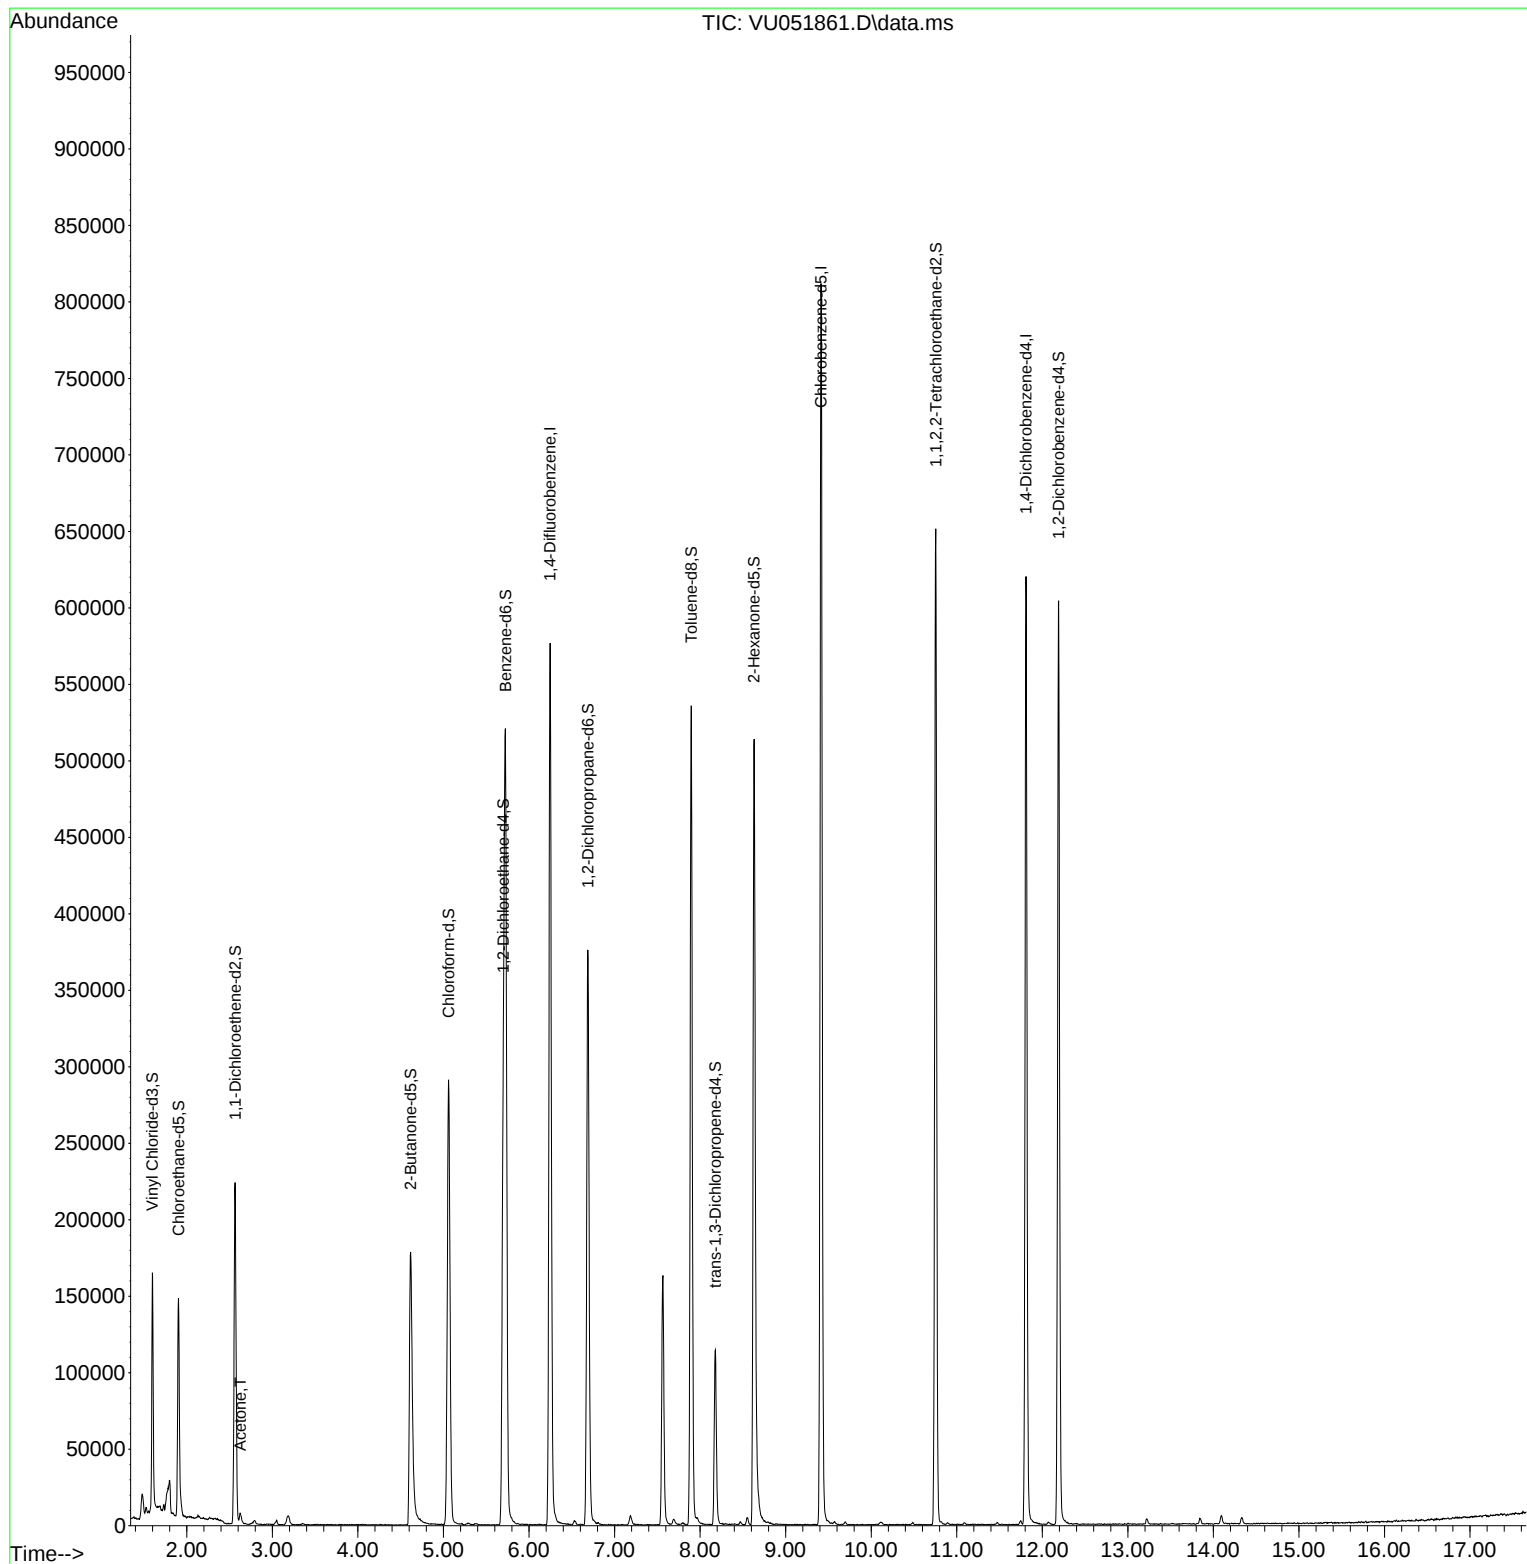

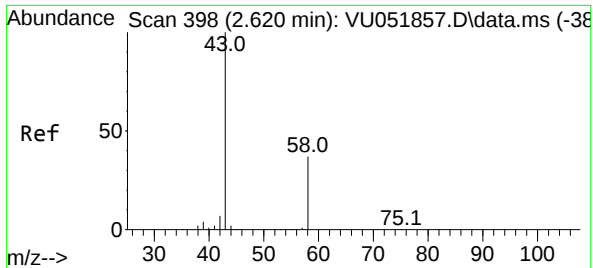

#13
 Acetone
 Concen: 2.586 ug/L
 RT: 2.623 min Scan# 398
 Delta R.T. 0.003 min
 Lab File: VU051861.D
 Acq: 15 Nov 2022 15:58

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK009

Tgt Ion: 43 Resp: 7297
 Ion Ratio Lower Upper
 43 100
 58 34.0 0.0 75.4

