

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111522\
 Data File : VU051863.D
 Acq On : 15 Nov 2022 16:47
 Operator : JC/MD
 Sample : VU1115WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK011

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

Signal : TIC: VU051863.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.478	34	43	53	rBV2	17165	36702	2.52%	0.306%
2	1.600	74	81	97	rVB	152078	175551	12.07%	1.464%
3	1.906	167	176	199	rVB	140947	204150	14.03%	1.702%
4	2.565	368	381	396	rBV	223842	366129	25.17%	3.053%
5	2.742	434	436	441	rVB2	388	288	0.02%	0.002%
6	2.793	443	452	457	rVV2	1317	1976	0.14%	0.016%
7	2.935	490	496	499	rBV	267	343	0.02%	0.003%
8	3.044	520	530	544	rVB2	6448	11743	0.81%	0.098%
9	3.115	550	552	560	rVB2	382	289	0.02%	0.002%
10	3.182	564	573	585	rBV3	1431	2946	0.20%	0.025%
11	3.253	592	595	599	rBV2	471	460	0.03%	0.004%
12	3.334	617	620	622	rBV2	363	270	0.02%	0.002%
13	3.356	624	627	631	rVB3	621	570	0.04%	0.005%
14	3.379	631	634	638	rBV3	316	279	0.02%	0.002%
15	3.665	718	723	727	rBV2	362	322	0.02%	0.003%
16	3.697	727	733	738	rVB2	279	341	0.02%	0.003%
17	4.616	1007	1019	1048	rBV	184929	449236	30.88%	3.746%
18	4.993	1131	1136	1137	rBV2	342	295	0.02%	0.002%
19	5.060	1140	1157	1179	rBV	289918	637521	43.82%	5.316%
20	5.269	1216	1222	1224	rBV3	401	399	0.03%	0.003%
21	5.292	1224	1229	1234	rVV5	878	1023	0.07%	0.009%
22	5.369	1248	1253	1255	rBV2	702	601	0.04%	0.005%
23	5.481	1281	1288	1293	rBV2	224	296	0.02%	0.002%
24	5.613	1326	1329	1333	rVB2	296	228	0.02%	0.002%
25	5.723	1341	1363	1395	rBV2	515820	1454826	100.00%	12.131%
26	6.112	1479	1484	1486	rBV3	277	281	0.02%	0.002%
27	6.179	1502	1505	1507	rBV2	370	278	0.02%	0.002%
28	6.247	1512	1526	1550	rBV	576561	1109617	76.27%	9.253%
29	6.533	1607	1615	1627	rVB6	2532	4816	0.33%	0.040%
30	6.604	1632	1637	1643	rVB5	509	704	0.05%	0.006%
31	6.687	1649	1663	1684	rBV	375834	723564	49.74%	6.034%
32	6.861	1713	1717	1721	rBV3	489	408	0.03%	0.003%
33	7.147	1801	1806	1808	rBV	411	268	0.02%	0.002%
34	7.182	1810	1817	1829	rBV2	6272	10300	0.71%	0.086%
35	7.301	1849	1854	1861	rBV2	539	785	0.05%	0.007%
36	7.340	1863	1866	1871	rVV	322	321	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111522\
 Data File : VU051863.D
 Acq On : 15 Nov 2022 16:47
 Operator : JC/MD
 Sample : VU1115WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK011

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

37	7.394	1878	1883	1886	rBV2	314	292	0.02%	0.002%
38	7.562	1923	1935	1956	rBV	163057	288528	19.83%	2.406%
39	7.687	1968	1974	1984	rBV4	2742	4675	0.32%	0.039%
40	7.793	2004	2007	2011	rBV3	407	346	0.02%	0.003%
41	7.896	2026	2039	2063	rBV	539776	920314	63.26%	7.674%
42	8.105	2102	2104	2110	rVB3	391	298	0.02%	0.002%
43	8.176	2114	2126	2149	rBV	116347	196922	13.54%	1.642%
44	8.327	2170	2173	2175	rBV2	361	228	0.02%	0.002%
45	8.417	2198	2201	2204	rVB	505	366	0.03%	0.003%
46	8.472	2211	2218	2220	rBV3	1007	932	0.06%	0.008%
47	8.513	2227	2231	2234	rBV2	486	364	0.03%	0.003%
48	8.552	2234	2243	2252	rBV5	3411	5754	0.40%	0.048%
49	8.629	2256	2267	2295	rBV2	520162	974024	66.95%	8.122%
50	8.819	2324	2326	2328	rVB	599	279	0.02%	0.002%
51	8.909	2349	2354	2360	rBV2	381	469	0.03%	0.004%
52	9.015	2383	2387	2389	rBV3	338	284	0.02%	0.002%
53	9.147	2425	2428	2433	rVB2	233	230	0.02%	0.002%
54	9.227	2448	2453	2456	rBV	417	409	0.03%	0.003%
55	9.246	2456	2459	2461	rVV2	339	232	0.02%	0.002%
56	9.414	2497	2511	2540	rBV	807251	1350609	92.84%	11.262%
57	9.613	2571	2573	2576	rVB2	435	245	0.02%	0.002%
58	9.697	2591	2599	2605	rBV3	692	1006	0.07%	0.008%
59	9.861	2646	2650	2653	rVB	490	394	0.03%	0.003%
60	9.896	2653	2661	2666	rBV2	343	612	0.04%	0.005%
61	10.034	2698	2704	2705	rBV	261	234	0.02%	0.002%
62	10.047	2705	2708	2713	rVB2	336	296	0.02%	0.002%
63	10.102	2722	2725	2730	rVV	534	460	0.03%	0.004%
64	10.127	2730	2733	2738	rVB2	403	351	0.02%	0.003%
65	10.478	2837	2842	2852	rVB2	576	874	0.06%	0.007%
66	10.526	2853	2857	2861	rBV	240	248	0.02%	0.002%
67	10.623	2881	2887	2891	rBV2	433	424	0.03%	0.004%
68	10.751	2915	2927	2960	rBV	642840	1039778	71.47%	8.670%
69	10.989	2996	3001	3004	rBV2	363	397	0.03%	0.003%
70	11.044	3013	3018	3022	rVB2	247	301	0.02%	0.003%
71	11.076	3022	3028	3030	rBV2	423	426	0.03%	0.004%
72	11.134	3043	3046	3048	rBV2	334	283	0.02%	0.002%
73	11.192	3062	3064	3069	rVB2	453	336	0.02%	0.003%
74	11.385	3119	3124	3128	rVB2	301	250	0.02%	0.002%
75	11.471	3146	3151	3154	rBV3	668	658	0.05%	0.005%
76	11.742	3231	3235	3242	rBV2	1031	1144	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111522\
 Data File : VU051863.D
 Acq On : 15 Nov 2022 16:47
 Operator : JC/MD
 Sample : VU1115WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK011

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

77	11.809	3244	3256	3279	rBV	615972	991909	68.18%	8.271%
78	11.983	3307	3310	3311	rBV	581	359	0.02%	0.003%
79	12.192	3361	3375	3399	rBV	597705	994017	68.33%	8.289%
80	12.346	3420	3423	3424	rBV	481	253	0.02%	0.002%
81	12.407	3439	3442	3446	rVB	384	278	0.02%	0.002%
82	12.491	3465	3468	3470	rBV2	468	276	0.02%	0.002%
83	12.529	3477	3480	3484	rBV3	594	392	0.03%	0.003%
84	12.549	3484	3486	3490	rVB	575	345	0.02%	0.003%
85	12.574	3490	3494	3496	rBV	371	277	0.02%	0.002%
86	12.690	3525	3530	3533	rBV	460	398	0.03%	0.003%
87	12.709	3533	3536	3539	rBV2	341	266	0.02%	0.002%
88	12.989	3616	3623	3626	rBV2	713	852	0.06%	0.007%
89	13.182	3678	3683	3685	rBV	459	401	0.03%	0.003%
90	13.230	3690	3698	3703	rVV6	1498	1887	0.13%	0.016%
91	13.404	3750	3752	3755	rBV2	408	253	0.02%	0.002%
92	13.481	3774	3776	3778	rBV2	397	262	0.02%	0.002%
93	13.629	3816	3822	3827	rBV2	696	773	0.05%	0.006%
94	13.844	3884	3889	3890	rBV2	1588	1146	0.08%	0.010%
95	13.954	3920	3923	3926	rBV3	383	307	0.02%	0.003%
96	14.047	3947	3952	3954	rBV4	563	516	0.04%	0.004%
97	14.295	4026	4029	4031	rBV2	389	297	0.02%	0.002%
98	14.336	4033	4042	4048	rBV7	1698	2960	0.20%	0.025%
99	14.622	4127	4131	4136	rBV2	1105	1203	0.08%	0.010%
100	14.745	4167	4169	4175	rVB2	485	334	0.02%	0.003%


Sum of corrected areas: 11992359

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111522\
Data File : VU051863.D
Acq On : 15 Nov 2022 16:47
Operator : JC/MD
Sample : VU1115WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK011

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

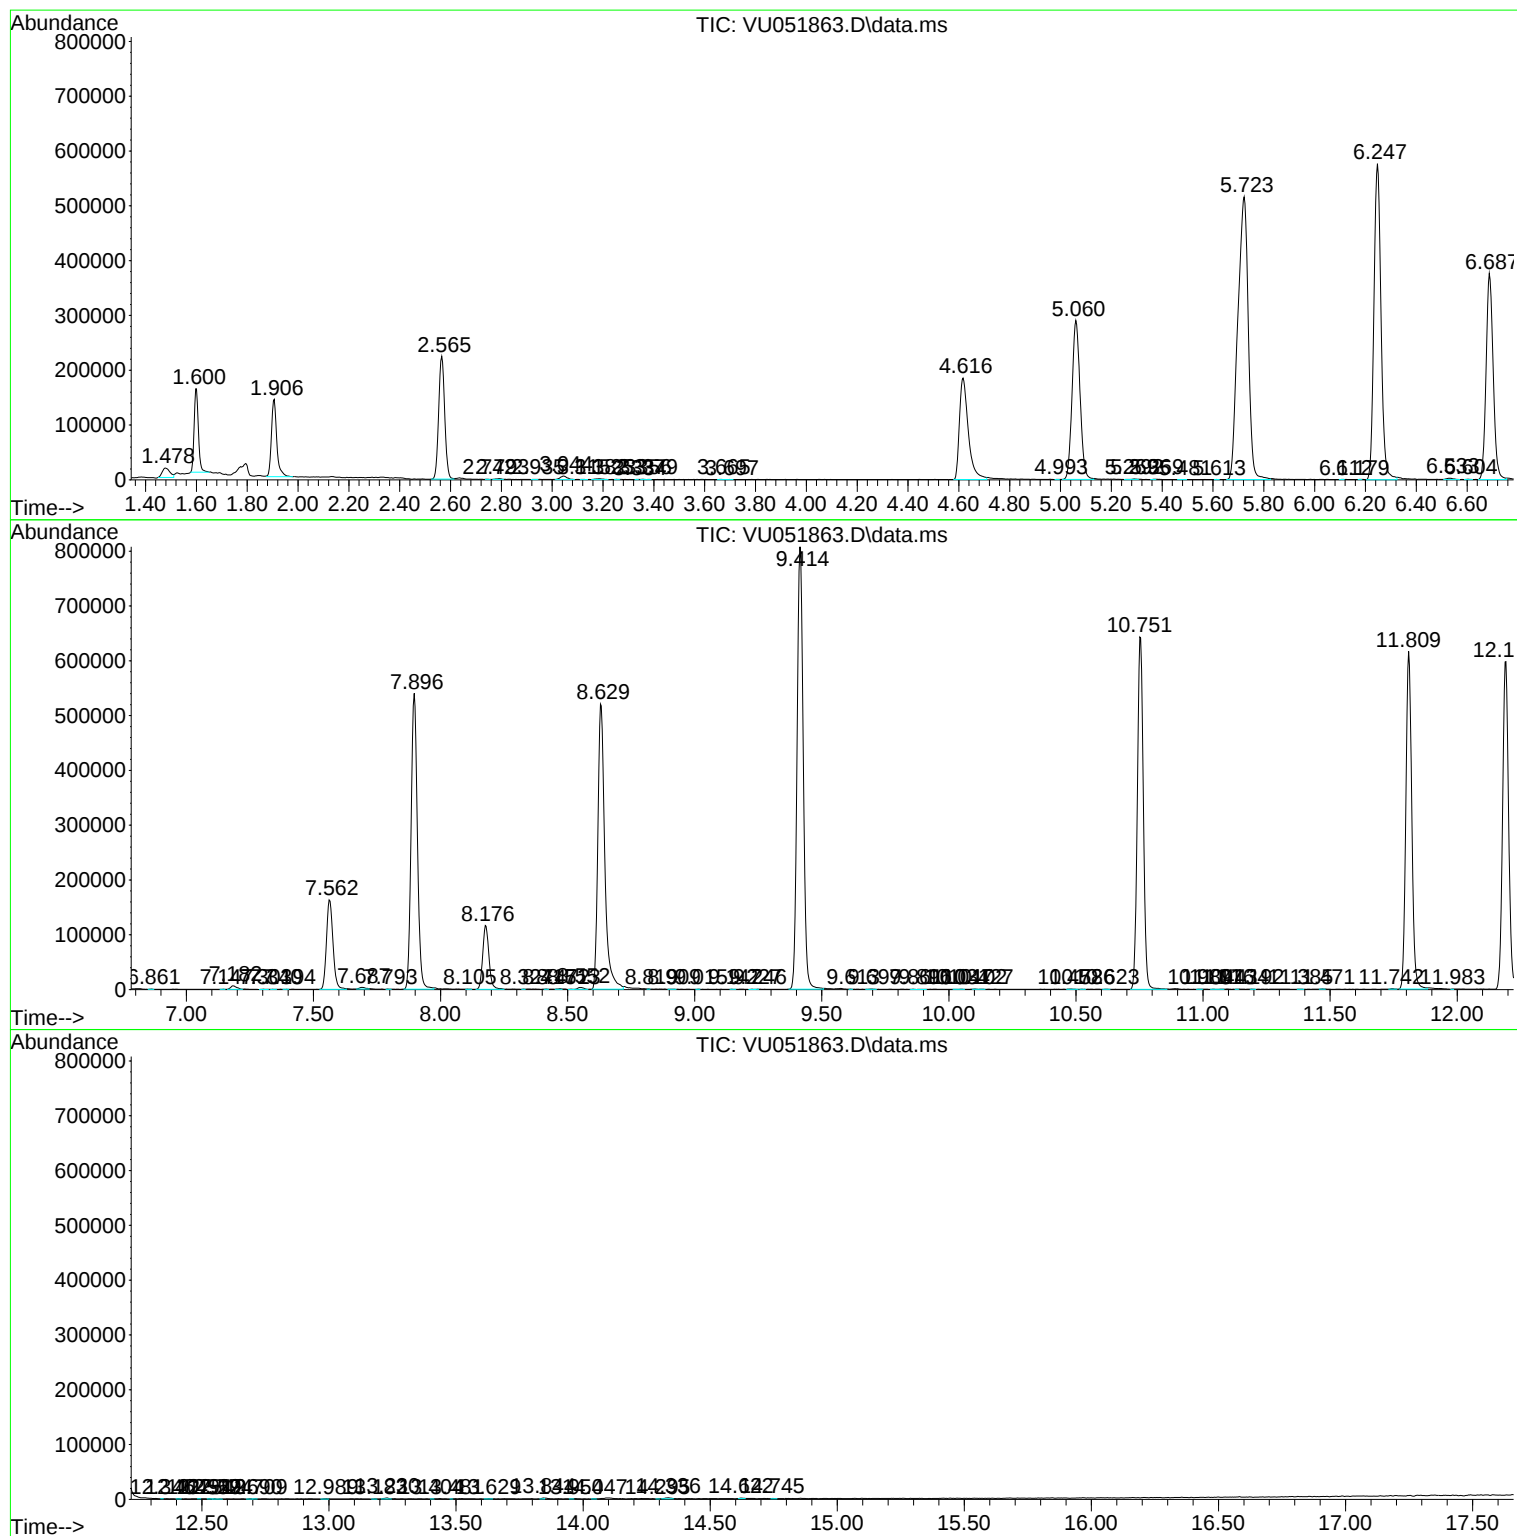

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111522\
Data File : VU051863.D
Acq On : 15 Nov 2022 16:47
Operator : JC/MD
Sample : VU1115WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK011

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111522\
Data File : VU051863.D
Acq On : 15 Nov 2022 16:47
Operator : JC/MD
Sample : VU1115WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK011

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc