

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111522\
 Data File : VU051864.D
 Acq On : 15 Nov 2022 17:11
 Operator : JC/MD
 Sample : VU1115WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK012

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M

Title : VOC Analysis

Signal : TIC: VU051864.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.481	34	44	52	rBV3	11595	24797	1.70%	0.205%
2	1.597	74	80	95	rBV	151200	173514	11.88%	1.432%
3	1.906	167	176	201	rVB	138375	203488	13.93%	1.679%
4	2.565	368	381	397	rBV	223439	362866	24.84%	2.994%
5	2.761	439	442	445	rBV2	659	522	0.04%	0.004%
6	2.970	505	507	511	rVB	530	295	0.02%	0.002%
7	3.044	520	530	546	rVB3	7765	13686	0.94%	0.113%
8	3.176	561	571	573	rBV2	3293	4202	0.29%	0.035%
9	3.350	620	625	627	rBV2	324	242	0.02%	0.002%
10	3.369	627	631	634	rBV2	292	328	0.02%	0.003%
11	3.449	652	656	662	rBV2	252	275	0.02%	0.002%
12	3.636	711	714	719	rVB2	461	396	0.03%	0.003%
13	3.668	719	724	727	rBV	382	330	0.02%	0.003%
14	3.800	762	765	768	rBV	388	281	0.02%	0.002%
15	4.044	838	841	847	rVB2	397	378	0.03%	0.003%
16	4.128	864	867	874	rVB2	361	367	0.03%	0.003%
17	4.282	911	915	920	rBV2	336	280	0.02%	0.002%
18	4.504	979	984	987	rBV	271	259	0.02%	0.002%
19	4.616	1005	1019	1046	rBV	191075	463383	31.72%	3.823%
20	4.841	1087	1089	1095	rVB3	488	382	0.03%	0.003%
21	4.906	1103	1109	1110	rBV	494	481	0.03%	0.004%
22	4.986	1128	1134	1136	rVV2	357	378	0.03%	0.003%
23	5.060	1141	1157	1182	rBV	291145	639132	43.74%	5.273%
24	5.269	1215	1222	1223	rBV2	530	497	0.03%	0.004%
25	5.285	1224	1227	1228	rBV3	510	256	0.02%	0.002%
26	5.327	1238	1240	1246	rVB3	409	337	0.02%	0.003%
27	5.359	1247	1250	1253	rBV2	357	282	0.02%	0.002%
28	5.427	1267	1271	1275	rBV2	357	284	0.02%	0.002%
29	5.491	1287	1291	1295	rVB3	339	279	0.02%	0.002%
30	5.722	1342	1363	1395	rBV2	521305	1461074	100.00%	12.054%
31	6.153	1493	1497	1500	rBV2	422	335	0.02%	0.003%
32	6.247	1511	1526	1562	rBV	583932	1112929	76.17%	9.182%
33	6.385	1567	1569	1573	rVB4	515	324	0.02%	0.003%
34	6.439	1584	1586	1598	rVB3	823	840	0.06%	0.007%
35	6.529	1606	1614	1615	rBV5	2723	3066	0.21%	0.025%
36	6.687	1646	1663	1684	rBV	368872	726620	49.73%	5.995%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111522\
 Data File : VU051864.D
 Acq On : 15 Nov 2022 17:11
 Operator : JC/MD
 Sample : VU1115WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK012

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

37	6.819	1702	1704	1714	rVB5	1235	1222	0.08%	0.010%
38	7.092	1783	1789	1792	rBV2	527	453	0.03%	0.004%
39	7.185	1810	1818	1830	rVV2	6909	11031	0.75%	0.091%
40	7.295	1849	1852	1858	rVB	310	296	0.02%	0.002%
41	7.333	1858	1864	1866	rBV2	419	394	0.03%	0.003%
42	7.382	1875	1879	1882	rBV	418	332	0.02%	0.003%
43	7.565	1923	1936	1961	rBV	166048	295706	20.24%	2.440%
44	7.655	1961	1964	1966	rVV4	643	491	0.03%	0.004%
45	7.690	1968	1975	1989	rVV4	3694	7571	0.52%	0.062%
46	7.896	2025	2039	2069	rBV	531092	925646	63.35%	7.637%
47	8.060	2089	2090	2096	rVB4	678	484	0.03%	0.004%
48	8.176	2115	2126	2145	rBV	116128	199192	13.63%	1.643%
49	8.275	2155	2157	2163	rVB3	549	403	0.03%	0.003%
50	8.343	2176	2178	2183	rVB3	429	330	0.02%	0.003%
51	8.365	2183	2185	2187	rBV	427	224	0.02%	0.002%
52	8.433	2203	2206	2207	rBV2	405	236	0.02%	0.002%
53	8.462	2210	2215	2216	rBV3	654	539	0.04%	0.004%
54	8.552	2235	2243	2251	rVB7	2703	4346	0.30%	0.036%
55	8.632	2255	2268	2293	rBV2	536921	1005671	68.83%	8.297%
56	8.777	2311	2313	2316	rBV4	715	274	0.02%	0.002%
57	8.976	2373	2375	2380	rVB2	390	289	0.02%	0.002%
58	9.005	2381	2384	2386	rBV2	438	283	0.02%	0.002%
59	9.414	2498	2511	2536	rBV	837752	1372740	93.95%	11.325%
60	9.697	2596	2599	2601	rVV2	491	278	0.02%	0.002%
61	9.906	2655	2664	2667	rBV2	395	513	0.04%	0.004%
62	10.102	2722	2725	2730	rBV3	403	379	0.03%	0.003%
63	10.369	2805	2808	2812	rBV	430	289	0.02%	0.002%
64	10.484	2838	2844	2851	rBV2	568	781	0.05%	0.006%
65	10.603	2878	2881	2886	rBV2	345	371	0.03%	0.003%
66	10.754	2914	2928	2953	rBV	641236	1045804	71.58%	8.628%
67	10.893	2967	2971	2978	rVB3	783	691	0.05%	0.006%
68	11.069	3020	3026	3029	rBV3	410	440	0.03%	0.004%
69	11.127	3040	3044	3046	rBV	266	241	0.02%	0.002%
70	11.230	3074	3076	3081	rVB	407	280	0.02%	0.002%
71	11.407	3128	3131	3133	rBV2	549	340	0.02%	0.003%
72	11.462	3143	3148	3152	rBV3	333	422	0.03%	0.003%
73	11.597	3187	3190	3195	rVB	445	314	0.02%	0.003%
74	11.751	3234	3238	3244	rVB4	946	888	0.06%	0.007%
75	11.809	3244	3256	3291	rBV	628680	1018007	69.68%	8.399%
76	11.967	3302	3305	3307	rBV	402	291	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111522\
 Data File : VU051864.D
 Acq On : 15 Nov 2022 17:11
 Operator : JC/MD
 Sample : VU1115WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK012

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

77	12.073	3335	3338	3340	rVB	423	237	0.02%	0.002%
78	12.192	3360	3375	3399	rBV	610195	1011901	69.26%	8.348%
79	12.452	3451	3456	3459	rBV2	413	347	0.02%	0.003%
80	12.561	3487	3490	3495	rVB2	402	317	0.02%	0.003%
81	12.767	3551	3554	3557	rBV2	412	262	0.02%	0.002%
82	12.790	3557	3561	3564	rVB3	450	375	0.03%	0.003%
83	12.809	3564	3567	3571	rBV2	305	277	0.02%	0.002%
84	12.889	3589	3592	3595	rBV2	367	278	0.02%	0.002%
85	12.950	3607	3611	3614	rVV2	316	278	0.02%	0.002%
86	13.034	3633	3637	3641	rBV2	469	519	0.04%	0.004%
87	13.233	3691	3699	3703	rVB5	1228	1649	0.11%	0.014%
88	13.352	3733	3736	3738	rBV2	315	260	0.02%	0.002%
89	13.397	3745	3750	3753	rBV3	571	522	0.04%	0.004%
90	13.449	3759	3766	3769	rBV3	573	709	0.05%	0.006%
91	13.513	3784	3786	3791	rVB3	473	319	0.02%	0.003%
92	13.584	3806	3808	3811	rBV2	480	383	0.03%	0.003%
93	13.745	3856	3858	3861	rBV2	559	368	0.03%	0.003%
94	14.098	3960	3968	3978	rBV4	1271	2663	0.18%	0.022%
95	14.330	4035	4040	4042	rBV4	960	960	0.07%	0.008%
96	15.108	4279	4282	4285	rBV3	773	645	0.04%	0.005%
97	15.227	4317	4319	4322	rVB3	669	307	0.02%	0.003%
98	15.542	4415	4417	4420	rBV2	482	386	0.03%	0.003%
99	15.616	4437	4440	4443	rBV2	605	404	0.03%	0.003%
100	15.822	4502	4504	4511	rBV5	784	892	0.06%	0.007%




Sum of corrected areas: 12121125

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111522\
Data File : VU051864.D
Acq On : 15 Nov 2022 17:11
Operator : JC/MD
Sample : VU1115WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK012

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

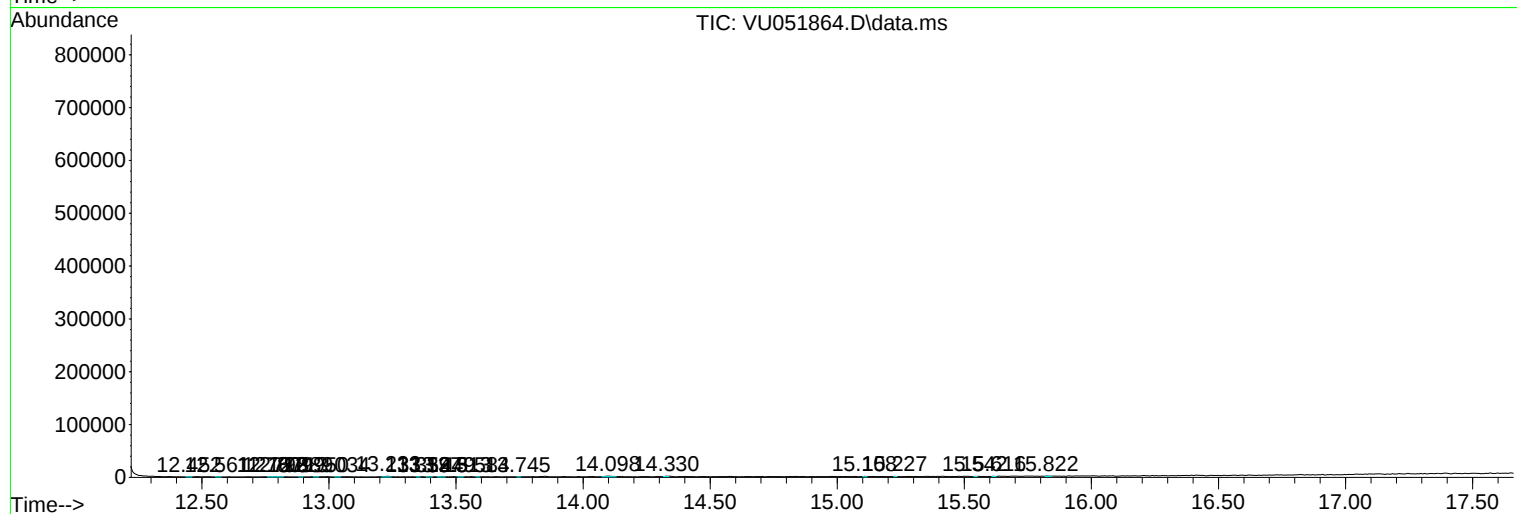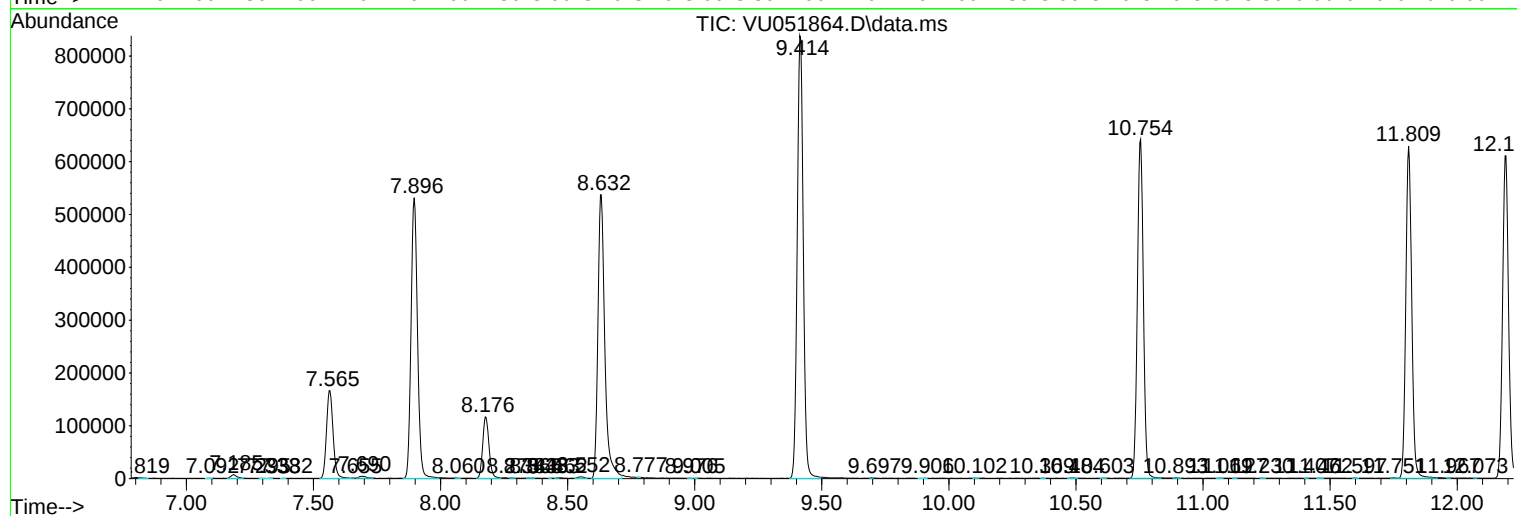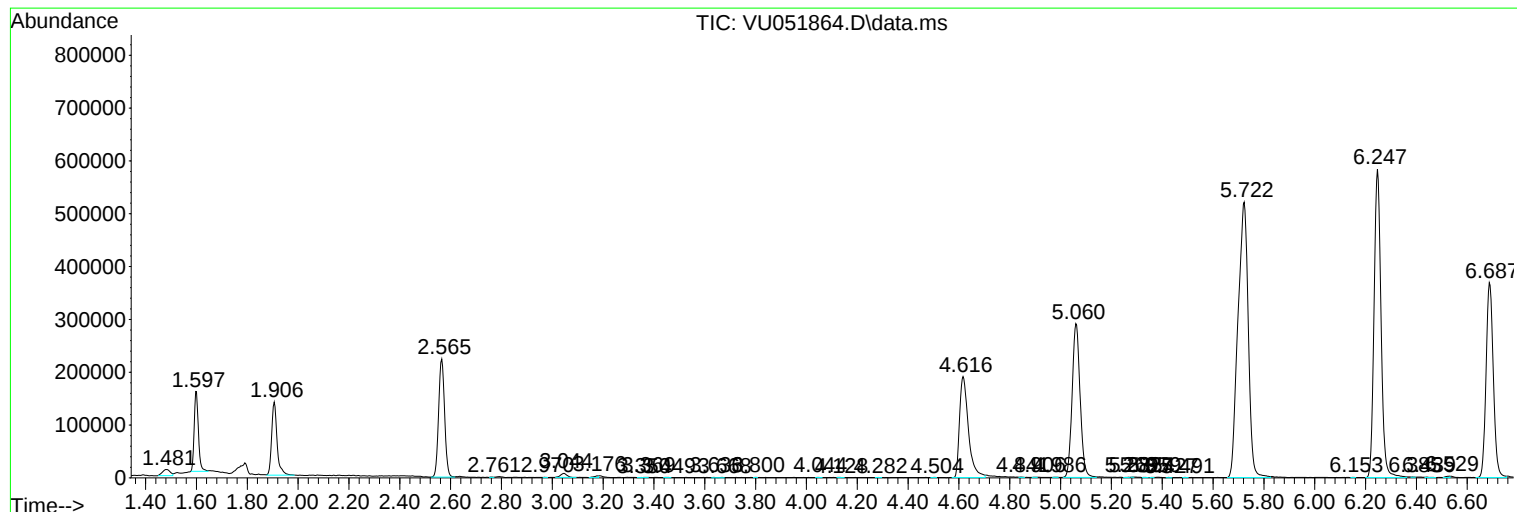

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111522\
Data File : VU051864.D
Acq On : 15 Nov 2022 17:11
Operator : JC/MD
Sample : VU1115WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK012

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111522\
Data File : VU051864.D
Acq On : 15 Nov 2022 17:11
Operator : JC/MD
Sample : VU1115WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK012

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc