

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111523\
 Data File : VU056359.D
 Acq On : 15 Nov 2023 16:50
 Operator : MD/SY
 Sample : 05340-18DL 5X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDM3DL

Quant Time: Nov 16 04:40:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 16 04:37:29 2023
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Mahesh
 Dadoda

11/17/2023
 Supervised By :Semsettin
 Yesilyurt

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	294949	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	294221	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	136709	5.000	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.597	65	115520	5.236	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.800%
7) Chloroethane-d5	1.903	69	75847	4.484	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.600%
11) 1,1-Dichloroethene-d2	2.558	65	51070	5.245	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	105.000%
20) 2-Butanone-d5	4.619	46	238892	54.306	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.620%
24) Chloroform-d	5.054	84	214633	5.030	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.600%
26) 1,2-Dichloroethane-d4	5.697	65	109507	5.554	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.000%
32) Benzene-d6	5.719	84	435259	4.965	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.400%
36) 1,2-Dichloropropane-d6	6.684	67	136809	5.178	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.600%
41) Toluene-d8	7.893	98	380200	4.912	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.200%
43) trans-1,3-Dichloroprop...	8.176	79	50263	4.961	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.200%
46) 2-Hexanone-d5	8.639	63	208540	52.372	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.740%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	101217	5.362	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.200%
66) 1,2-Dichlorobenzene-d4	12.188	152	140483	5.563	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.200%

Target Compounds					Qvalue
12) 1,1-Dichloroethene	2.568	96	3914	0.217 ug/L #	1
16) Methylene chloride	3.038	84	12813	0.536 ug/L	96
17) Methyl tert-butyl Ether	3.356	73	8526	0.194 ug/L	98
19) 1,1-Dichloroethane	3.870	63	6246m	0.170 ug/L	
22) cis-1,2-Dichloroethene	4.665	96	4766	0.226 ug/L	85
27) 1,2-Dichloroethane	5.796	62	4429	0.196 ug/L #	94
29) 1,1,1-Trichloroethane	5.314	97	5242	0.155 ug/L	99
33) Benzene	5.764	78	10452	0.125 ug/L	100
34) Trichloroethene	6.536	95	220943	9.659 ug/L	98
37) 1,2-Dichloropropane	6.787	63	3430	0.157 ug/L	98
38) Bromodichloromethane	7.105	83	4458	0.158 ug/L	93
39) cis-1,3-Dichloropropene	7.606	75	4832	0.150 ug/L	86
44) trans-1,3-Dichloropropene	8.211	75	4205	0.164 ug/L	100
47) Tetrachloroethene	8.549	164	39207	2.542 ug/L	98
49) Dibromochloromethane	8.806	129	2341	0.141 ug/L	99
50) 1,2-Dibromoethane	8.922	107	2269	0.165 ug/L #	93
51) Chlorobenzene	9.449	112	9770	0.175 ug/L #	81
52) Ethylbenzene	9.568	91	15532	0.161 ug/L	94
53) m,p-Xylene	9.693	106	8422	0.237 ug/L	86

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111523\
 Data File : VU056359.D
 Acq On : 15 Nov 2023 16:50
 Operator : MD/SY
 Sample : 05340-18DL 5X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDM3DL

Quant Time: Nov 16 04:40:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 16 04:37:29 2023
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Reviewed By :Mahesh
 Dadoda

11/17/2023
 Supervised By :Semsettin
 Yesilyurt

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
54) o-Xylene	10.098	106	6100	0.177	ug/L	98
59) Bromoform	10.291	173	1644	0.193	ug/L #	95
60) Isopropylbenzene	10.484	105	13098	0.149	ug/L	96
61) 1,2,3-Trichloropropane	10.822	75	2332	0.199	ug/L #	86
62) 1,3,5-Trimethylbenzene	11.085	105	10284	0.142	ug/L	98
63) 1,2,4-Trimethylbenzene	11.468	105	10850	0.152	ug/L	95
64) 1,3-Dichlorobenzene	11.745	146	7300	0.182	ug/L	95
65) 1,4-Dichlorobenzene	11.835	146	6989	0.174	ug/L	97
67) 1,2-Dichlorobenzene	12.211	146	6931	0.188	ug/L	89

11/17/2023

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111523\
Data File : VU056359.D
Acq On : 15 Nov 2023 16:50
Operator : MD/SY
Sample : 05340-18DL 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCDM3DL


Quant Time: Nov 16 04:40:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 16 04:37:29 2023
Response via : Initial Calibration


Manual Integrations
APPROVED

Reviewed By :Mahesh
Dadoda

11/17/2023
Supervised By :Semsettin
Yesilyurt

11/17/2023

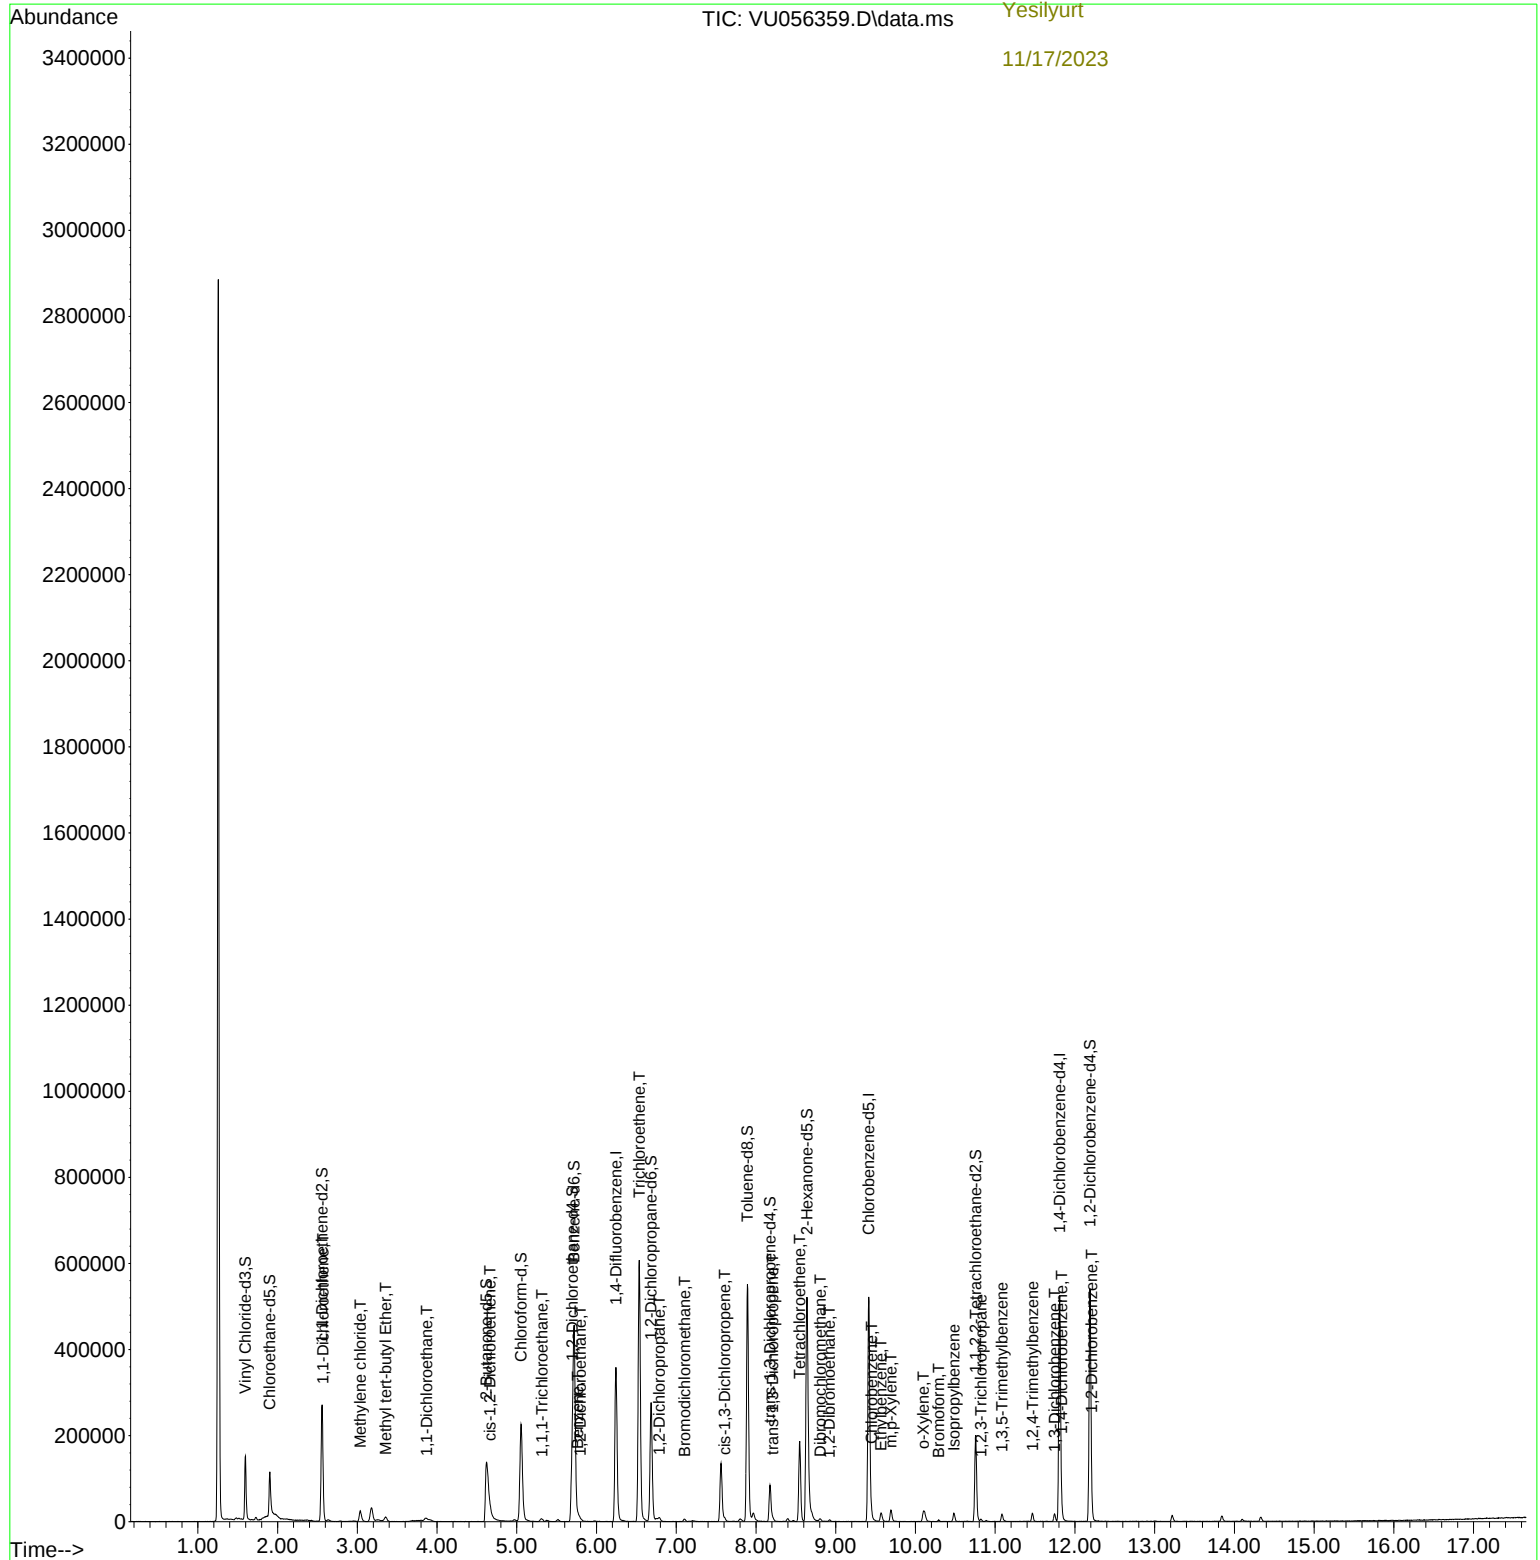

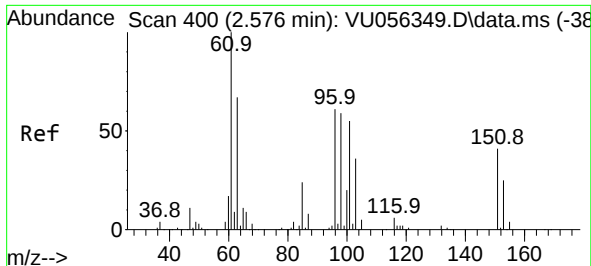

#12

1,1-Dichloroethene

Concen: 0.217 ug/L

RT: 2.568 min Scan# 70

Delta R.T. -0.008 min

Lab File: VU056359.D

Acq: 15 Nov 2023 16:50

Instrument :

MSVOA_U

ClientSampleId :

GCDM3DL

Tgt Ion: 96 Resp: 3914

Ion Ratio Lower Upper

96 100

61 393.6 123.1 228.7

63 2732.4 93.3 173.1

Manual Integrations

APPROVED

Reviewed By :Mahesh





Dadoda

11/17/2023

Supervised By :Semsettin

Yesilyurt

11/17/2023

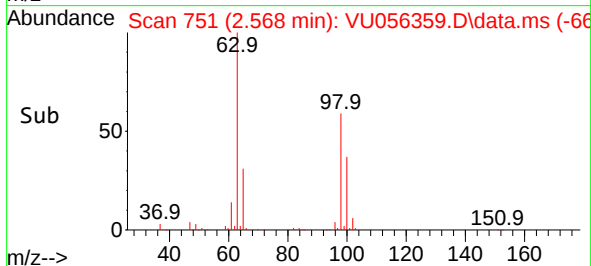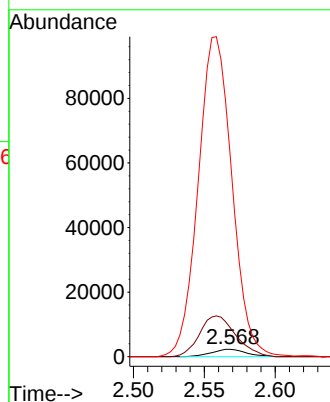

#16

Methylene chloride

Concen: 0.536 ug/L

RT: 3.038 min Scan# 897

Delta R.T. -0.002 min

Lab File: VU056359.D

Acq: 15 Nov 2023 16:50




Tgt Ion: 84 Resp: 12813


Ion Ratio Lower Upper

84 100

86 68.7 44.7 83.1

49 114.1 81.8 152.0

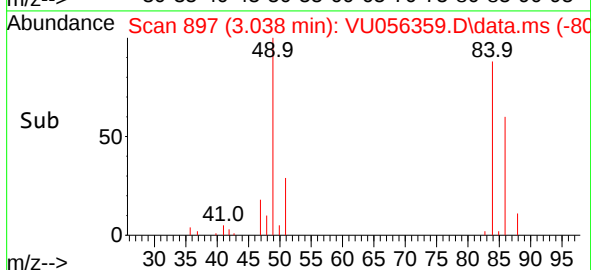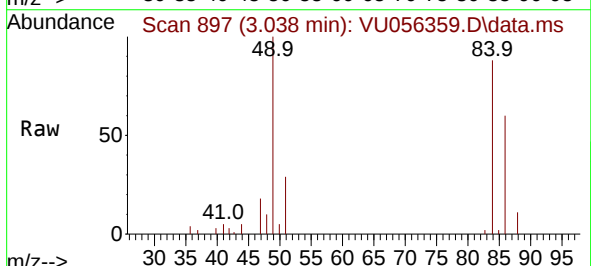

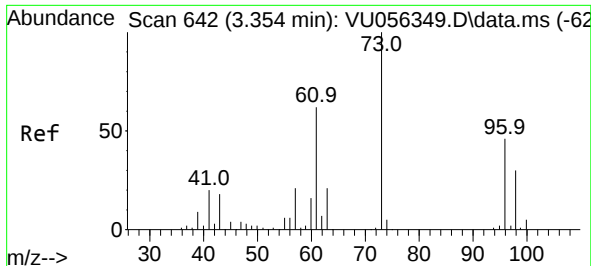

#17

Methyl tert-butyl Ether

Concen: 0.194 ug/L

RT: 3.356 min Scan# 91

Delta R.T. 0.002 min

Lab File: VU056359.D

Acq: 15 Nov 2023 16:50

Instrument :

MSVOA_U

ClientSampleId :

GCDM3DL

Tgt Ion: 73	Resp: 8520
Ion Ratio	Lower Upper
73 100	
43 18.5	15.1 22.7
57 20.9	17.8 26.8





Manual Integrations
APPROVED

Reviewed By :Mahesh
Dadoda

11/17/2023

Supervised By :Semsettin
Yesilyurt

11/17/2023

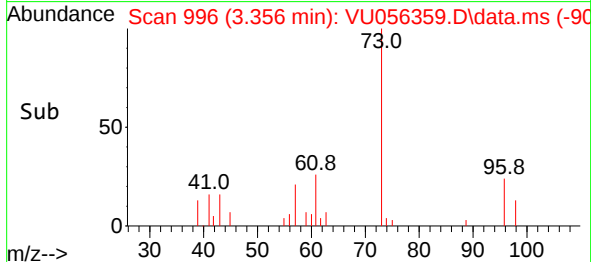

#19

1,1-Dichloroethane

Concen: 0.170 ug/L m




RT: 3.870 min Scan# 1156


Delta R.T. 0.008 min

Lab File: VU056359.D

Acq: 15 Nov 2023 16:50

Tgt Ion: 63	Resp: 6246
Ion Ratio	Lower Upper
63 100	
65 0.0	21.8 40.6
83 13.6	9.7 17.9

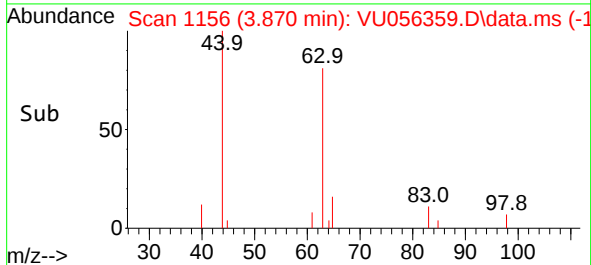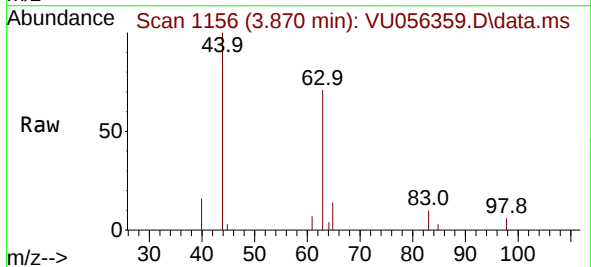

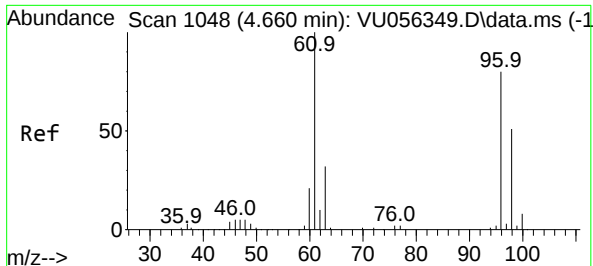

#22

cis-1,2-Dichloroethene

Concen: 0.226 ug/L

RT: 4.665 min Scan# 1403

Delta R.T. 0.005 min

Lab File: VU056359.D

Acq: 15 Nov 2023 16:50

Instrument :

MSVOA_U

ClientSampleId :

GCDM3DL

Tgt Ion:	96	Resp:	4760
Ion	Ratio	Lower	Upper
96	100		
61	111.9	93.2	173.2
98	71.9	44.8	83.2

Manual Integrations





APPROVED

Reviewed By :Mahesh
Dadoda

11/17/2023

Supervised By :Semsettin
Yesilyurt

11/17/2023

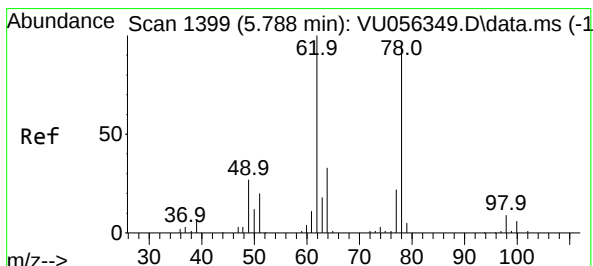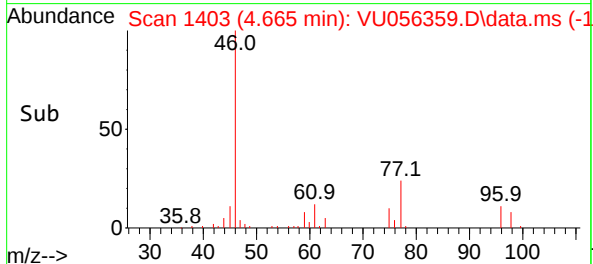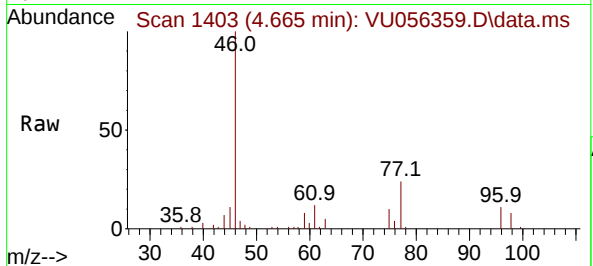

#27

1,2-Dichloroethane

Concen: 0.196 ug/L




RT: 5.796 min Scan# 1755


Delta R.T. 0.008 min

Lab File: VU056359.D

Acq: 15 Nov 2023 16:50

Tgt Ion:	62	Resp:	4429
Ion	Ratio	Lower	Upper
62	100		
98	10.4	6.6	10.0#

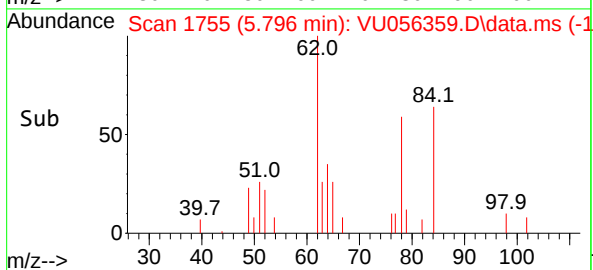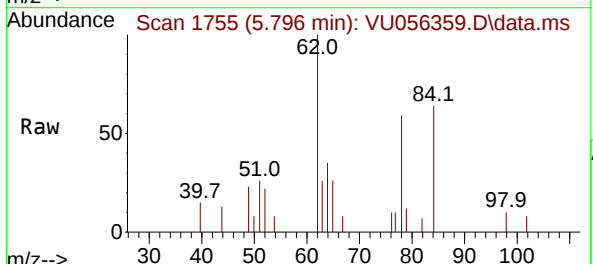

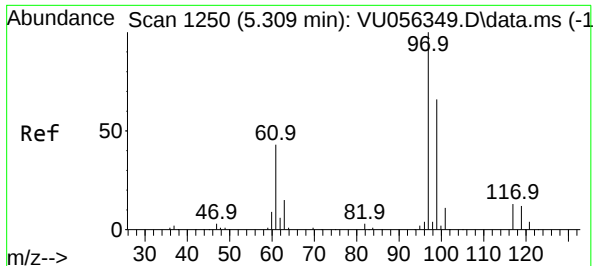

#29
1,1,1-Trichloroethane
Concen: 0.155 ug/L
RT: 5.314 min Scan# 1745
Delta R.T. 0.005 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50

Instrument :
MSVOA_U
ClientSampleId :
GCDM3DL





Tgt Ion: 97 Resp: 524
Ion Ratio Lower Upper
97 100
99 64.0 51.6 77.4
61 41.8 34.3 51.5

Manual Integrations
APPROVED

Reviewed By :Mahesh
Dadoda




11/17/2023
Supervised By :Semsettin
Yesilyurt


11/17/2023

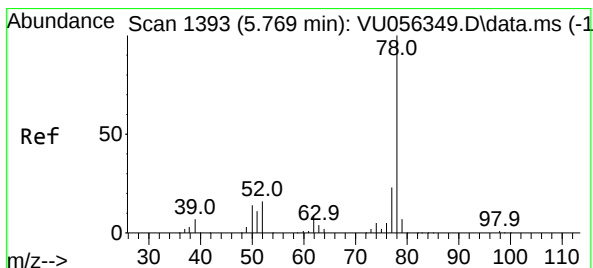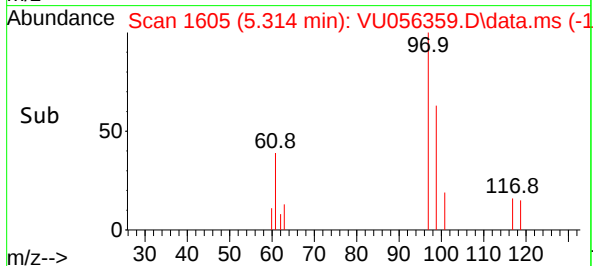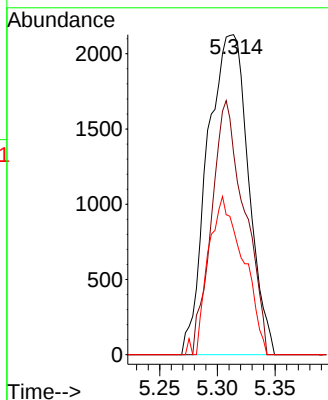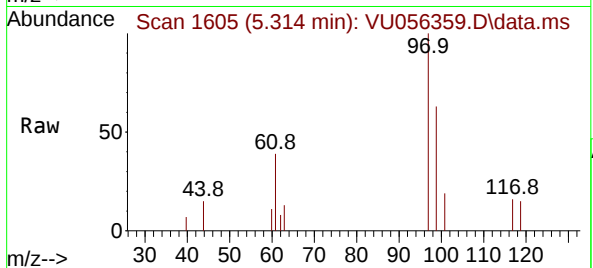

#33
Benzene
Concen: 0.125 ug/L
RT: 5.764 min Scan# 1745
Delta R.T. -0.005 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50


Tgt Ion: 78 Resp: 10452

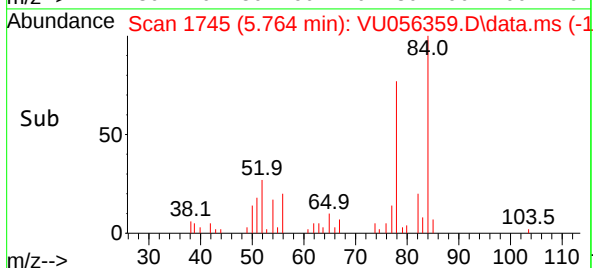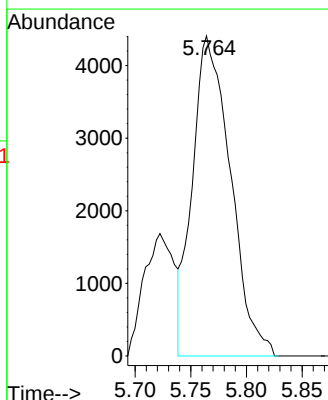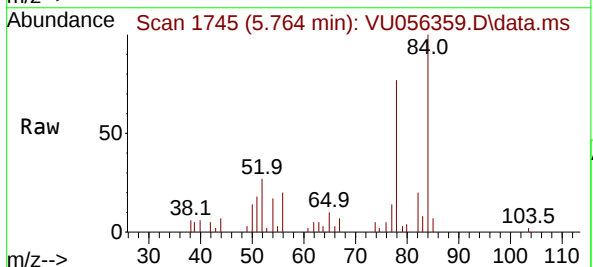

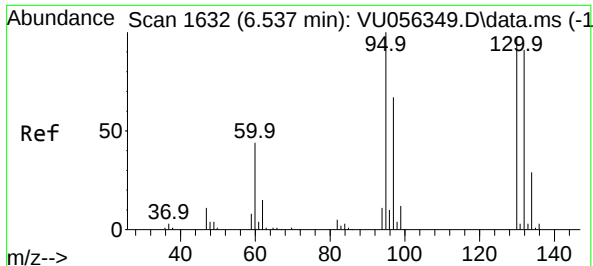

#34
Trichloroethene
Concen: 9.659 ug/L
RT: 6.536 min Scan# 1985
Delta R.T. -0.002 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50

Instrument :
MSVOA_U
ClientSampleId :
GCDM3DL

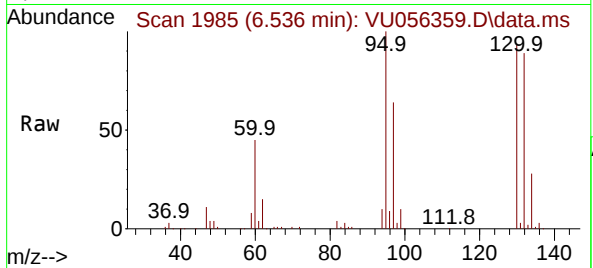



Tgt Ion: 95 Resp: 22094
Ion Ratio Lower Upper
95 100
97 63.7 46.5 86.3
132 89.5 62.0 115.2
130 93.0 66.3 123.1

Manual Integrations
APPROVED

Reviewed By :Mahesh
Dadoda




11/17/2023
Supervised By :Semsettin
Yesilyurt


11/17/2023

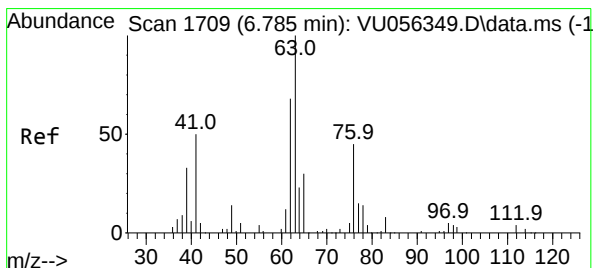

#37
1,2-Dichloropropane
Concen: 0.157 ug/L
RT: 6.787 min Scan# 2063
Delta R.T. 0.002 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50

Tgt Ion: 63 Resp: 3430
Ion Ratio Lower Upper
63 100
112 3.3 3.2 4.8

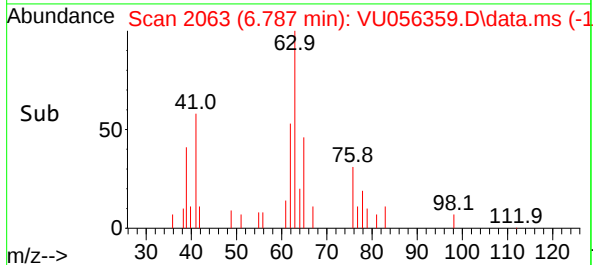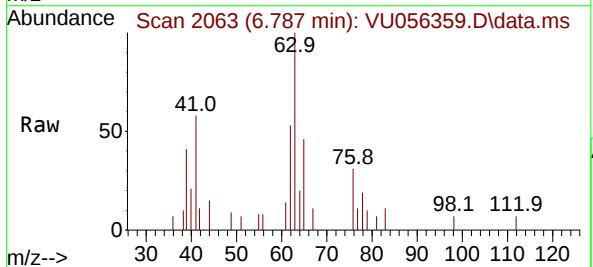

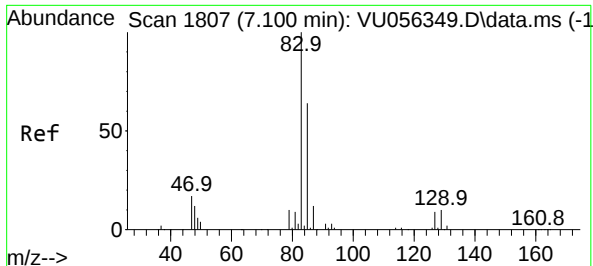

#38
Bromodichloromethane
Concen: 0.158 ug/L
RT: 7.105 min Scan# 2162
Delta R.T. 0.005 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50

Instrument :
MSVOA_U
ClientSampleId :
GCDM3DL





Tgt Ion: 83 Resp: 4458
Ion Ratio Lower Upper
83 100
85 70.1 44.9 83.5
127 8.1 6.9 10.3

Manual Integrations
APPROVED

Reviewed By :Mahesh
Dadoda




11/17/2023
Supervised By :Semsettin
Yesilyurt


11/17/2023

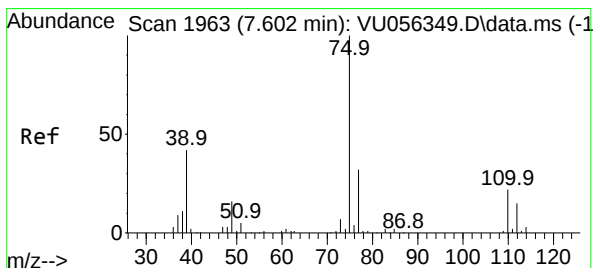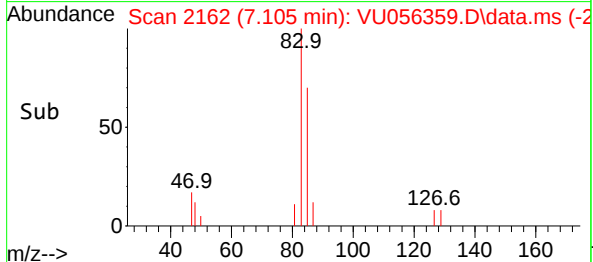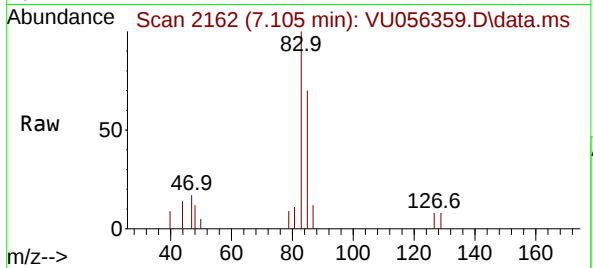

#39
cis-1,3-Dichloropropene
Concen: 0.150 ug/L
RT: 7.606 min Scan# 2318
Delta R.T. 0.005 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50

Tgt Ion: 75 Resp: 4832
Ion Ratio Lower Upper
75 100
77 38.5 21.5 39.9

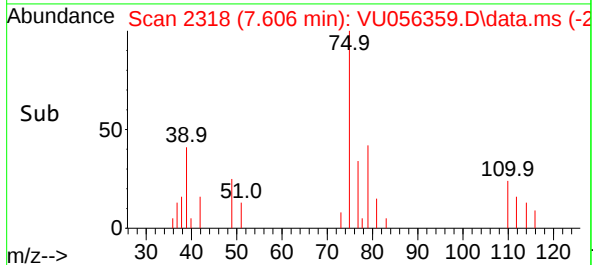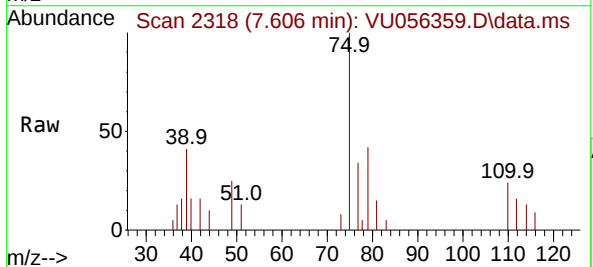



#44
trans-1,3-Dichloropropene
Concen: 0.164 ug/L
RT: 8.211 min Scan# 2151
Delta R.T. 0.005 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50

Instrument :
MSVOA_U
ClientSampleId :
GCDM3DL





Tgt Ion: 75 Resp: 420
Ion Ratio Lower Upper
75 100
77 32.7 22.8 42.4

Manual Integrations
APPROVED

Reviewed By :Mahesh
Dadoda




11/17/2023
Supervised By :Semsettin
Yesilyurt


11/17/2023

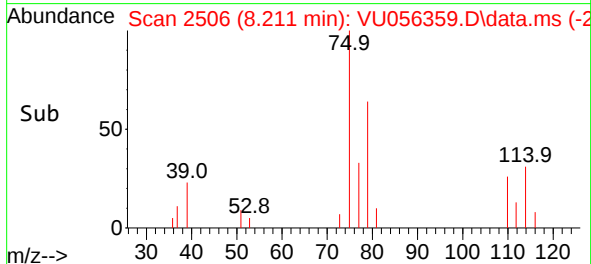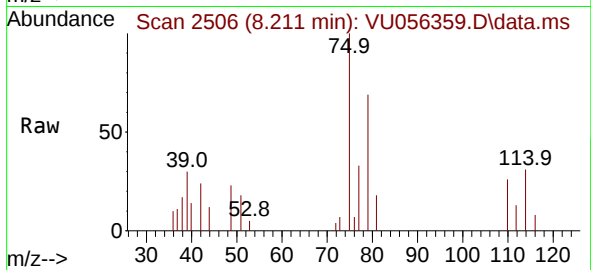

#47
Tetrachloroethene
Concen: 2.542 ug/L
RT: 8.549 min Scan# 2611
Delta R.T. -0.002 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50

Tgt Ion:164 Resp: 39207
Ion Ratio Lower Upper
164 100
129 102.7 71.0 131.9
131 104.5 70.3 130.7
166 131.0 89.8 166.8

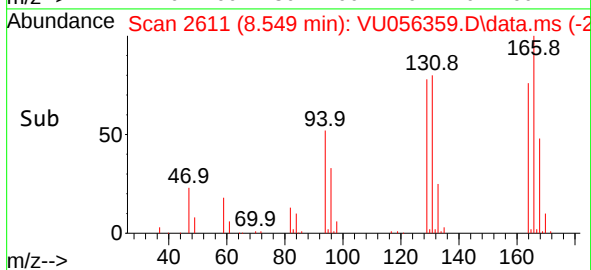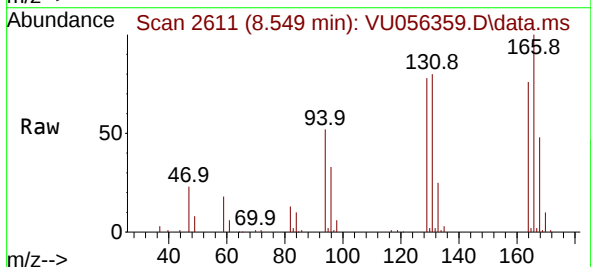

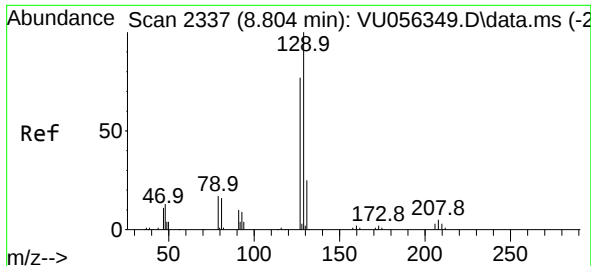

#49

Dibromochloromethane

Concen: 0.141 ug/L

RT: 8.806 min Scan# 2

Delta R.T. 0.002 min

Lab File: VU056359.D

Acq: 15 Nov 2023 16:50

Instrument :

MSVOA_U

ClientSampleId :

GCDM3DL

Tgt Ion:129 Resp: 234

Ion Ratio Lower Upper

129 100

127 74.6 52.9 98.3

Manual Integrations





APPROVED

Reviewed By :Mahesh
Dadoda

11/17/2023

Supervised By :Semsettin
Yesilyurt

11/17/2023

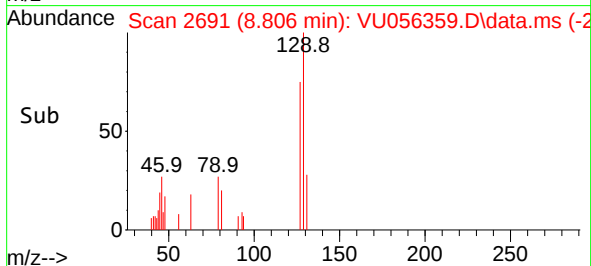

#50

1,2-Dibromoethane

Concen: 0.165 ug/L

RT: 8.922 min Scan# 2727

Delta R.T. 0.002 min

Lab File: VU056359.D

Acq: 15 Nov 2023 16:50




Tgt Ion:107 Resp: 2269


Ion Ratio Lower Upper

107 100

109 97.9 64.2 119.2


188 0.0 2.6 4.0#

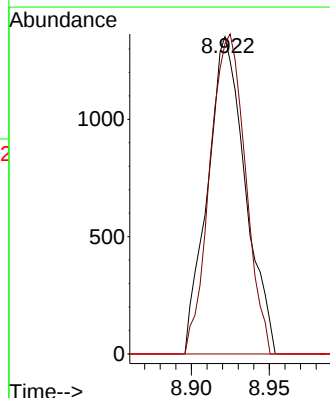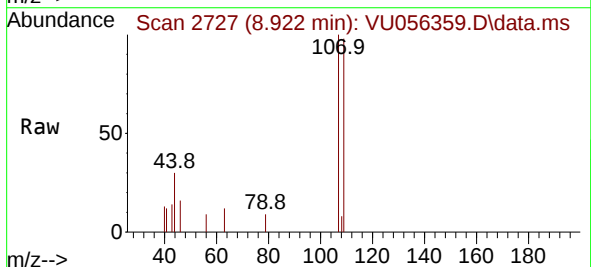

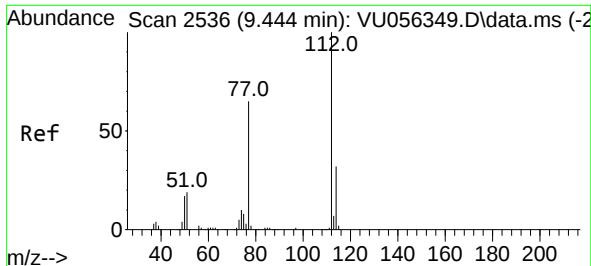

#51
Chlorobenzene
Concen: 0.175 ug/L
RT: 9.449 min Scan# 21
Delta R.T. 0.005 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50

Instrument :
MSVOA_U
ClientSampleId :
GCDM3DL






Tgt Ion: 112 Resp: 9770
Ion Ratio Lower Upper
112 100
114 31.7 22.5 41.7
77 42.5 51.7 77.5

Manual Integrations
APPROVED

Reviewed By :Mahesh
Dadoda




11/17/2023
Supervised By :Semsettin
Yesilyurt


11/17/2023

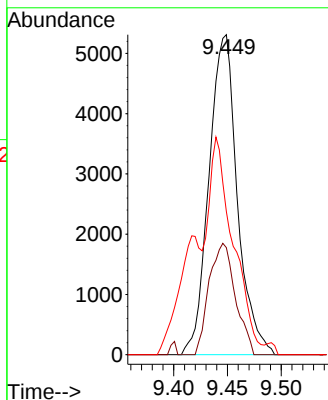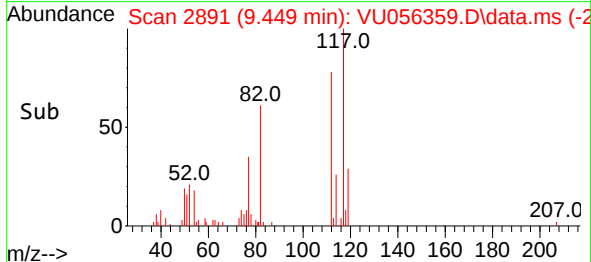

#52
Ethylbenzene
Concen: 0.161 ug/L
RT: 9.568 min Scan# 2928
Delta R.T. 0.002 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50

Tgt Ion: 91 Resp: 15532
Ion Ratio Lower Upper
91 100
106 26.8 21.1 39.1

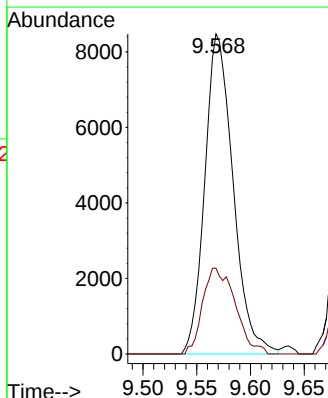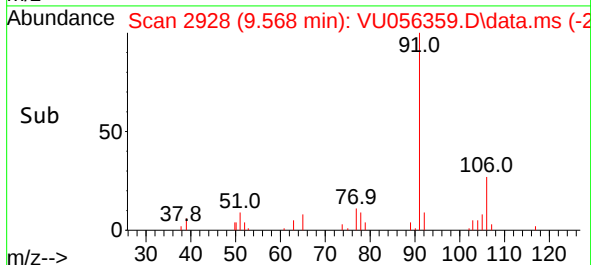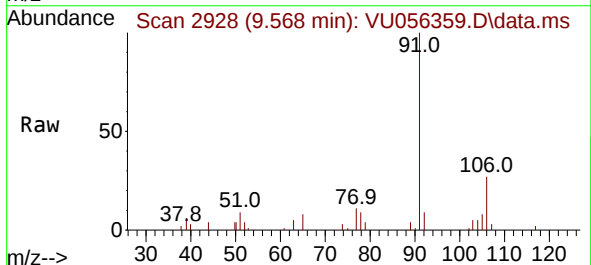



#53
m,p-Xylene
Concen: 0.237 ug/L
RT: 9.693 min Scan# 2967
Delta R.T. 0.002 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50

Instrument :
MSVOA_U
ClientSampleId :
GCDM3DL





Tgt Ion:106 Resp: 842
Ion Ratio Lower Upper
106 100
91 190.9 149.6 277.8

Manual Integrations
APPROVED

Reviewed By :Mahesh
Dadoda




11/17/2023
Supervised By :Semsettin
Yesilyurt


11/17/2023

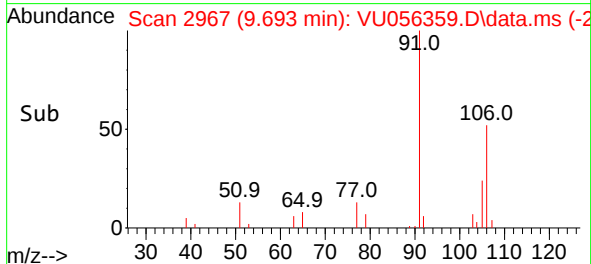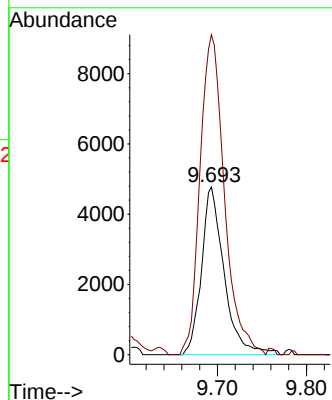

#54
o-Xylene
Concen: 0.177 ug/L
RT: 10.098 min Scan# 3093
Delta R.T. 0.002 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50


Tgt Ion:106 Resp: 6100
Ion Ratio Lower Upper
106 100
91 231.0 159.3 295.9

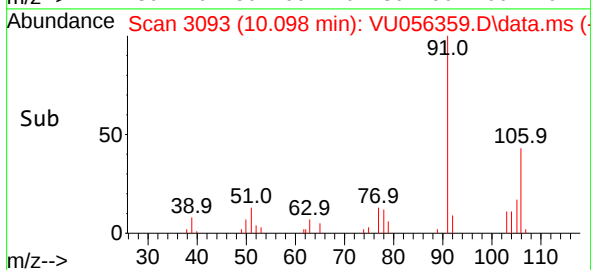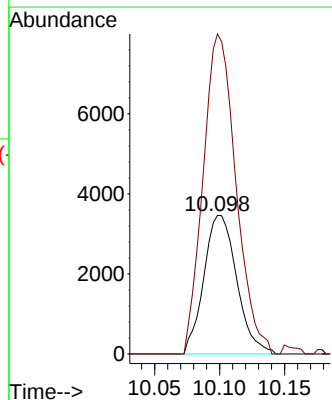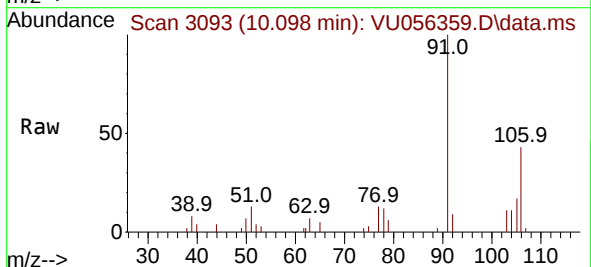

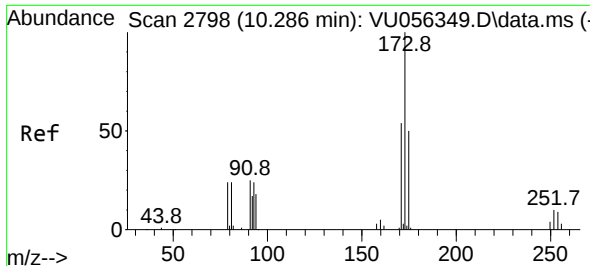

#59
Bromoform
Concen: 0.193 ug/L
RT: 10.291 min Scan# 3153
Delta R.T. 0.005 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50

Instrument :
MSVOA_U
ClientSampleId :
GCDM3DL

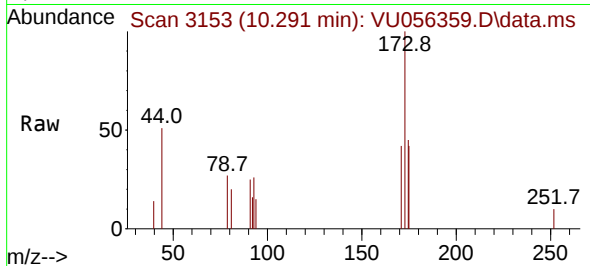




Tgt Ion:173 Resp: 1644
Ion Ratio Lower Upper
173 100
175 49.6 38.9 58.3
254 0.0 6.7 10.1

Manual Integrations
APPROVED

Reviewed By :Mahesh
Dadoda




11/17/2023
Supervised By :Semsettin
Yesilyurt


11/17/2023

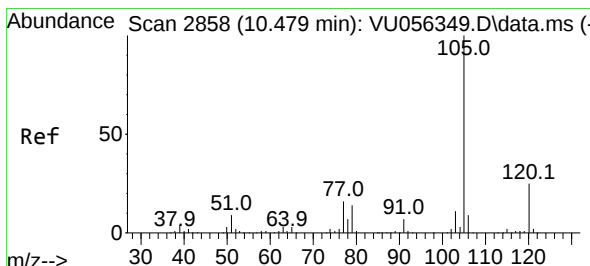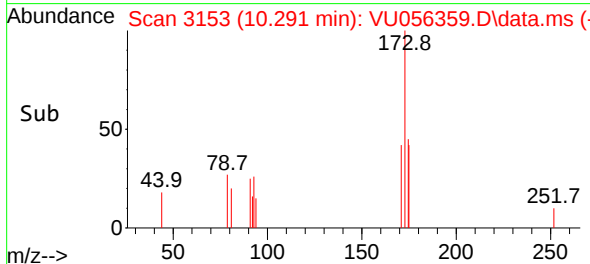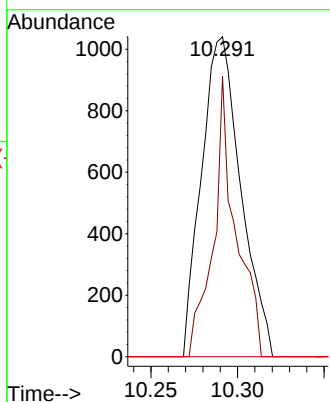

#60
Isopropylbenzene
Concen: 0.149 ug/L
RT: 10.484 min Scan# 3213
Delta R.T. 0.005 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50


Tgt Ion:105 Resp: 13098
Ion Ratio Lower Upper
105 100
120 22.9 20.4 30.6
77 17.4 13.3 19.9

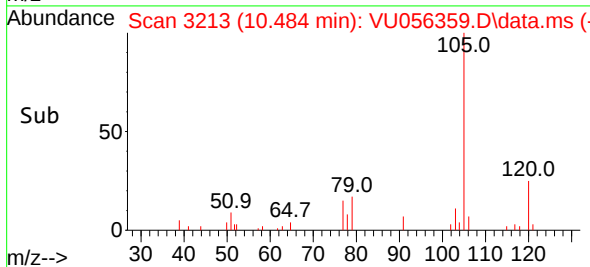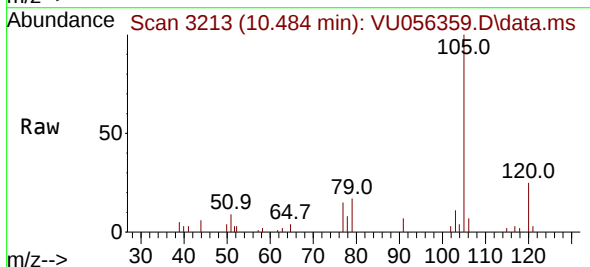

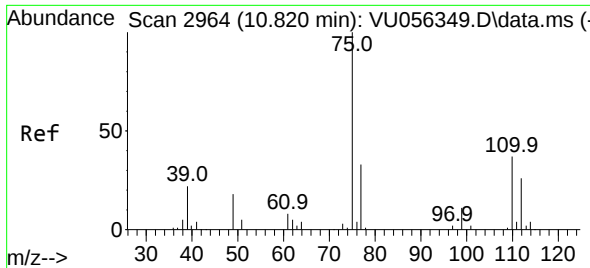

#61
1,2,3-Trichloropropane
Concen: 0.199 ug/L
RT: 10.822 min Scan# 3110
Delta R.T. 0.002 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50

Instrument :
MSVOA_U
ClientSampleId :
GCDM3DL

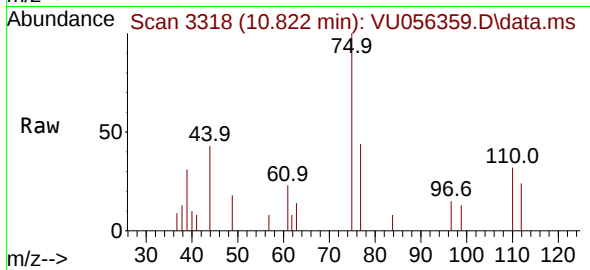




Tgt Ion: 75 Resp: 233
Ion Ratio Lower Upper
75 100
110 31.6 30.4 45.6
77 43.4 27.0 40.6

Manual Integrations
APPROVED

Reviewed By :Mahesh
Dadoda




11/17/2023
Supervised By :Semsettin
Yesilyurt


11/17/2023

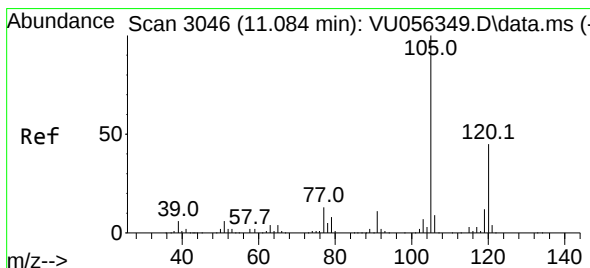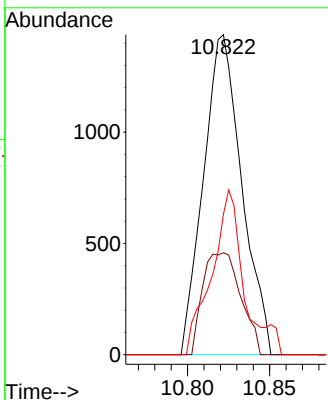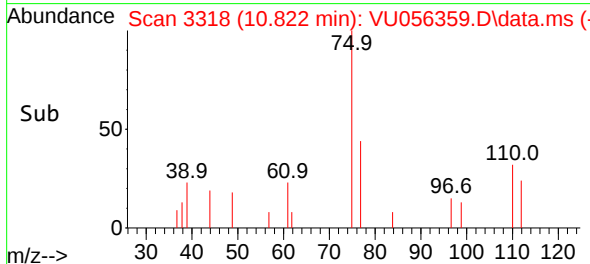

#62
1,3,5-Trimethylbenzene
Concen: 0.142 ug/L
RT: 11.085 min Scan# 3400
Delta R.T. 0.002 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50

Tgt Ion:105 Resp: 10284
Ion Ratio Lower Upper
105 100
120 45.0 37.2 55.8

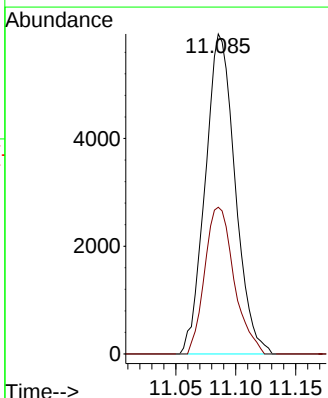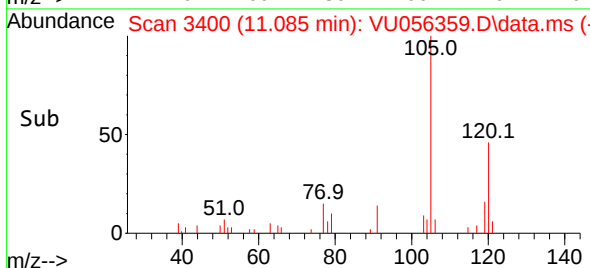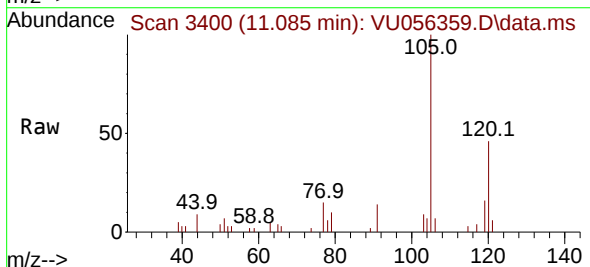

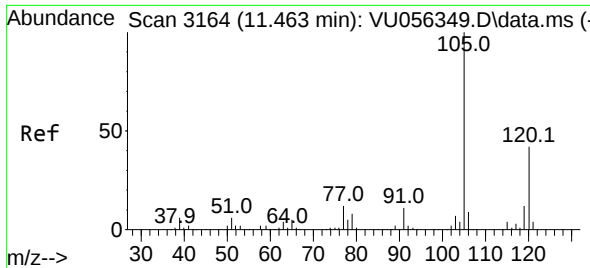

#63
1,2,4-Trimethylbenzene
Concen: 0.152 ug/L
RT: 11.468 min Scan# 3164
Delta R.T. 0.005 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50

Instrument :
MSVOA_U
ClientSampleId :
GCDM3DL





Tgt Ion:105 Resp: 10850
Ion Ratio Lower Upper
105 100
120 45.4 34.0 51.0

Manual Integrations
APPROVED

Reviewed By :Mahesh
Dadoda




11/17/2023
Supervised By :Semsettin
Yesilyurt


11/17/2023

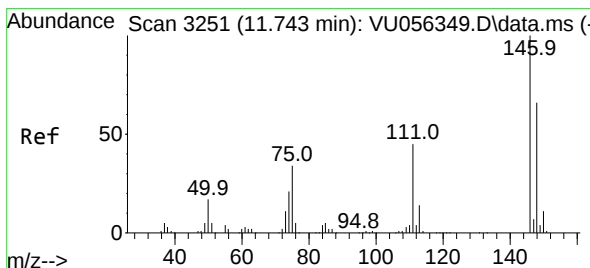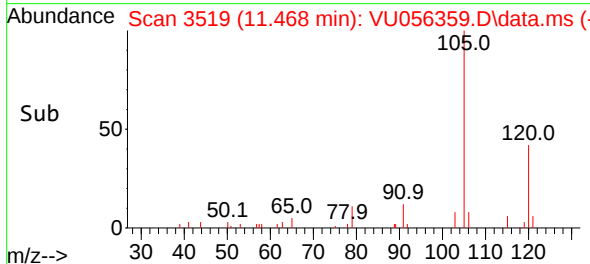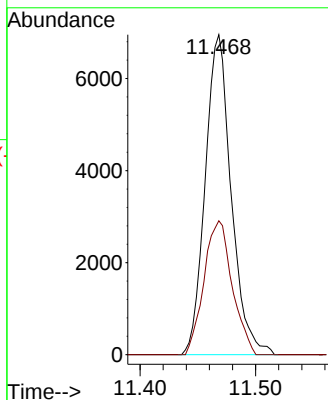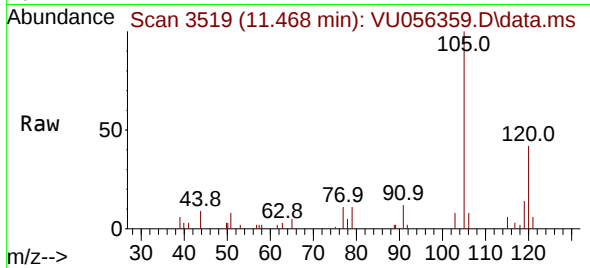

#64
1,3-Dichlorobenzene
Concen: 0.182 ug/L
RT: 11.745 min Scan# 3605
Delta R.T. 0.002 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50

Tgt Ion:146 Resp: 7300
Ion Ratio Lower Upper
146 100
111 44.6 31.1 57.7
148 58.6 45.1 83.9

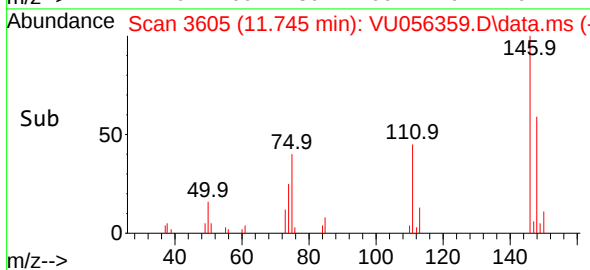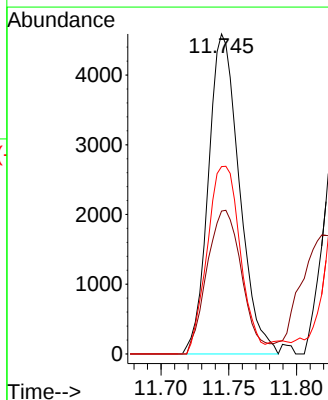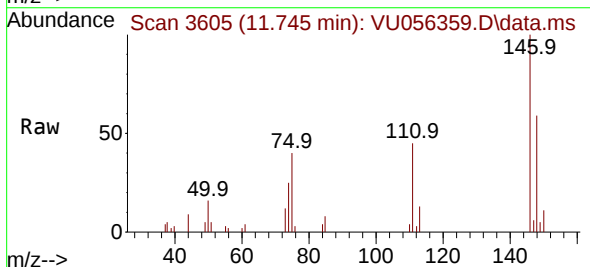



#65
1,4-Dichlorobenzene
Concen: 0.174 ug/L
RT: 11.835 min Scan# 30
Delta R.T. 0.002 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50

Instrument :
MSVOA_U
ClientSampleId :
GCDM3DL





Tgt Ion:146 Resp: 6989
Ion Ratio Lower Upper
146 100
111 40.2 30.5 56.7
148 62.6 44.8 83.2

Manual Integrations
APPROVED

Reviewed By :Mahesh
Dadoda

11/17/2023
Supervised By :Semsettin
Yesilyurt

11/17/2023

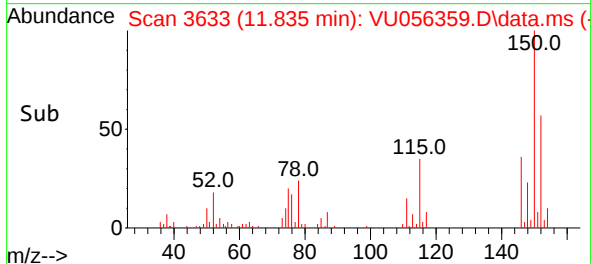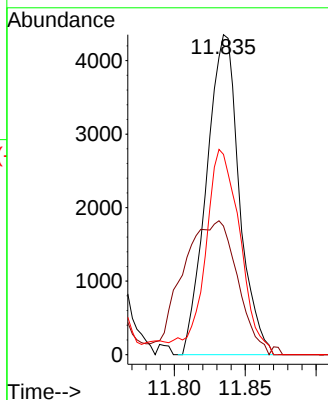

#67
1,2-Dichlorobenzene
Concen: 0.188 ug/L
RT: 12.211 min Scan# 3750
Delta R.T. 0.002 min
Lab File: VU056359.D
Acq: 15 Nov 2023 16:50

Tgt Ion:146 Resp: 6931
Ion Ratio Lower Upper
146 100
111 56.5 38.3 57.5
148 72.8 52.2 78.4

