


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111523\
 Data File : VU056348.D
 Acq On : 15 Nov 2023 11:07
 Operator : MD/SY
 Sample : BFB074
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB074

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Nov 17 04:03:21 2023

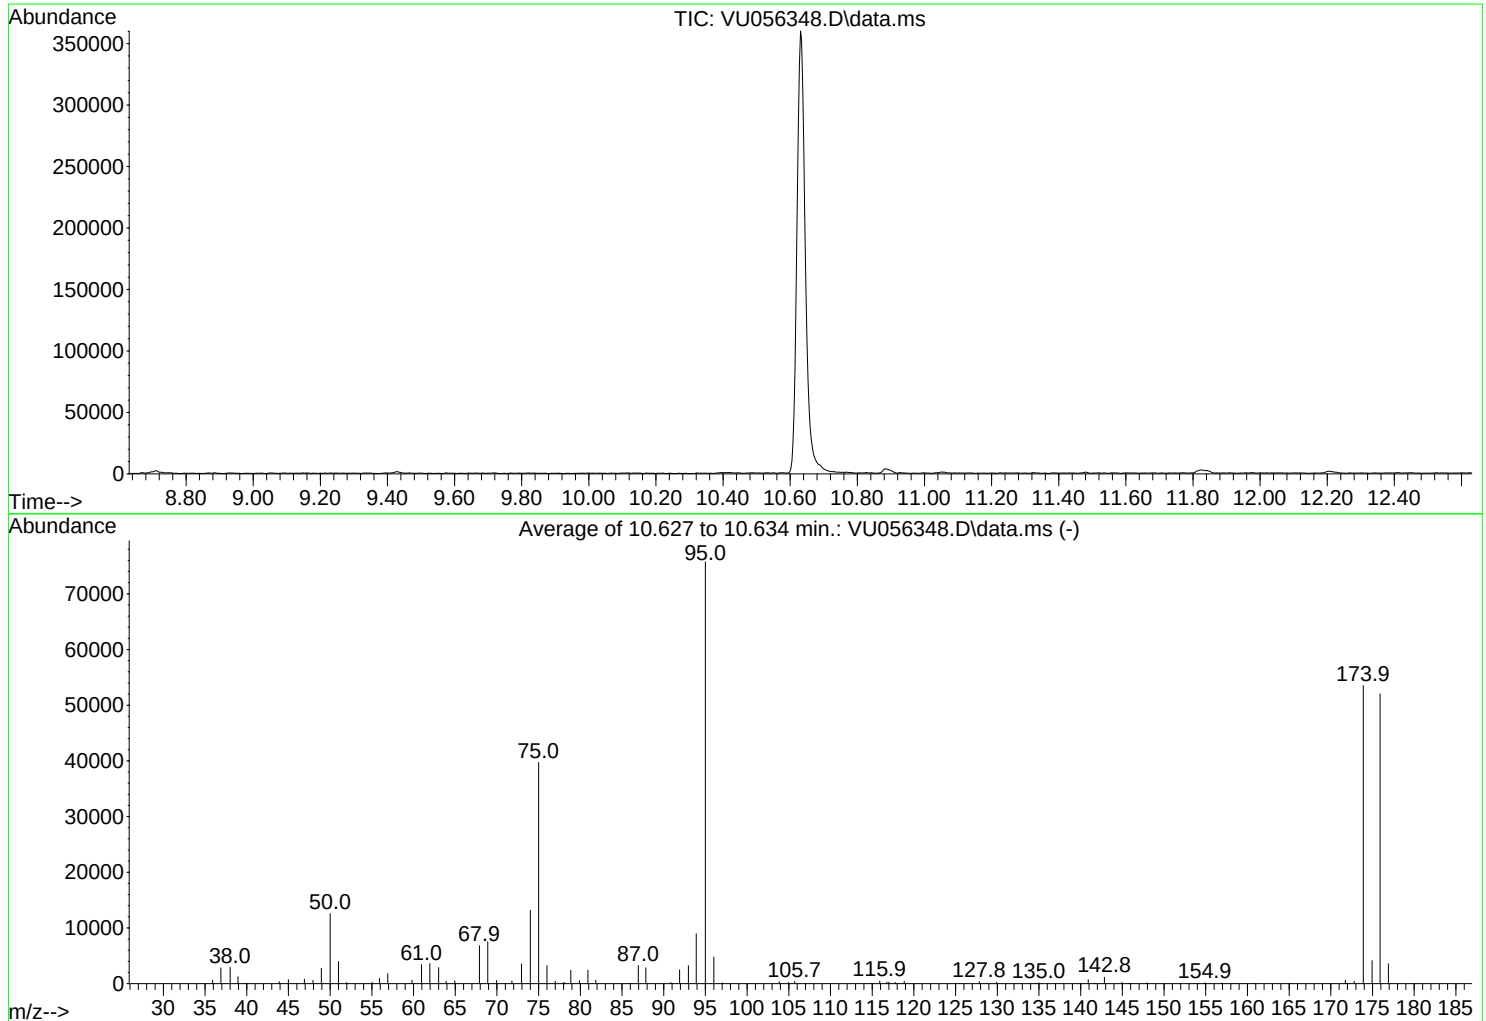

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	12569	PASS
75	95	30	80	52.4	39720	PASS
95	95	100	100	100.0	75741	PASS
96	95	5	9	6.4	4810	PASS
173	174	0.00	2	0.8	440	PASS
174	95	50	120	70.7	53536	PASS
175	174	5	9	7.7	4127	PASS
176	174	95	101	97.2	52043	PASS
177	176	5	9	6.8	3562	PASS

m/z	Abundance
37.60	124.0
39.90	184.0
43.90	414.0

Instrument :
MSVOA_U
ClientSampleId :
BFB074

m/z	Abundance
35.90	553.0
36.90	2732.0
38.00	2861.0
39.00	1213.0
40.00	247.0
44.00	747.0
45.00	653.0
46.80	708.0
47.90	607.0
48.90	2889.0
50.00	11949.0
51.00	3974.0
52.00	147.0
55.00	203.0
55.90	932.0
56.90	1769.0
59.80	560.0
60.90	3499.0
61.90	3602.0
63.00	2933.0
63.80	401.0
64.90	562.0
67.90	6650.0
68.90	7668.0
69.90	482.0
71.80	525.0
73.00	3616.0
74.00	12587.0
75.00	38648.0
76.00	3110.0
77.00	444.0
77.90	283.0
78.90	2423.0
79.90	556.0
80.90	2437.0
81.90	640.0
87.00	2930.0
87.90	2635.0
90.80	206.0
91.90	2367.0
92.90	3139.0
93.90	8675.0
95.00	71832.0
96.00	4730.0
97.10	177.0
103.80	287.0
105.00	272.0
105.70	284.0
115.90	417.0
117.00	456.0
117.80	220.0
118.80	394.0
127.80	378.0
130.00	251.0
134.60	111.0
135.00	107.0
140.90	708.0
142.90	1038.0
144.90	275.0
148.00	179.0
154.90	172.0
156.90	119.0
158.70	122.0
171.70	585.0
172.80	631.0
173.90	49352.0
174.90	3957.0
175.90	49312.0
176.90	3226.0

Instrument :
MSVOA_U
ClientSampleId :
BFB074

m/z	Abundance
35.90	600.0
36.90	2880.0
38.00	2995.0
39.00	1320.0
40.00	277.0
44.00	794.0
45.00	759.0
46.90	802.0
48.00	633.0
48.90	2858.0
50.00	13028.0
51.00	4085.0
52.00	216.0
55.10	208.0
55.90	1015.0
56.90	1838.0
59.80	600.0
61.00	3502.0
61.90	3729.0
63.00	2958.0
63.90	471.0
64.90	553.0
67.90	6980.0
68.90	7702.0
70.00	602.0
71.80	490.0
72.90	3602.0
74.00	13656.0
75.00	40728.0
76.00	3373.0
77.00	493.0
78.10	346.0
78.80	2436.0
79.90	561.0
80.90	2445.0
81.90	619.0
86.90	3380.0
87.80	2918.0
90.90	204.0
91.90	2574.0
93.00	3316.0
93.90	9272.0
95.00	78288.0
96.00	4902.0
97.00	118.0
103.90	351.0
104.90	266.0
105.70	422.0
114.90	106.0
115.90	484.0
116.70	423.0
117.00	436.0
117.80	233.0
118.80	430.0
127.90	390.0
128.70	110.0
129.90	253.0
135.00	127.0
140.90	712.0
141.70	106.0
142.90	1192.0
144.90	211.0
148.00	159.0
154.90	208.0
156.90	121.0
171.70	619.0
172.80	688.0
173.90	55192.0
175.00	4274.0
175.90	53840.0
176.90	3718.0

Instrument :
MSVOA_U
ClientSampleId :
BFB074

m/z	Abundance
35.90	619.0
36.90	2805.0
38.00	2933.0
38.90	1206.0
39.90	312.0
43.90	769.0
45.00	770.0
47.00	885.0
47.90	552.0
49.00	2543.0
50.00	12731.0
51.00	3853.0
52.00	246.0
55.10	187.0
55.90	957.0
56.90	1840.0
59.80	616.0
61.00	3292.0
62.00	3486.0
63.00	2763.0
64.00	457.0
65.00	469.0
67.90	6836.0
68.90	7232.0
70.00	637.0
71.80	438.0
72.90	3416.0
74.00	13220.0
75.00	39784.0
76.00	3284.0
77.00	392.0
78.00	342.0
78.90	2393.0
79.90	496.0
80.90	2321.0
81.80	545.0
85.90	104.0
86.90	3451.0
87.80	2955.0
90.90	215.0
91.90	2456.0
93.00	3244.0
93.90	8946.0
95.00	77104.0
96.00	4799.0
97.00	123.0
103.80	368.0
104.90	190.0
105.70	445.0
114.80	112.0
115.90	464.0
116.80	451.0
117.70	273.0
118.90	483.0
127.90	338.0
128.70	139.0
129.80	262.0
135.00	176.0
140.90	772.0
141.70	137.0
142.80	1208.0
145.00	198.0
145.80	112.0
147.80	127.0
154.90	173.0
156.90	103.0
160.80	115.0
171.80	630.0
173.90	56064.0
175.00	4151.0
175.90	52976.0
176.90	3741.0

Instrument :
MSVOA_U
ClientSampleId :
BFB074