

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU111618\
 Data File : VU028199.D
 Acq On : 16 Nov 2018 21:21
 Operator : MD/SY
 Sample : J5960-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK5

Quant Time: Nov 17 03:27:17 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111418WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 16 23:59:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	152866	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	147777	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	64769	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	45062	3.55	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.00%
7) Chloroethane-d5	1.68	69	42963	4.26	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.20%
11) 1,1-Dichloroethene-d2	2.28	63	66472	2.81	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.20%#
20) 2-Butanone-d5	4.20	46	209174	56.85	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.70%
24) Chloroform-d	4.65	84	92364	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.60%
26) 1,2-Dichloroethane-d4	5.31	65	56864	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.00%
32) Benzene-d6	5.34	84	179743	4.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.80%
36) 1,2-Dichloropropane-d6	6.33	67	69280	4.57	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.40%
41) Toluene-d8	7.57	98	144170	3.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.00%
43) trans-1,3-Dichloropropene-	7.85	79	19015	3.51	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.20%
46) 2-Hexanone-d5	8.31	63	151362	48.96	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.92%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	52467	4.89	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.80%
64) 1,2-Dichlorobenzene-d4	11.86	152	54636	4.51	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.20%


Target Compounds					Qvalue
13) Acetone	2.33	43	5152	2.079 ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU111618\
Data File : VU028199.D
Acq On : 16 Nov 2018 21:21
Operator : MD/SY
Sample : J5960-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK5

Quant Time: Nov 17 03:27:17 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111418WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 16 23:59:22 2018
Response via : Initial Calibration

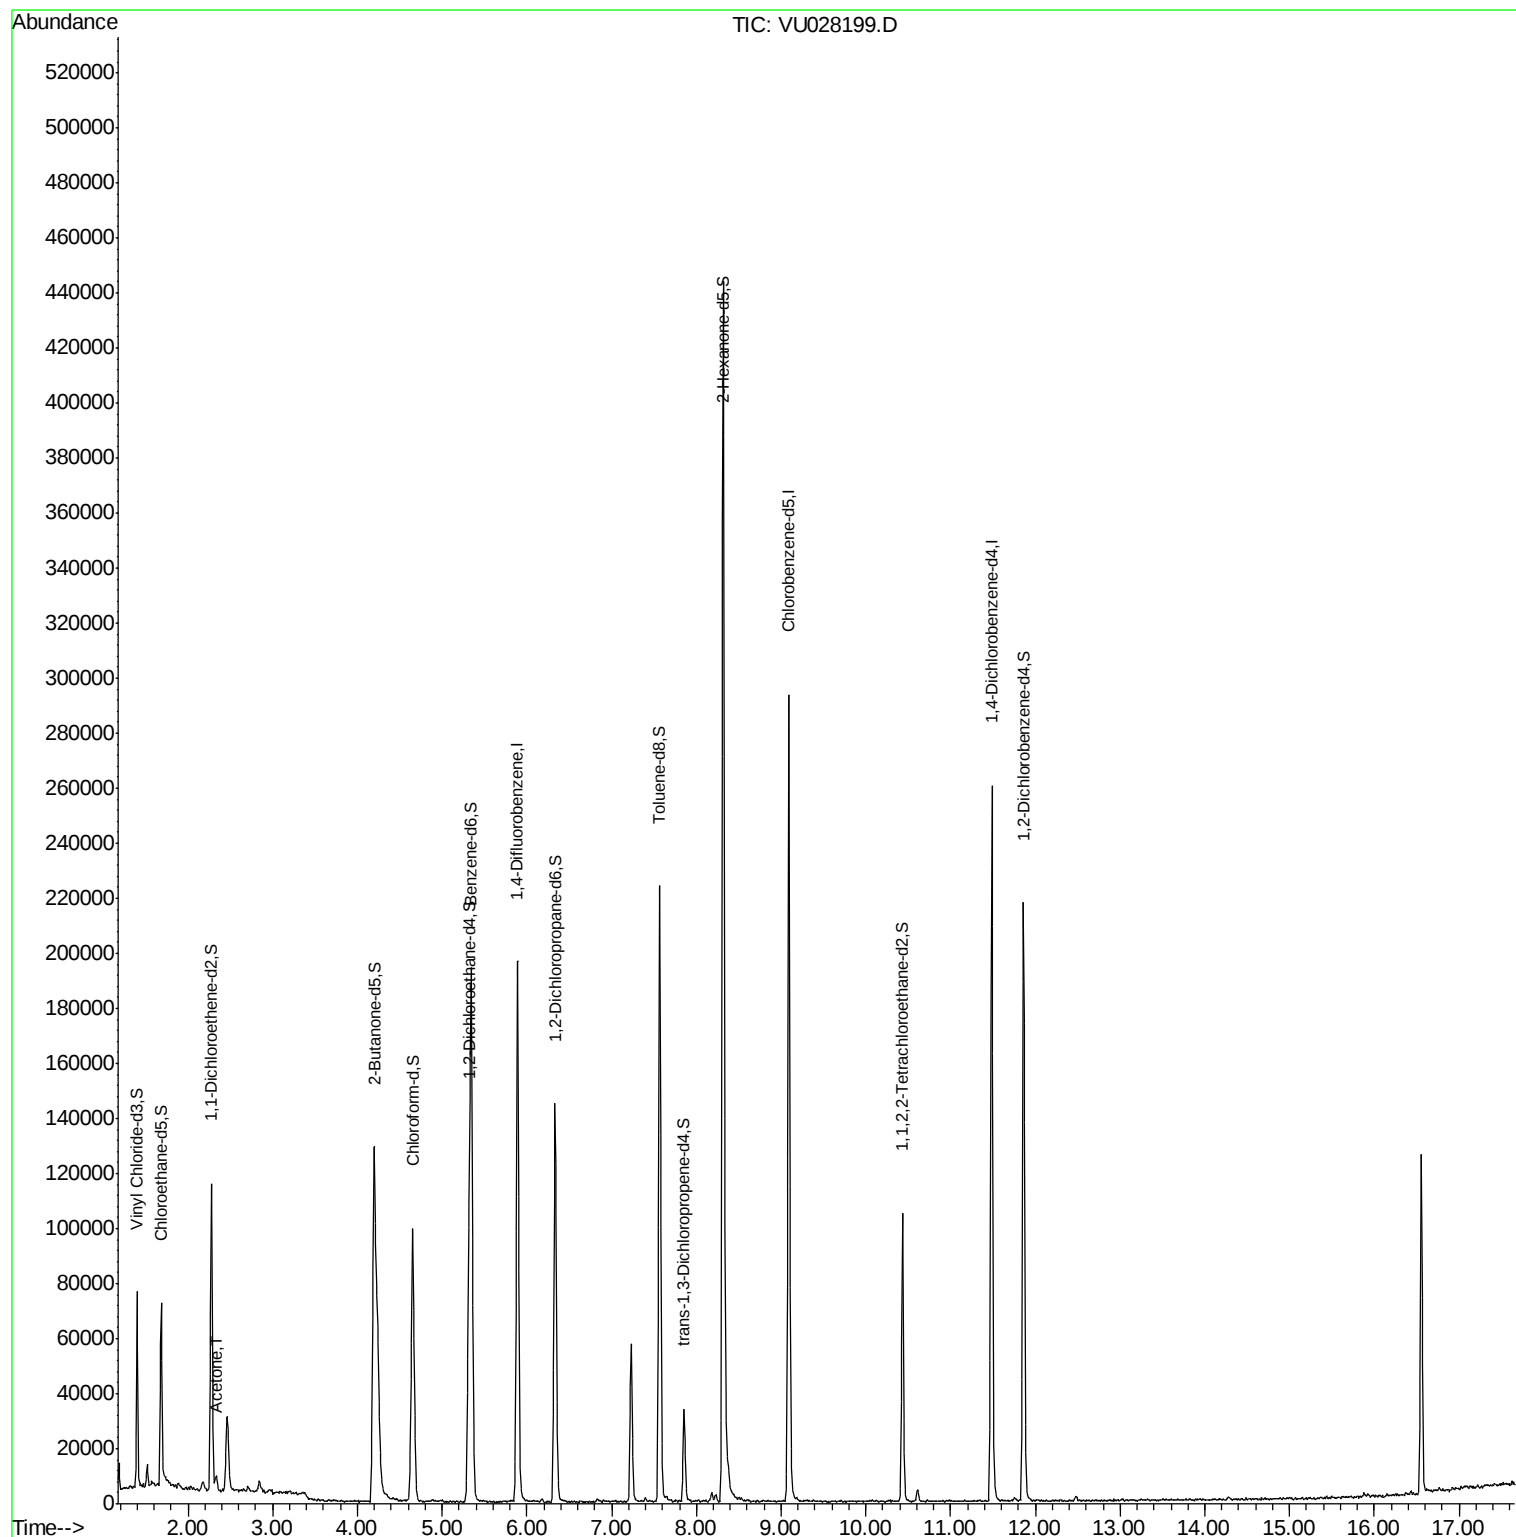

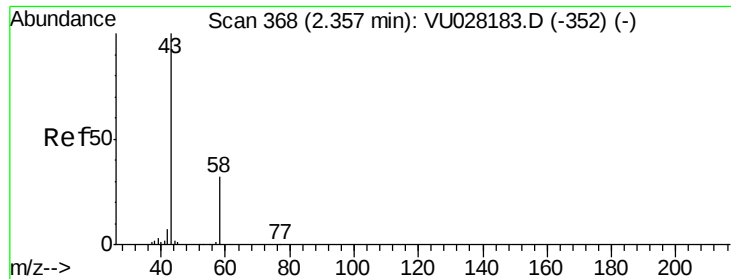

#13

Acetone

Concen: 2.079 ug/L

RT: 2.33 min Scan# 360

Delta R.T. -0.03 min

Lab File: VU028199.D

Acq: 16 Nov 2018 21:21

Instrument :

MSVOA_U

ClientSampleId :

C0AK5

Tgt Ion: 43 Resp: 5152

Ion Ratio Lower Upper

43 100

58 21.9 0.0 61.6

