

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU111618\
 Data File : VU028207.D
 Acq On : 17 Nov 2018 01:18
 Operator : MD/SY
 Sample : J5986-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0FG8

Quant Time: Nov 17 04:02:06 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111418WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Nov 17 03:46:40 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	156550	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	150004	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	68362	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	63862	4.92	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.40%
7) Chloroethane-d5	1.68	69	50802	4.92	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.40%
11) 1,1-Dichloroethene-d2	2.28	63	92299	3.80	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.00%
20) 2-Butanone-d5	4.20	46	217093	57.62	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.24%
24) Chloroform-d	4.65	84	105725	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.40%
26) 1,2-Dichloroethane-d4	5.31	65	63341	5.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.80%
32) Benzene-d6	5.34	84	218584	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.40%
36) 1,2-Dichloropropane-d6	6.33	67	80602	5.23	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.60%
41) Toluene-d8	7.57	98	189289	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.40%
43) trans-1,3-Dichloropropene-	7.85	79	23829	4.34	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.80%
46) 2-Hexanone-d5	8.31	63	163833	52.20	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.40%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	57422	5.27	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.40%
64) 1,2-Dichlorobenzene-d4	11.86	152	65092	5.10	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.00%

Target Compounds


					Qvalue
5) Vinyl chloride	1.40	62	91391	5.450 ug/L	99
17) Methyl tert-butyl Ether	3.01	73	219876	7.555 ug/L	98
18) trans-1,2-Dichloroethene	2.98	96	29925	2.704 ug/L	96
19) 1,1-Dichloroethane	3.45	63	17348	0.745 ug/L	97
22) cis-1,2-Dichloroethene	4.23	96	992064	81.306 ug/L	96
33) Benzene	5.40	78	9920	0.196 ug/L	100
34) Trichloroethene	6.19	95	192809	15.438 ug/L	97
47) Tetrachloroethene	8.23	164	2293	0.226 ug/L #	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU111618\
Data File : VU028207.D
Acq On : 17 Nov 2018 01:18
Operator : MD/SY
Sample : J5986-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0FG8

Quant Time: Nov 17 04:02:06 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111418WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Nov 17 03:46:40 2018
Response via : Initial Calibration

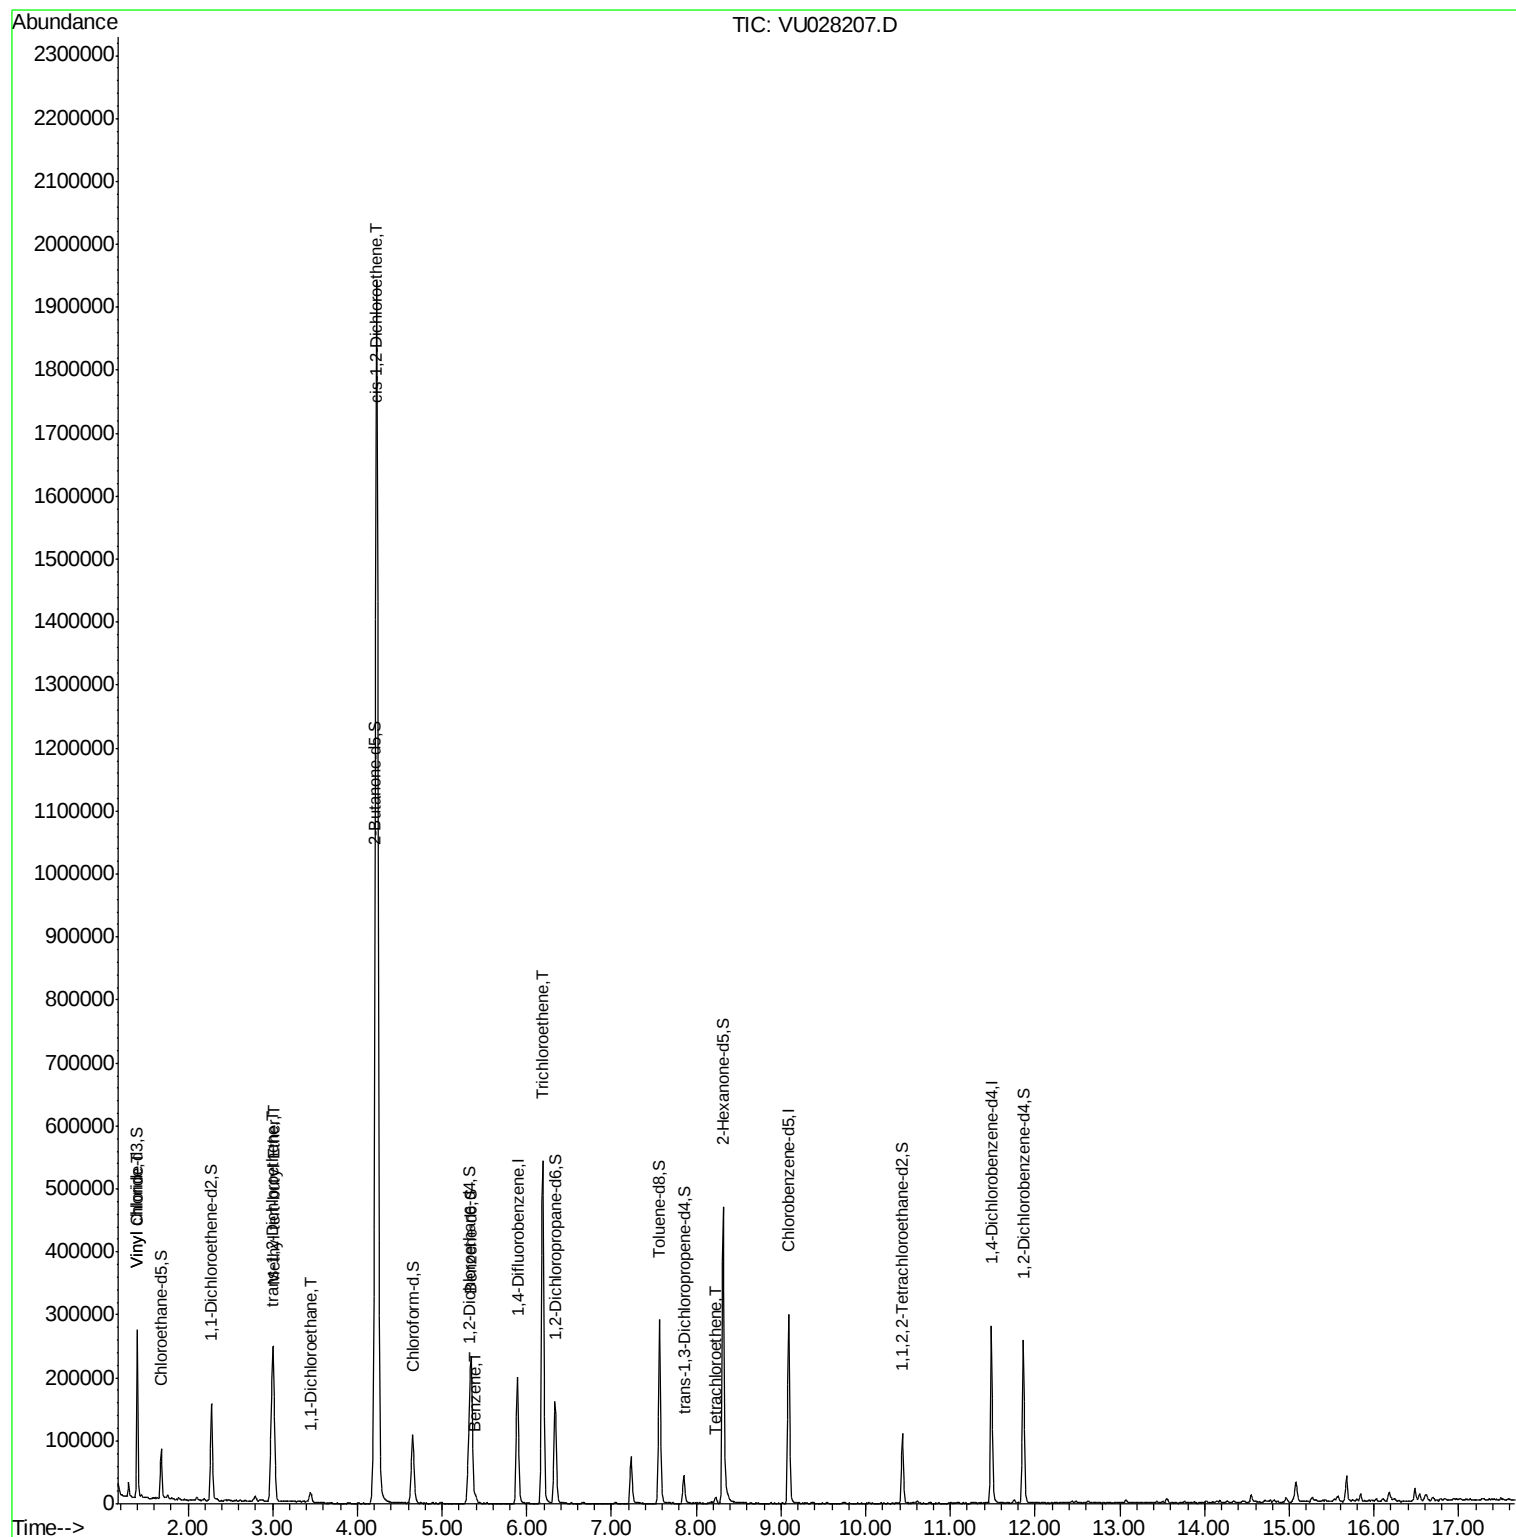

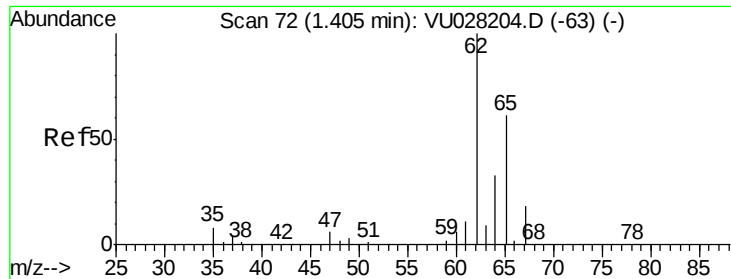

#5

Vinyl chloride

Concen: 5.450 ug/L

RT: 1.40 min Scan# 72

Delta R.T. -0.00 min

Lab File: VU028207.D

Acq: 17 Nov 2018 01:18

Instrument :

MSVOA_U

ClientSampled :


H0FG8

Tgt Ion: 62 Resp: 91391

Ion Ratio Lower Upper




62 100

64 33.0 22.7 42.3

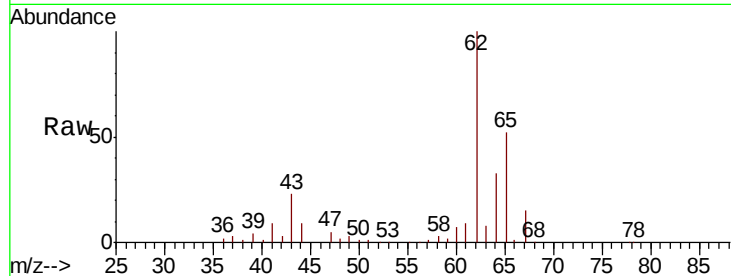

Abundance Ion 62.00 (61.70 to 62.70): VU0

Ion 64.10 (63.80 to 64.80): VU0

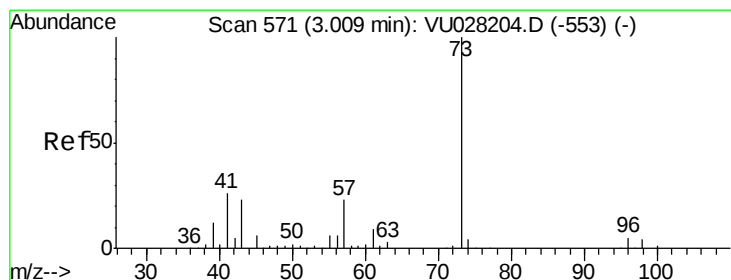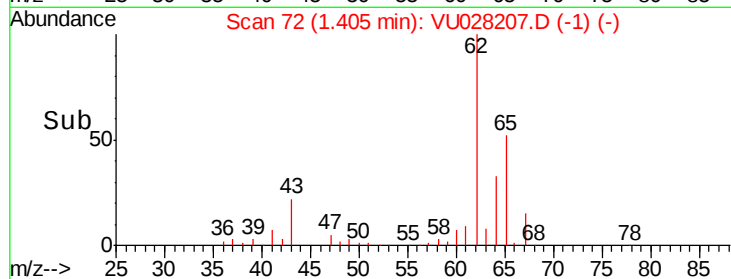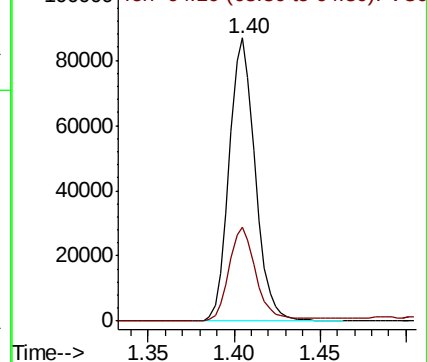

#17

Methyl tert-butyl Ether

Concen: 7.555 ug/L

RT: 3.01 min Scan# 570

Delta R.T. -0.00 min

Lab File: VU028207.D

Acq: 17 Nov 2018 01:18


Tgt Ion: 73 Resp: 219876

Ion Ratio Lower Upper

73 100

43 24.6 18.1 27.1



57 25.0 20.0 30.0

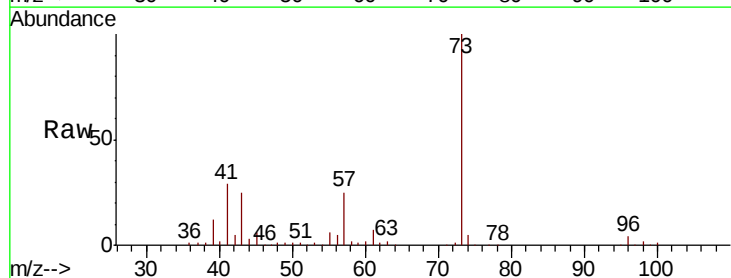


Abundance Ion 73.10 (72.80 to 73.80): VU0

Ion 43.05 (42.75 to 43.75): VU0

Ion 57.10 (56.80 to 57.80): VU0

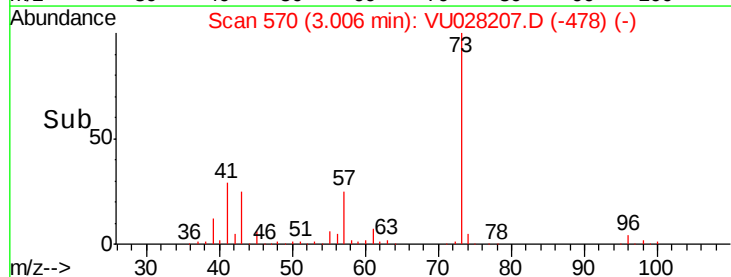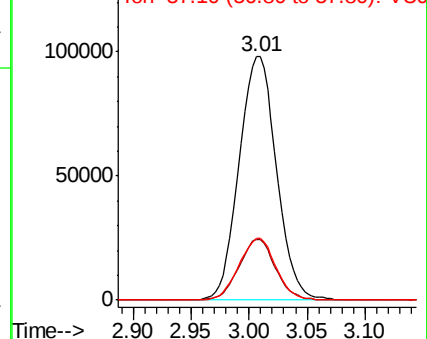


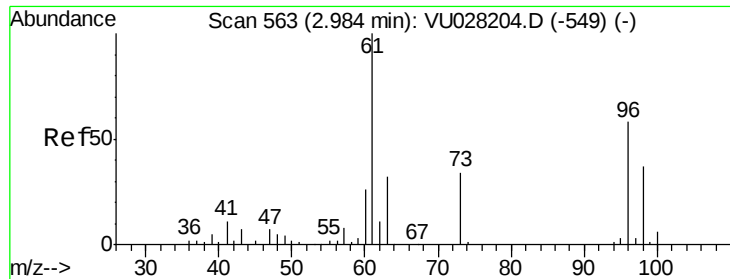




#18
trans-1,2-Dichloroethene
Concen: 2.704 ug/L
RT: 2.98 min Scan# 563
Delta R.T. -0.00 min
Lab File: VU028207.D
Acq: 17 Nov 2018 01:18

Instrument :
MSVOA_U
ClientSampleId :
H0FG8

Tgt Ion: 96 Resp: 29925
Ion Ratio Lower Upper
96 100
61 175.8 118.5 220.1
98 61.2 44.9 83.5

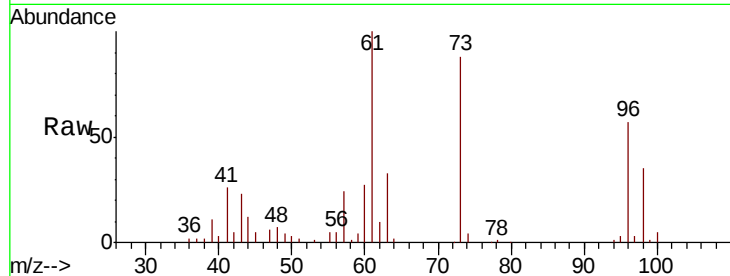


Abundance Ion 96.00 (95.70 to 96.70): VU0
Ion 61.05 (60.75 to 61.75): VU0
Ion 97.95 (97.65 to 98.65): VU0

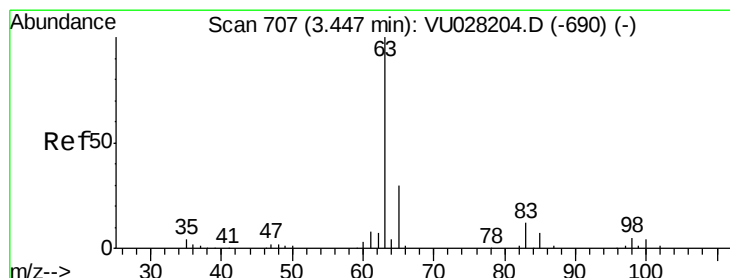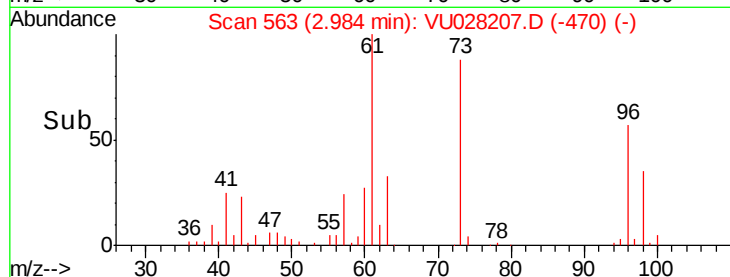
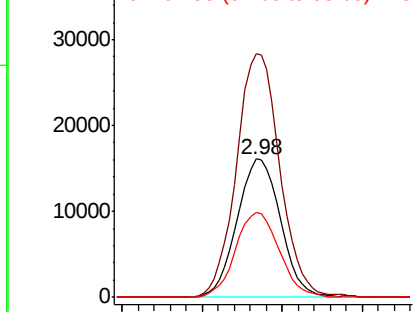



#19
1,1-Dichloroethane
Concen: 0.745 ug/L
RT: 3.45 min Scan# 707
Delta R.T. -0.00 min
Lab File: VU028207.D
Acq: 17 Nov 2018 01:18

Tgt Ion: 63 Resp: 17348
Ion Ratio Lower Upper
63 100
65 33.7 22.2 41.2
83 12.3 8.9 16.5

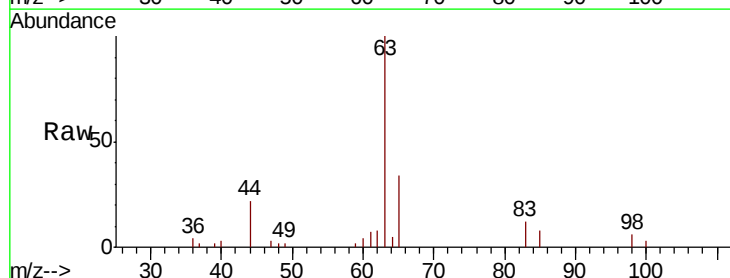

Abundance Ion 63.10 (62.80 to 63.80): VU0
Ion 65.10 (64.80 to 65.80): VU0
Ion 83.05 (82.75 to 83.75): VU0

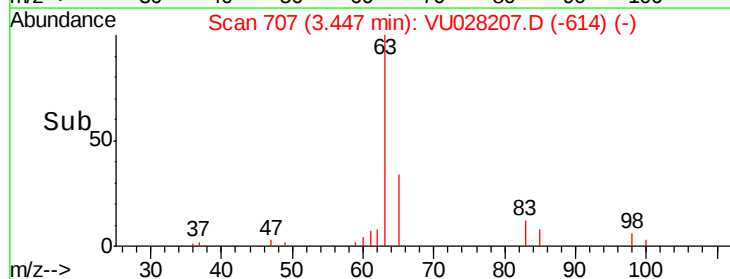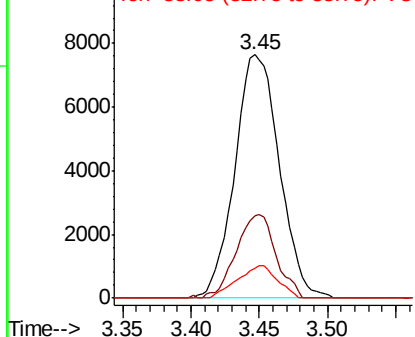

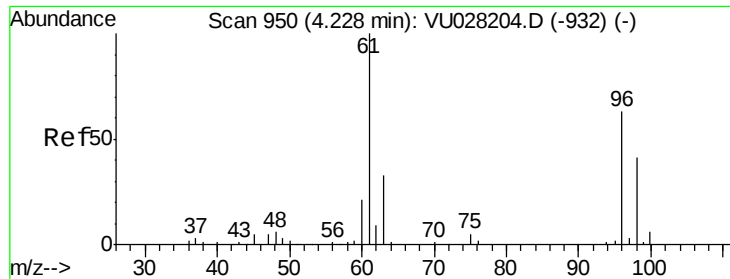

#22

cis-1,2-Dichloroethene

Concen: 81.306 ug/L

RT: 4.23 min Scan# 950

Delta R.T. -0.00 min

Lab File: VU028207.D

Acq: 17 Nov 2018 01:18

Instrument :

MSVOA_U

ClientSampleId :

H0FG8


Tgt Ion: 96 Resp: 992064

Ion Ratio Lower Upper

96 100

61 150.6 101.8 189.0




68 0.0 0.0 0.0

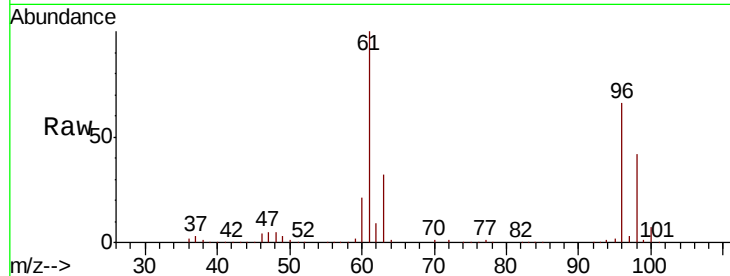

Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 61.05 (60.75 to 61.75): VU0

Ion 68.15 (67.85 to 68.85): VU0

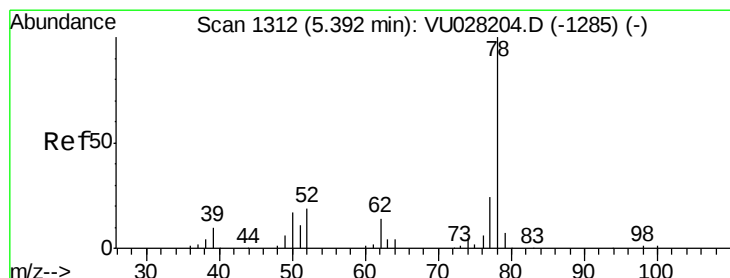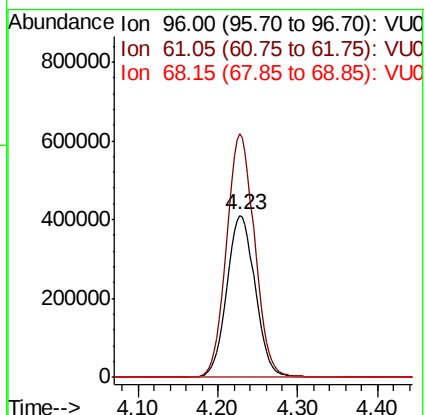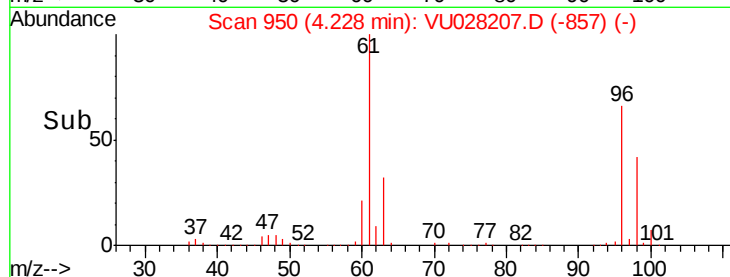

#33

Benzene

Concen: 0.196 ug/L


RT: 5.40 min Scan# 1313

Delta R.T. 0.00 min



Lab File: VU028207.D


Acq: 17 Nov 2018 01:18

Tgt Ion: 78 Resp: 9920

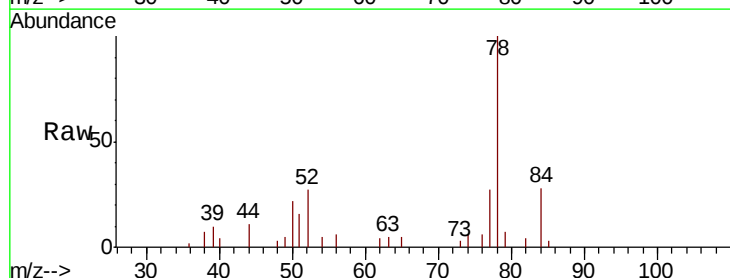

Abundance Ion 78.10 (77.80 to 78.80): VU0

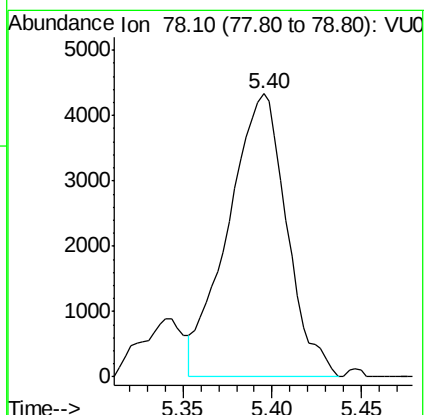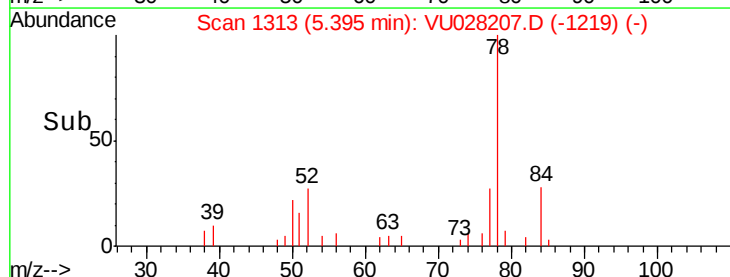

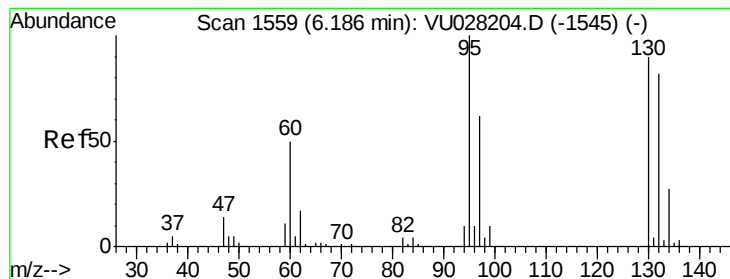

#34

Trichloroethene

Concen: 15.438 ug/L

RT: 6.19 min Scan# 1559

Delta R.T. -0.00 min

Lab File: VU028207.D

Acq: 17 Nov 2018 01:18

Instrument :

MSVOA_U

ClientSampleId :

H0FG8

Tgt Ion: 95 Resp: 192809


Ion Ratio Lower Upper

95 100

97 67.4 45.3 84.1

132 86.0 63.0 117.0

130 90.1 63.6 118.2



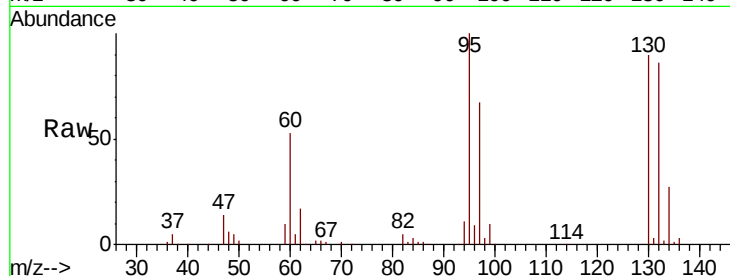


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

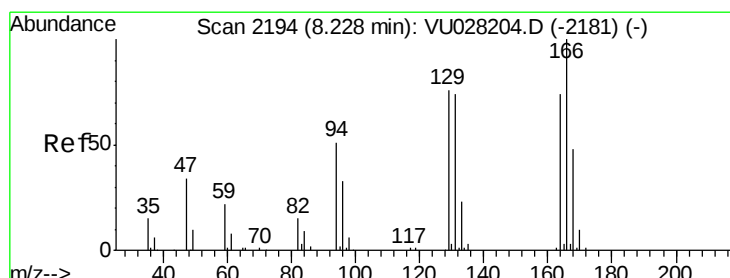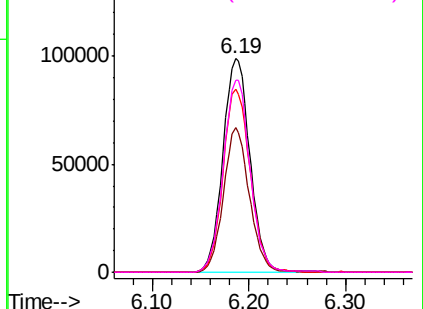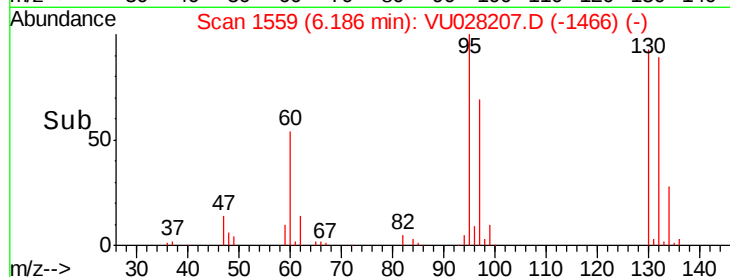

#47

Tetrachloroethene

Concen: 0.226 ug/L

RT: 8.23 min Scan# 2195

Delta R.T. 0.00 min

Lab File: VU028207.D

Acq: 17 Nov 2018 01:18

Tgt Ion: 164 Resp: 2293


Ion Ratio Lower Upper

164 100

129 67.5 69.7 129.4#

131 79.3 64.0 118.8

166 117.6 86.4 160.4

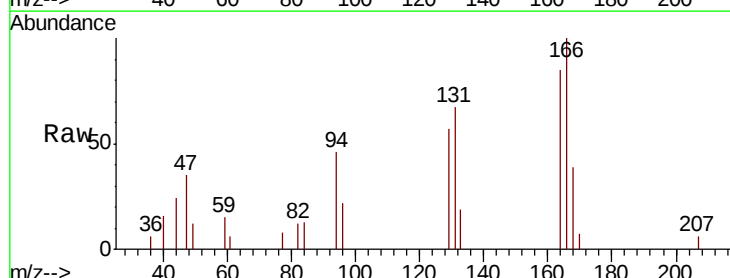

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

