

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU111620\
 Data File : VU041245.D
 Acq On : 16 Nov 2020 14:10
 Operator : SY/MD
 Sample : L4754-04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BW6

Quant Time: Nov 17 07:25:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Nov 16 12:08:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	69122	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	73038	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	28616	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	24009	4.72	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.40%
7) Chloroethane-d5	1.92	69	22949	5.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.60%
11) 1,1-Dichloroethene-d2	2.58	63	38087	3.63	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.60%
20) 2-Butanone-d5	4.66	46	106668	50.88	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.76%
24) Chloroform-d	5.08	84	54802	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.60%
26) 1,2-Dichloroethane-d4	5.72	65	33888	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.40%
32) Benzene-d6	5.74	84	97748	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.20%
36) 1,2-Dichloropropane-d6	6.70	67	33678	4.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.20%
41) Toluene-d8	7.90	98	75032	4.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.00%
43) trans-1,3-Dichloropropene-	8.19	79	11380	3.90	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.00%
46) 2-Hexanone-d5	8.64	63	74669	47.87	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.74%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	27545	4.18	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.60%
64) 1,2-Dichlorobenzene-d4	12.19	152	29168	5.22	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.40%


Target Compounds					Ovalue
13) Acetone	2.66	43	4297	3.090 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU111620\
Data File : VU041245.D
Acq On : 16 Nov 2020 14:10
Operator : SY/MD
Sample : L4754-04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BW6

Quant Time: Nov 17 07:25:00 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Nov 16 12:08:29 2020
Response via : Initial Calibration

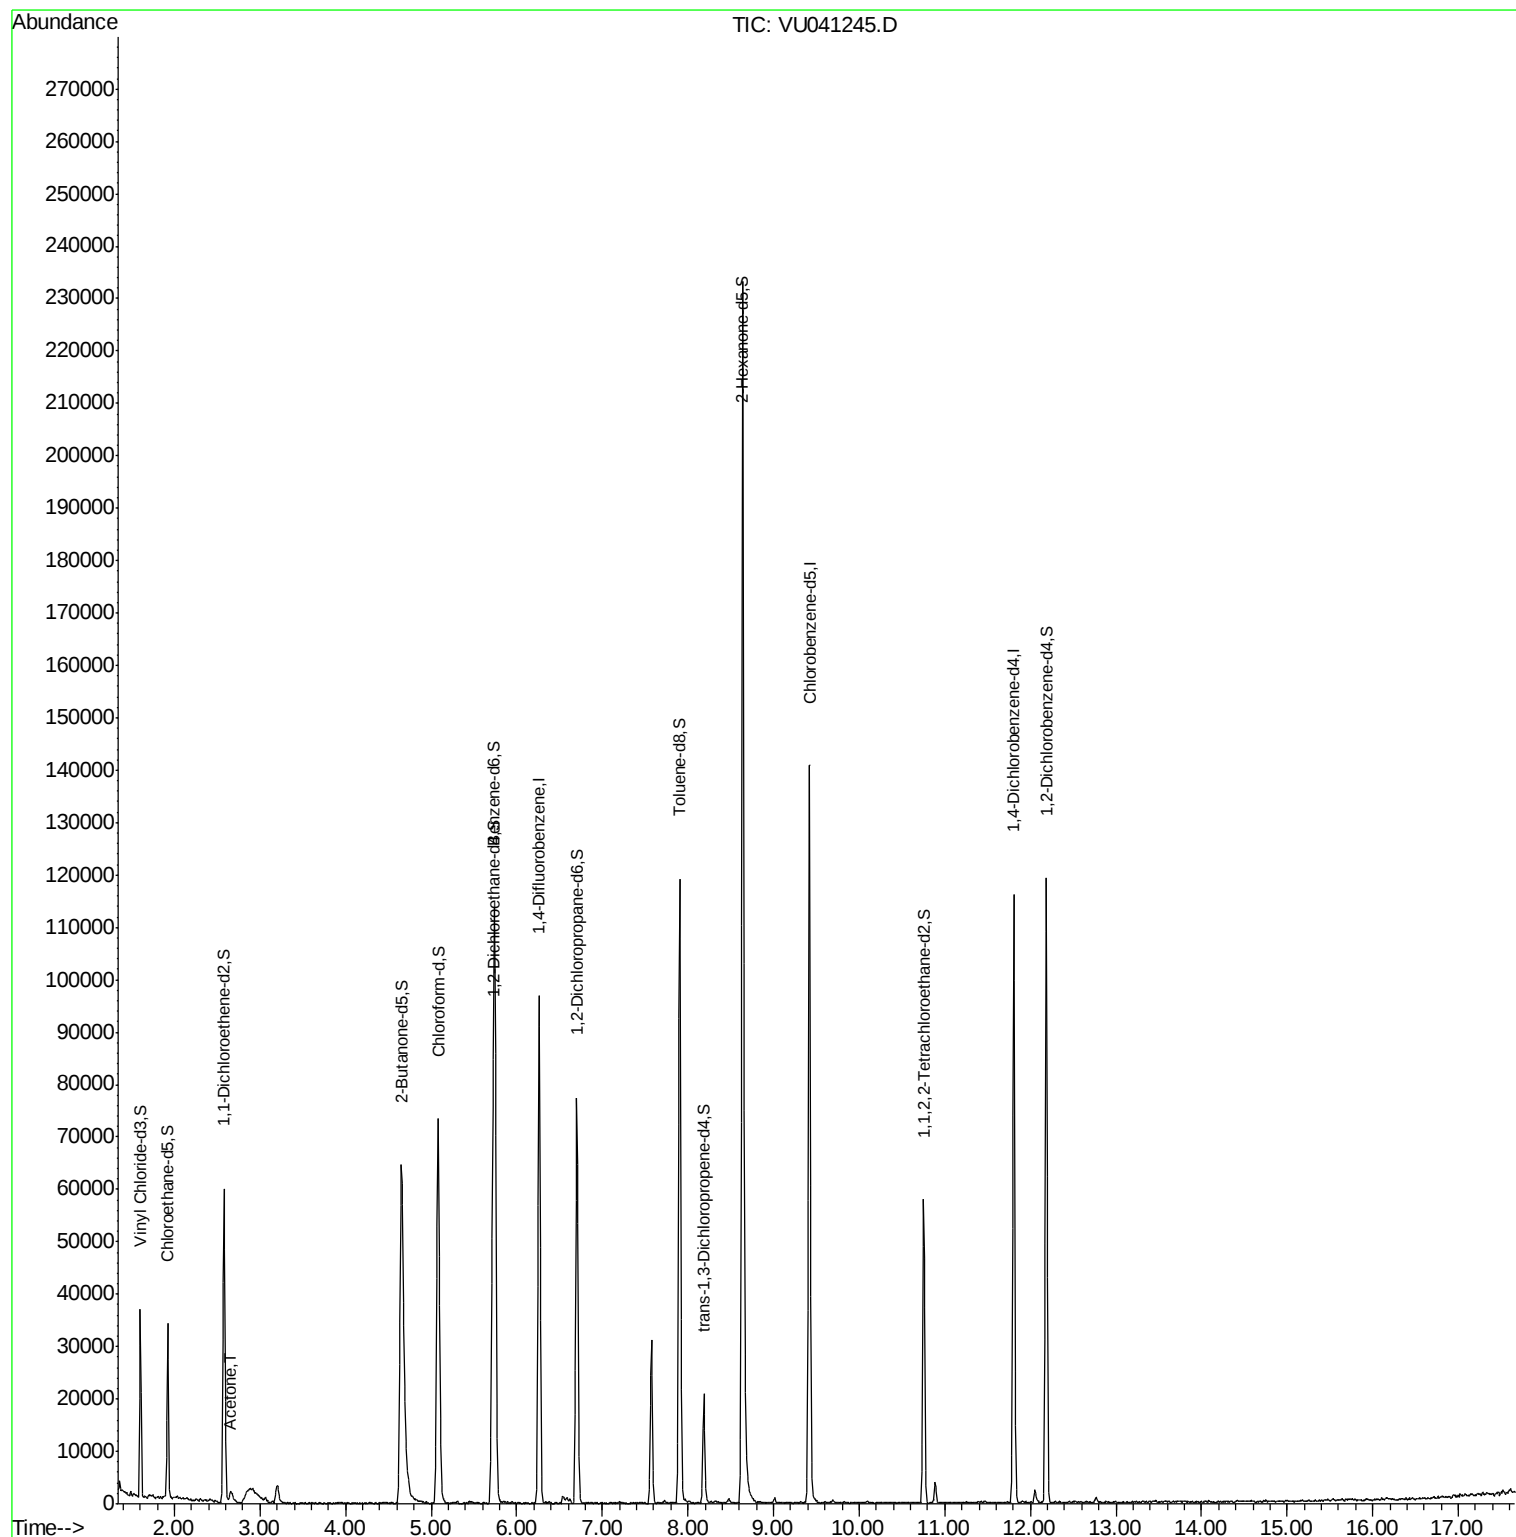

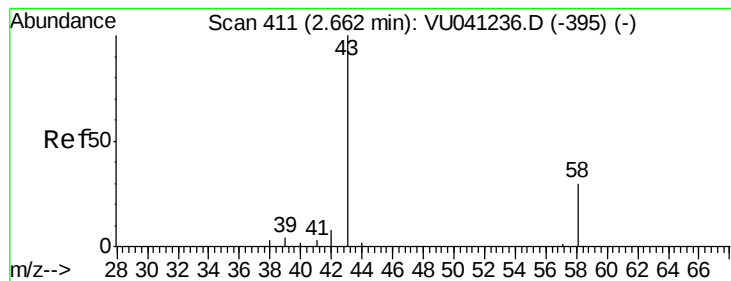

#13
 Acetone
 Concen: 3.090 ug/L
 RT: 2.66 min Scan# 410
 Delta R.T. -0.00 min
 Lab File: VU041245.D
 Acq: 16 Nov 2020 14:10

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BW6

Tot Ion: 43 Resp: 4297
 Ion Ratio Lower Upper
 43 100
 58 16.8 0.0 25.4

