

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU111620\
 Data File : VU041258.D
 Acq On : 16 Nov 2020 19:35
 Operator : SY/MD
 Sample : L4759-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4387

Quant Time: Nov 17 10:01:35 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Nov 16 12:08:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	70318	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	73250	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	29351	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	24270	4.69	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.80%
7) Chloroethane-d5	1.92	69	21869	4.94	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.80%
11) 1,1-Dichloroethene-d2	2.58	63	35676	3.34	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.80%
20) 2-Butanone-d5	4.66	46	100647	47.19	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.38%
24) Chloroform-d	5.08	84	52065	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.00%
26) 1,2-Dichloroethane-d4	5.72	65	35120	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.20%
32) Benzene-d6	5.74	84	95496	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
36) 1,2-Dichloropropane-d6	6.70	67	35313	5.19	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.80%
41) Toluene-d8	7.91	98	74794	4.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.40%
43) trans-1,3-Dichloropropene-	8.19	79	13647	4.66	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.20%
46) 2-Hexanone-d5	8.64	63	73902	47.24	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.48%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	31583	4.78	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.60%
64) 1,2-Dichlorobenzene-d4	12.19	152	30422	5.31	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.20%


Target Compounds					Ovalue
13) Acetone	2.66	43	3119	2.205 ug/L	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU111620\
Data File : VU041258.D
Acq On : 16 Nov 2020 19:35
Operator : SY/MD
Sample : L4759-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4387

Quant Time: Nov 17 10:01:35 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Nov 16 12:08:29 2020
Response via : Initial Calibration

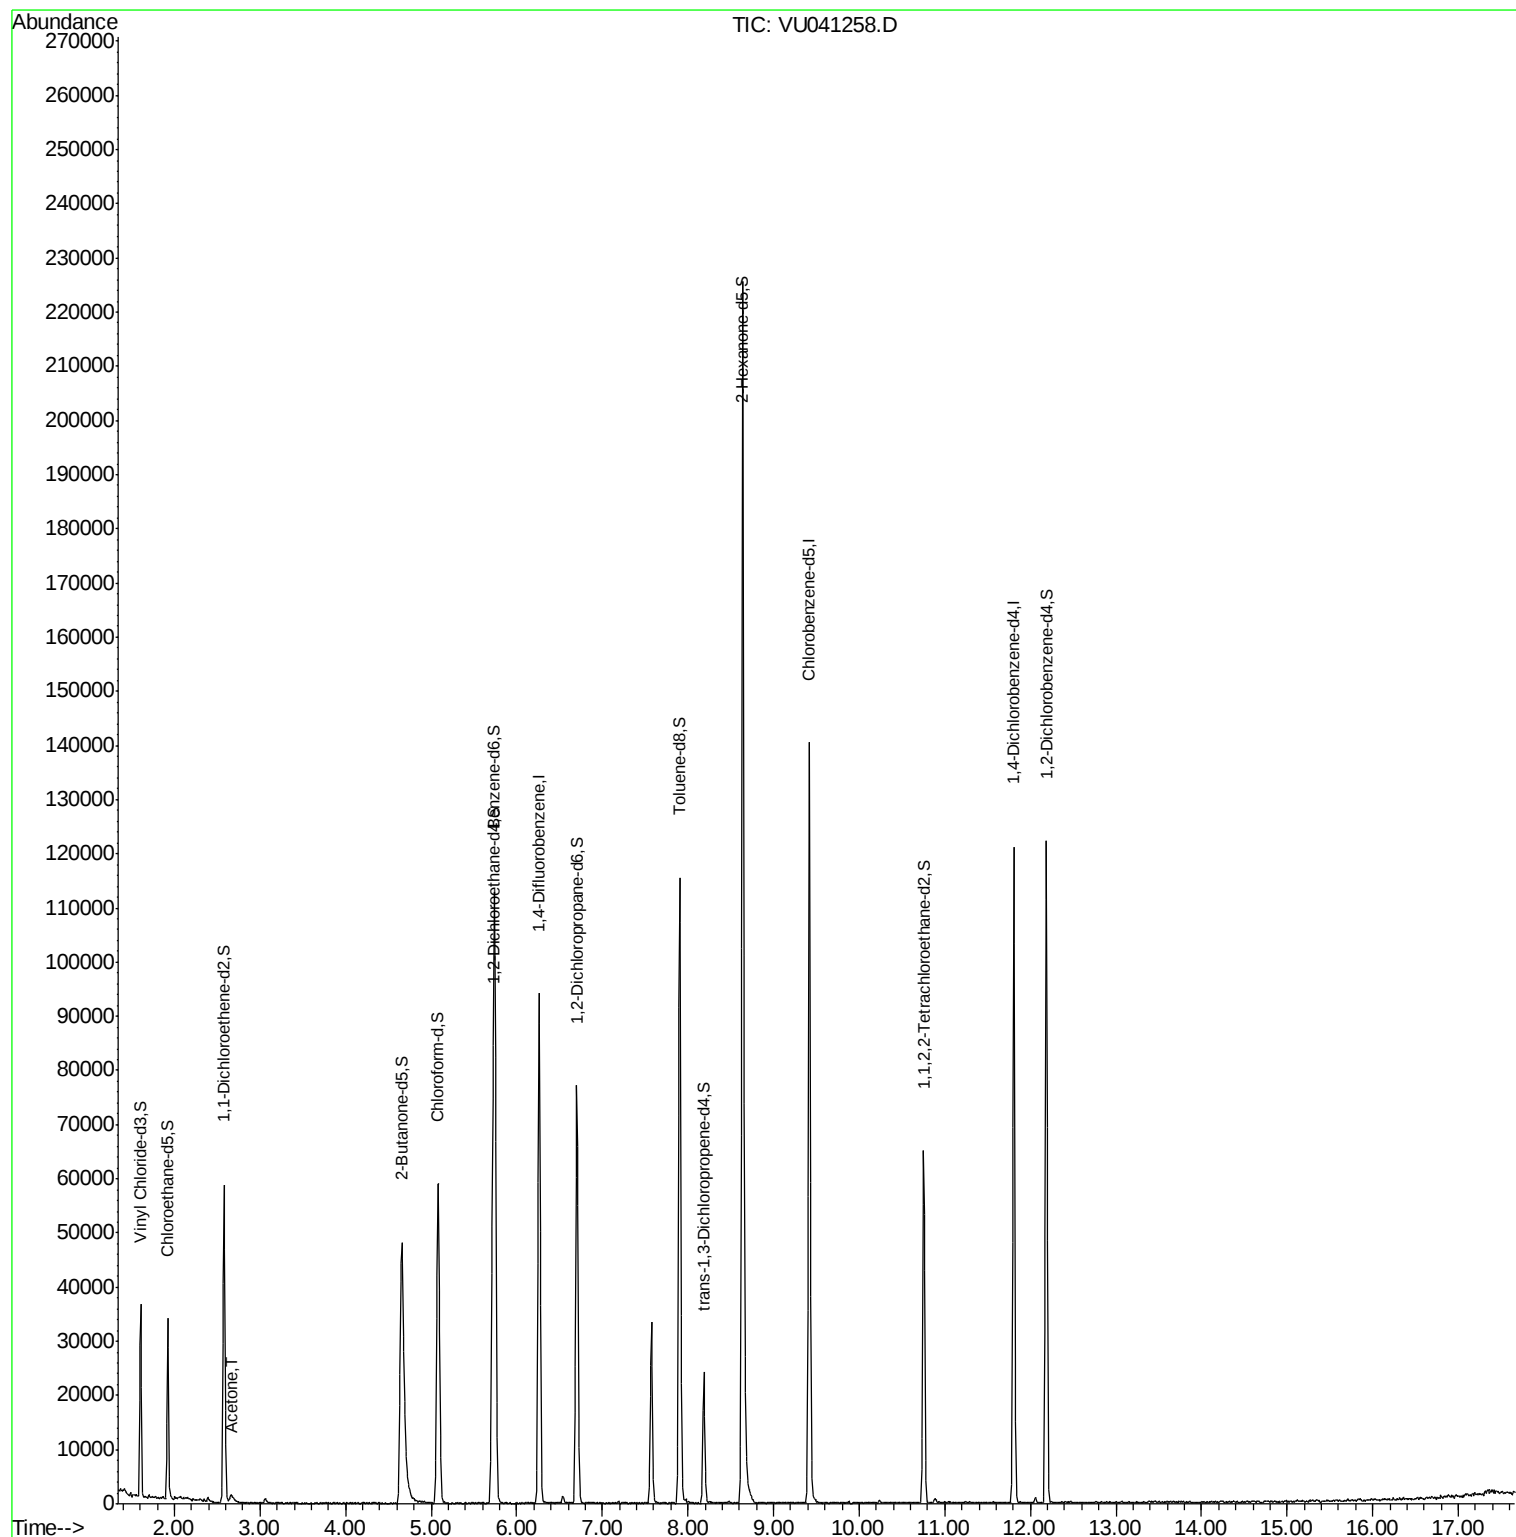

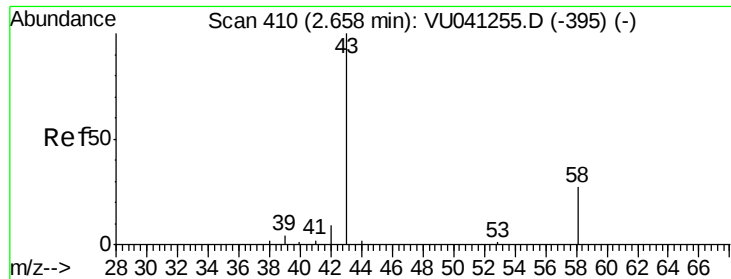

#13
 Acetone
 Concen: 2.205 ug/L
 RT: 2.66 min Scan# 411
 Delta R.T. 0.00 min
 Lab File: VU041258.D
 Acq: 16 Nov 2020 19:35

Instrument :
 MSVOA_U
 ClientSampleId :
 H4387

Tot Ion: 43 Resp: 3119
 Ion Ratio Lower Upper
 43 100
 58 21.9 0.0 25.4

