

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU111620\
 Data File : VU041264.D
 Acq On : 16 Nov 2020 21:54
 Operator : SY/MD
 Sample : L4740-13
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB118

Quant Time: Nov 17 10:24:07 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Nov 16 12:08:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	69345	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	66696	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	28184	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	24790	4.86	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.20%
7) Chloroethane-d5	1.92	69	21991	5.04	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.80%
11) 1,1-Dichloroethene-d2	2.58	63	33966	3.22	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.40%
20) 2-Butanone-d5	4.65	46	97291	46.26	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.52%
24) Chloroform-d	5.08	84	50673	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.80%
26) 1,2-Dichloroethane-d4	5.72	65	32175	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.40%
32) Benzene-d6	5.74	84	93074	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.60%
36) 1,2-Dichloropropane-d6	6.70	67	33720	5.44	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.80%
41) Toluene-d8	7.90	98	71223	4.20	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.00%
43) trans-1,3-Dichloropropene-	8.19	79	10740	4.03	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.60%
46) 2-Hexanone-d5	8.64	63	71740	50.36	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.72%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	28954	4.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.40%
64) 1,2-Dichlorobenzene-d4	12.19	152	26864	4.89	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.80%


Target Compounds					Ovalue
13) Acetone	2.66	43	1809	1.297 ug/L	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU111620\
Data File : VU041264.D
Acq On : 16 Nov 2020 21:54
Operator : SY/MD
Sample : L4740-13
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB118

Quant Time: Nov 17 10:24:07 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Nov 16 12:08:29 2020
Response via : Initial Calibration

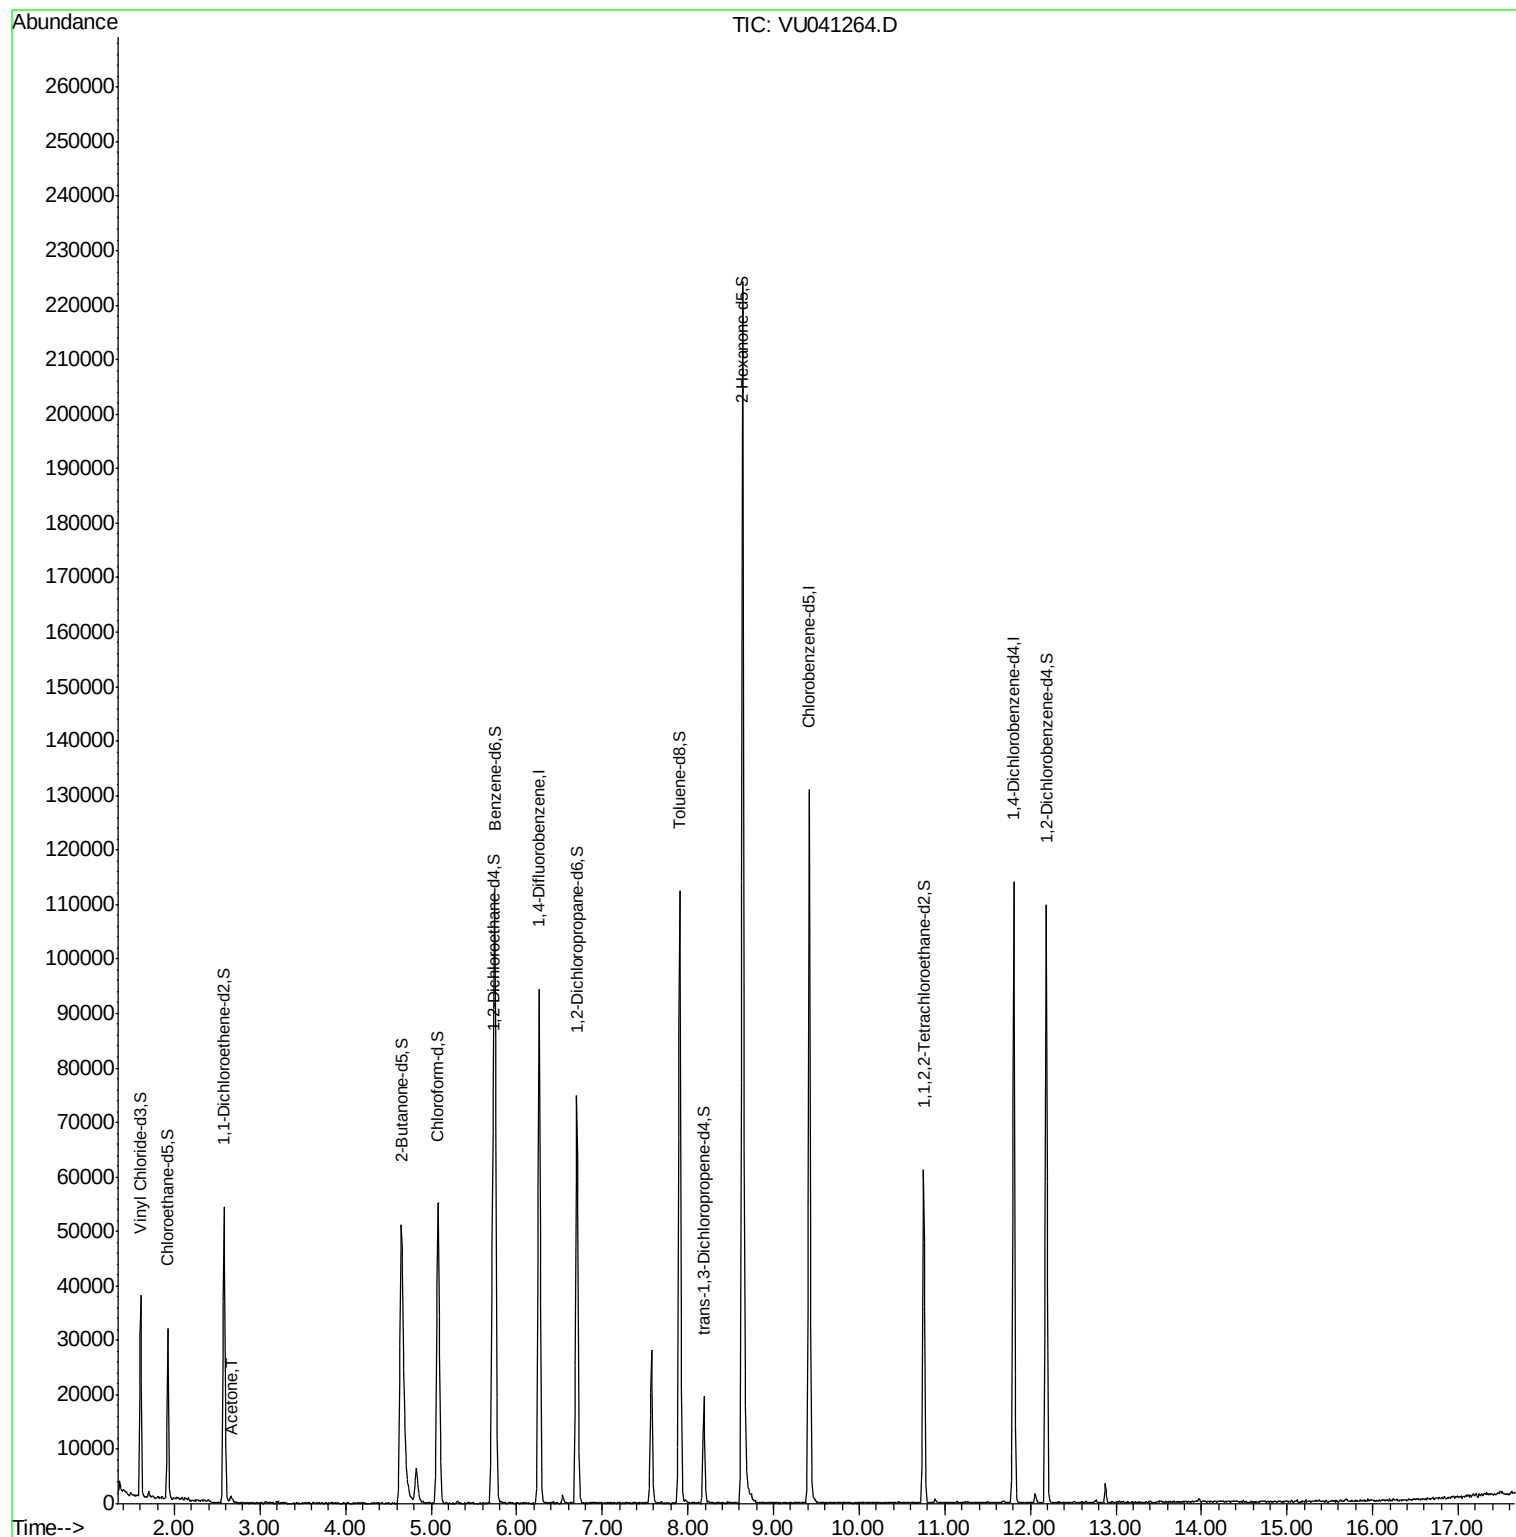

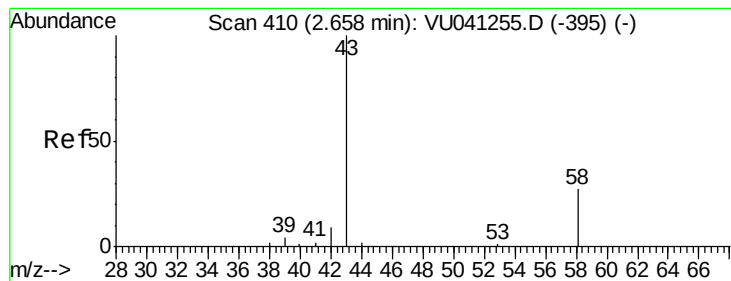

#13
 Acetone
 Concen: 1.297 ug/L
 RT: 2.66 min Scan# 411
 Delta R.T. 0.00 min
 Lab File: VU041264.D
 Acq: 16 Nov 2020 21:54

Instrument :
 MSVOA_U
 ClientSampleId :
 GB118

Tot Ion: 43 Resp: 1809
 Ion Ratio Lower Upper
 43 100
 58 22.1 0.0 25.4

