


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU111620\
 Data File : VU041233.D
 Acq On : 16 Nov 2020 08:09
 Operator : SY/MD
 Sample : BFB12
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB12

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Nov 16 12:08:29 2020

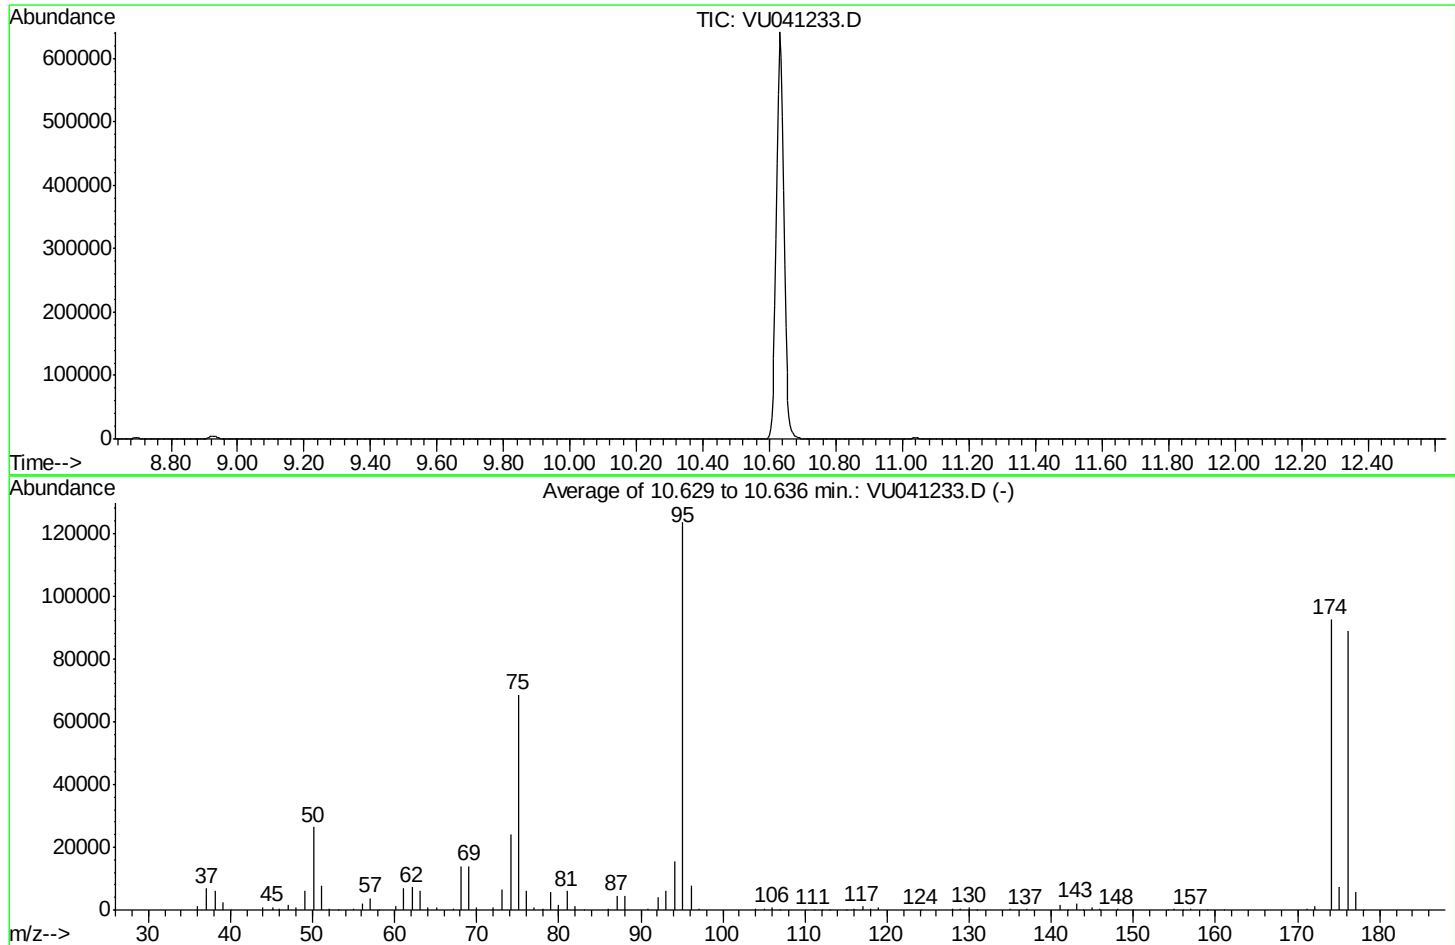

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	26333	PASS
75	95	30	80	55.6	68661	PASS
95	95	100	100	100.0	123488	PASS
96	95	5	9	6.4	7897	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.9	92520	PASS
175	174	5	9	7.9	7307	PASS
176	174	95	101	96.0	88821	PASS
177	176	5	9	6.2	5551	PASS

m/z	Abundance
36.00	1140.0
37.10	6897.0
38.10	6376.0
39.10	2688.0
40.00	151.0
44.00	903.0
45.10	936.0
46.10	293.0
47.10	1736.0
48.00	859.0
49.00	6297.0
50.10	26920.0
51.10	8112.0
52.10	417.0
53.10	212.0
55.00	443.0
56.00	2022.0
57.10	3854.0
58.10	142.0
60.10	1361.0
61.10	7144.0
62.10	7286.0
63.10	6081.0
64.10	957.0
65.10	1073.0
67.10	397.0
68.10	14037.0
69.10	13904.0
70.00	1010.0
72.00	717.0
73.10	6838.0
74.10	24088.0
75.10	69568.0
76.10	6004.0
77.10	857.0
78.00	515.0
79.00	5785.0
80.00	1710.0
81.00	6125.0
82.00	1161.0
83.00	172.0
86.10	227.0
87.10	4903.0
88.10	4726.0
90.90	548.0
92.10	4129.0
93.10	5982.0
94.10	15393.0
95.10	123128.0
96.10	7998.0
97.10	253.0
103.90	619.0
105.00	228.0
106.00	709.0
107.00	133.0
110.00	126.0
111.00	137.0
113.00	152.0
115.10	180.0
116.00	540.0
117.00	1073.0
118.00	509.0
119.00	945.0
124.10	100.0
128.00	578.0
129.00	229.0
130.00	655.0
131.00	232.0
135.00	277.0
137.00	289.0
141.00	1536.0
142.00	230.0
143.10	2166.0
143.90	129.0
145.00	776.0
145.90	238.0
148.00	272.0
150.00	153.0
154.10	149.0
155.00	250.0
157.00	267.0
159.00	129.0
171.10	322.0
172.10	1001.0
174.10	90480.0
175.10	7148.0
176.10	86952.0
177.10	5524.0
178.00	213.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
36.00	1091.0
37.10	7110.0
38.10	6515.0
39.10	2664.0
40.00	159.0
44.00	909.0
45.10	991.0
46.00	243.0
47.10	1760.0
48.10	919.0
49.00	6262.0
50.10	27136.0
51.10	8152.0
52.00	443.0
53.10	151.0
55.00	450.0
56.00	2131.0
57.10	3894.0
58.10	172.0
60.10	1314.0
61.10	7177.0
62.10	7448.0
63.10	6212.0
64.10	1013.0
65.10	947.0
67.10	419.0
68.10	14492.0
69.10	14431.0
70.00	1005.0
72.00	744.0
73.10	6886.0
74.10	24704.0
75.10	70856.0
76.10	6345.0
77.10	822.0
78.00	530.0
79.00	5874.0
80.00	1752.0
81.00	6215.0
82.00	1219.0
83.00	174.0
86.10	253.0
87.10	4874.0
88.10	4715.0
90.90	594.0
92.10	4484.0
93.10	6270.0
94.10	16051.0
95.10	127648.0
96.10	8175.0
97.10	237.0
104.00	610.0
105.10	239.0
106.00	712.0
106.90	156.0
110.00	125.0
111.10	147.0
112.90	150.0
115.10	157.0
116.00	587.0
117.00	1086.0
118.00	591.0
119.00	950.0
124.10	123.0
128.00	595.0
129.00	268.0
130.00	670.0
131.00	223.0
135.00	303.0
137.00	311.0
141.00	1622.0
142.00	204.0
143.00	2105.0
143.90	118.0
145.00	703.0
145.90	247.0
148.00	280.0
150.00	148.0
154.10	144.0
155.00	264.0
156.00	111.0
157.00	272.0
159.00	138.0
160.90	108.0
171.10	347.0
172.10	1100.0
174.10	95632.0
175.10	7561.0
176.10	91832.0
177.10	5695.0
178.00	205.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
36.00	1005.0
37.10	6615.0
38.10	6047.0
39.10	2413.0
40.00	168.0
44.00	861.0
45.10	989.0
45.90	223.0
47.10	1629.0
48.00	875.0
49.00	5581.0
50.10	24944.0
51.10	7477.0
52.00	405.0
55.00	393.0
56.10	2039.0
57.10	3626.0
58.10	164.0
60.10	1169.0
61.10	6567.0
62.10	6763.0
63.10	5604.0
64.10	960.0
65.10	815.0
67.10	384.0
68.10	13280.0
69.10	13592.0
70.00	991.0
72.00	715.0
73.10	6012.0
74.10	23000.0
75.10	65560.0
76.10	6060.0
77.00	738.0
78.00	526.0
79.00	5446.0
80.00	1603.0
81.00	5660.0
82.00	1124.0
83.00	139.0
86.10	250.0
87.10	4320.0
88.00	4299.0
90.90	542.0
92.10	4259.0
93.10	5977.0
94.10	15135.0
95.10	119688.0
96.10	7520.0
97.10	188.0
104.00	576.0
105.10	223.0
106.00	627.0
106.90	149.0
111.10	150.0
112.00	116.0
112.90	143.0
115.10	134.0
116.00	521.0
117.00	1022.0
118.00	609.0
119.00	847.0
124.10	100.0
128.00	568.0
128.90	283.0
130.00	598.0
130.90	180.0
135.00	293.0
137.00	308.0
141.00	1548.0
142.00	172.0
143.10	1852.0
145.00	533.0
146.00	217.0
148.10	269.0
150.00	147.0
155.00	256.0
156.00	102.0
157.00	238.0
159.00	126.0
161.00	125.0
171.10	288.0
172.10	1083.0
174.10	91448.0
175.10	7212.0
176.10	87680.0
177.10	5435.0
178.00	196.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12

m/z	Abundance
43.90	125.0

Instrument :
MSVOA_U
ClientSampleId :
BFB12