


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111621\
Data File : VU045798.D
Acq On : 16 Nov 2021 09:11
Operator : SY/MD
Sample : BFB026
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB026

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Nov 19 00:50:55 2021

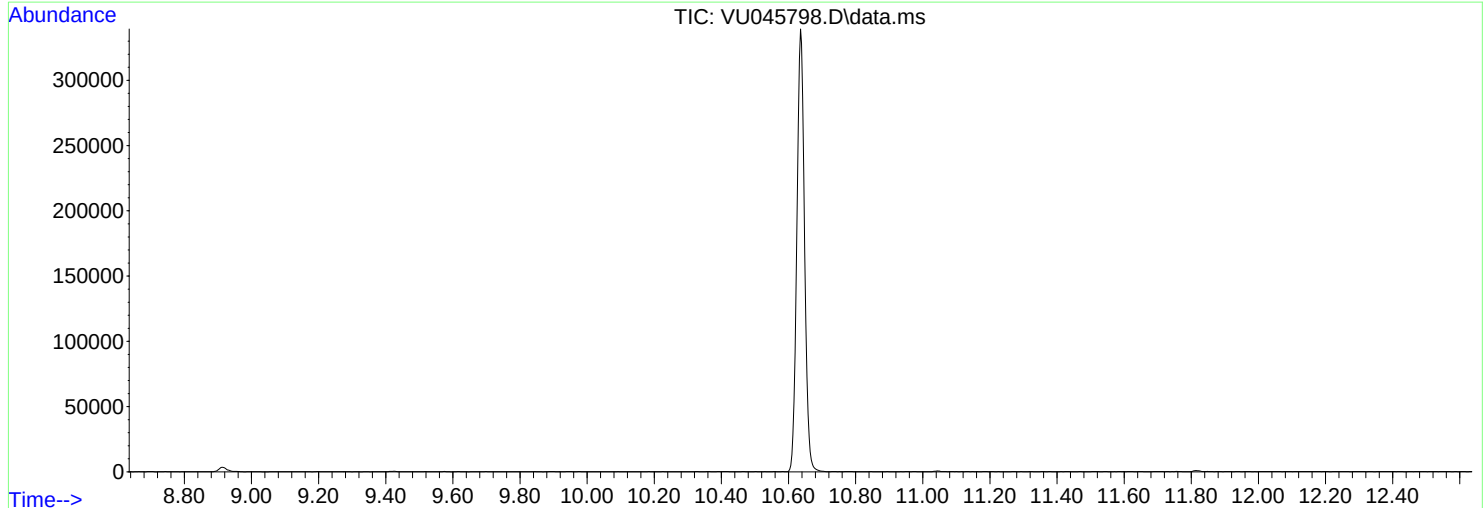

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	13091	PASS
75	95	30	80	52.7	36168	PASS
95	95	100	100	100.0	68688	PASS
96	95	5	9	6.7	4579	PASS
173	174	0.00	2	0.8	436	PASS
174	95	50	120	74.9	51440	PASS
175	174	5	9	7.0	3593	PASS
176	174	95	101	96.9	49840	PASS
177	176	5	9	6.5	3216	PASS

m/z	Abundance
36.00	456.0
37.00	2854.0
38.00	2457.0
39.00	1052.0
43.90	567.0
45.00	502.0
46.10	141.0
47.00	780.0
47.90	384.0
49.00	2748.0
50.00	12725.0
51.00	3836.0
52.00	230.0
54.90	262.0
56.00	975.0
57.00	1744.0
60.00	761.0
61.00	3628.0
62.00	3295.0
63.00	2651.0
64.00	440.0
65.00	459.0
67.00	109.0
68.00	6813.0
69.00	7043.0
70.00	482.0
72.00	394.0
73.00	3210.0
74.00	11971.0
75.00	35608.0
76.00	3064.0
77.00	439.0
78.00	218.0
78.90	2415.0
79.90	694.0
80.90	2670.0
81.90	518.0
85.90	156.0
87.00	3229.0
88.00	2822.0
90.90	265.0
92.00	2038.0
93.00	3339.0
94.00	7815.0
95.00	68280.0
96.00	4610.0
97.10	175.0
103.90	302.0
104.80	103.0
105.90	244.0
115.90	354.0
116.90	477.0
118.00	262.0
118.90	492.0
127.90	252.0
128.90	102.0
129.90	328.0
141.00	815.0
142.90	883.0
144.90	251.0
147.80	150.0
155.00	183.0
157.00	103.0
172.00	605.0
173.00	422.0
174.00	52952.0
175.00	3619.0
176.00	50904.0
177.00	3218.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
43.90	162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
36.00	444.0
37.00	2786.0
38.00	2529.0
39.00	1124.0
44.00	451.0
45.00	547.0
47.00	831.0
48.00	372.0
49.00	2703.0
50.00	12889.0
51.00	3536.0
52.00	191.0
54.90	189.0
56.00	1055.0
57.00	2082.0
60.00	617.0
61.00	3486.0
62.00	3212.0
63.00	2703.0
64.00	385.0
65.00	625.0
67.00	128.0
68.00	6730.0
69.00	6933.0
70.00	455.0
72.00	410.0
73.00	3169.0
74.00	11868.0
75.00	35440.0
76.00	3179.0
77.00	467.0
77.90	200.0
78.90	2391.0
79.90	806.0
80.90	2609.0
82.00	528.0
85.80	113.0
87.00	2957.0
88.00	2678.0
90.90	275.0
92.00	2007.0
93.00	3081.0
94.00	7749.0
95.00	66688.0
96.00	4407.0
97.00	131.0
103.80	255.0
104.80	131.0
105.90	265.0
115.90	294.0
117.00	496.0
117.90	255.0
118.90	463.0
127.90	223.0
129.90	246.0
137.00	102.0
141.00	893.0
142.90	823.0
144.90	283.0
145.90	100.0
147.90	160.0
155.00	181.0
172.00	625.0
173.00	435.0
174.00	48400.0
175.00	3461.0
176.00	47024.0
177.00	3090.0
177.90	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
36.00	482.0
37.00	2886.0
38.00	2578.0
39.00	1127.0
43.90	518.0
45.00	562.0
46.10	147.0
47.00	858.0
48.00	358.0
49.00	2886.0
50.00	13658.0
51.00	3799.0
52.00	228.0
54.90	238.0
56.00	1085.0
57.00	2015.0
60.00	703.0
61.00	3796.0
62.00	3460.0
63.00	2745.0
64.00	426.0
65.00	548.0
67.00	126.0
68.00	7126.0
69.00	7382.0
70.00	471.0
72.00	414.0
73.00	3423.0
74.00	12575.0
75.00	37456.0
76.00	3269.0
77.00	469.0
77.90	188.0
78.90	2571.0
79.90	791.0
80.90	2788.0
81.90	534.0
85.90	136.0
87.00	3234.0
88.00	2844.0
90.90	279.0
92.00	2111.0
93.00	3461.0
94.00	8218.0
95.00	71096.0
96.00	4721.0
97.00	162.0
103.80	311.0
104.80	130.0
105.90	261.0
115.90	347.0
117.00	519.0
117.90	272.0
118.90	521.0
127.90	235.0
129.90	316.0
136.90	100.0
141.00	915.0
142.90	921.0
144.90	286.0
147.80	167.0
155.00	202.0
170.90	109.0
172.00	661.0
173.00	451.0
174.00	52968.0
175.00	3699.0
176.00	51592.0
177.00	3339.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026