

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111622\
 Data File : VU051875.D
 Acq On : 16 Nov 2022 11:31
 Operator : JC/MD
 Sample : VU1116WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK016

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

Signal : TIC: VU051875.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.481	36	44	52	rBV4	10686	19542	1.28%	0.156%
2	1.597	73	80	103	rBV	157979	182303	11.93%	1.459%
3	1.906	167	176	197	rVB	144454	211906	13.86%	1.696%
4	2.565	368	381	398	rBV	226659	372877	24.39%	2.984%
5	2.710	423	426	431	rVB2	499	359	0.02%	0.003%
6	2.752	436	439	442	rVB2	340	231	0.02%	0.002%
7	2.790	445	451	458	rBV3	818	1355	0.09%	0.011%
8	2.848	467	469	473	rVB	396	249	0.02%	0.002%
9	2.880	476	479	482	rBV	311	270	0.02%	0.002%
10	2.960	500	504	506	rBV3	261	218	0.01%	0.002%
11	3.044	517	530	544	rBV2	5706	11023	0.72%	0.088%
12	3.137	556	559	562	rBV2	334	223	0.01%	0.002%
13	3.186	562	574	584	rVB3	1386	3189	0.21%	0.026%
14	3.292	603	607	610	rBV2	307	249	0.02%	0.002%
15	3.362	624	629	630	rBV2	310	220	0.01%	0.002%
16	3.462	657	660	664	rVB3	343	229	0.01%	0.002%
17	3.845	775	779	783	rBV2	236	218	0.01%	0.002%
18	3.867	783	786	793	rVB2	325	365	0.02%	0.003%
19	3.983	818	822	828	rVB2	262	328	0.02%	0.003%
20	4.285	911	916	919	rBV	195	236	0.02%	0.002%
21	4.462	966	971	974	rBV2	230	229	0.01%	0.002%
22	4.523	988	990	996	rVB2	405	443	0.03%	0.004%
23	4.562	996	1002	1007	rBV2	474	696	0.05%	0.006%
24	4.616	1007	1019	1055	rBV	195393	477090	31.21%	3.817%
25	5.060	1140	1157	1181	rVV	300041	664445	43.46%	5.317%
26	5.292	1221	1229	1239	rVB4	1340	2727	0.18%	0.022%
27	5.369	1248	1253	1255	rBV2	684	651	0.04%	0.005%
28	5.497	1287	1293	1295	rBV2	450	467	0.03%	0.004%
29	5.722	1342	1363	1397	rVV2	543321	1528691	100.00%	12.232%
30	6.070	1466	1471	1475	rBV3	311	361	0.02%	0.003%
31	6.247	1511	1526	1558	rBV	587193	1124524	73.56%	8.998%
32	6.488	1597	1601	1604	rBV	421	345	0.02%	0.003%
33	6.529	1605	1614	1625	rVV6	3364	5675	0.37%	0.045%
34	6.687	1648	1663	1694	rBV	385610	763137	49.92%	6.106%
35	6.838	1708	1710	1714	rVB2	353	221	0.01%	0.002%
36	6.896	1723	1728	1731	rBV3	370	352	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111622\
 Data File : VU051875.D
 Acq On : 16 Nov 2022 11:31
 Operator : JC/MD
 Sample : VU1116WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK016

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

37	6.986	1752	1756	1762	rBV2	405	409	0.03%	0.003%
38	7.018	1762	1766	1769	rBV2	233	227	0.01%	0.002%
39	7.182	1810	1817	1832	rBV5	6559	11923	0.78%	0.095%
40	7.410	1884	1888	1891	rBV2	295	249	0.02%	0.002%
41	7.517	1914	1921	1923	rBV2	347	446	0.03%	0.004%
42	7.562	1923	1935	1955	rVV	171480	305459	19.98%	2.444%
43	7.648	1959	1962	1965	rVV2	628	463	0.03%	0.004%
44	7.693	1967	1976	1990	rVB4	3928	7512	0.49%	0.060%
45	7.800	2005	2009	2011	rBV2	406	318	0.02%	0.003%
46	7.896	2026	2039	2057	rBV	567505	972439	63.61%	7.781%
47	8.044	2082	2085	2086	rBV2	378	231	0.02%	0.002%
48	8.176	2115	2126	2144	rBV	120887	206661	13.52%	1.654%
49	8.282	2155	2159	2161	rBV3	340	248	0.02%	0.002%
50	8.439	2205	2208	2211	rBV2	338	272	0.02%	0.002%
51	8.500	2223	2227	2228	rBV2	379	272	0.02%	0.002%
52	8.552	2237	2243	2251	rVB5	2546	3421	0.22%	0.027%
53	8.629	2255	2267	2305	rBV2	552370	1041076	68.10%	8.330%
54	8.838	2330	2332	2335	rVB	422	228	0.01%	0.002%
55	9.044	2393	2396	2404	rVB2	598	773	0.05%	0.006%
56	9.076	2404	2406	2411	rVB2	418	324	0.02%	0.003%
57	9.108	2411	2416	2417	rBV2	395	324	0.02%	0.003%
58	9.163	2429	2433	2439	rVB3	432	389	0.03%	0.003%
59	9.369	2493	2497	2498	rBV	429	296	0.02%	0.002%
60	9.414	2498	2511	2541	rVV	845070	1389245	90.88%	11.116%
61	9.642	2579	2582	2587	rVB4	473	471	0.03%	0.004%
62	9.690	2593	2597	2599	rBV2	575	432	0.03%	0.003%
63	10.012	2694	2697	2703	rVB2	363	355	0.02%	0.003%
64	10.108	2724	2727	2728	rBV2	369	235	0.02%	0.002%
65	10.282	2778	2781	2787	rVB2	332	317	0.02%	0.003%
66	10.404	2817	2819	2825	rVB2	254	221	0.01%	0.002%
67	10.488	2836	2845	2849	rVB2	502	641	0.04%	0.005%
68	10.754	2914	2928	2949	rBV	661104	1072616	70.17%	8.582%
69	10.870	2961	2964	2967	rBV	442	340	0.02%	0.003%
70	10.954	2987	2990	2995	rVB2	513	371	0.02%	0.003%
71	11.153	3048	3052	3057	rBV	540	663	0.04%	0.005%
72	11.317	3100	3103	3106	rVV	329	232	0.02%	0.002%
73	11.407	3128	3131	3134	rVB3	597	335	0.02%	0.003%
74	11.449	3140	3144	3146	rBV2	363	310	0.02%	0.002%
75	11.465	3146	3149	3155	rVB2	477	494	0.03%	0.004%
76	11.533	3164	3170	3172	rBV2	309	304	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111622\
 Data File : VU051875.D
 Acq On : 16 Nov 2022 11:31
 Operator : JC/MD
 Sample : VU1116WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK016

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

77	11.748	3234	3237	3240	rVB	630	431	0.03%	0.003%
78	11.809	3243	3256	3283	rBV	636487	1038287	67.92%	8.308%
79	12.024	3320	3323	3324	rBV2	404	235	0.02%	0.002%
80	12.066	3334	3336	3341	rVB2	649	462	0.03%	0.004%
81	12.188	3360	3374	3394	rBV	627707	1053854	68.94%	8.432%
82	12.439	3449	3452	3457	rBV2	349	333	0.02%	0.003%
83	12.500	3469	3471	3473	rVV	551	249	0.02%	0.002%
84	12.523	3476	3478	3483	rVB2	369	264	0.02%	0.002%
85	12.632	3508	3512	3514	rBV2	343	270	0.02%	0.002%
86	12.825	3569	3572	3574	rBV	340	245	0.02%	0.002%
87	12.899	3592	3595	3597	rBV2	410	304	0.02%	0.002%
88	12.938	3603	3607	3610	rVB2	464	329	0.02%	0.003%
89	13.008	3627	3629	3632	rVB2	516	290	0.02%	0.002%
90	13.201	3686	3689	3692	rBV2	477	390	0.03%	0.003%
91	13.381	3742	3745	3748	rBV2	320	235	0.02%	0.002%
92	13.491	3776	3779	3782	rVB2	360	216	0.01%	0.002%
93	13.687	3837	3840	3842	rBV	407	276	0.02%	0.002%
94	13.848	3885	3890	3892	rBV3	1106	1056	0.07%	0.008%
95	13.960	3920	3925	3930	rBV3	757	923	0.06%	0.007%
96	14.272	4019	4022	4025	rVB3	415	242	0.02%	0.002%
97	14.426	4066	4070	4072	rBV	627	520	0.03%	0.004%
98	14.671	4143	4146	4149	rBV2	562	341	0.02%	0.003%
99	14.954	4231	4234	4235	rBV	483	316	0.02%	0.003%
100	15.481	4396	4398	4403	rVB4	700	461	0.03%	0.004%




Sum of corrected areas: 12497715

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111622\
Data File : VU051875.D
Acq On : 16 Nov 2022 11:31
Operator : JC/MD
Sample : VU1116WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK016

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

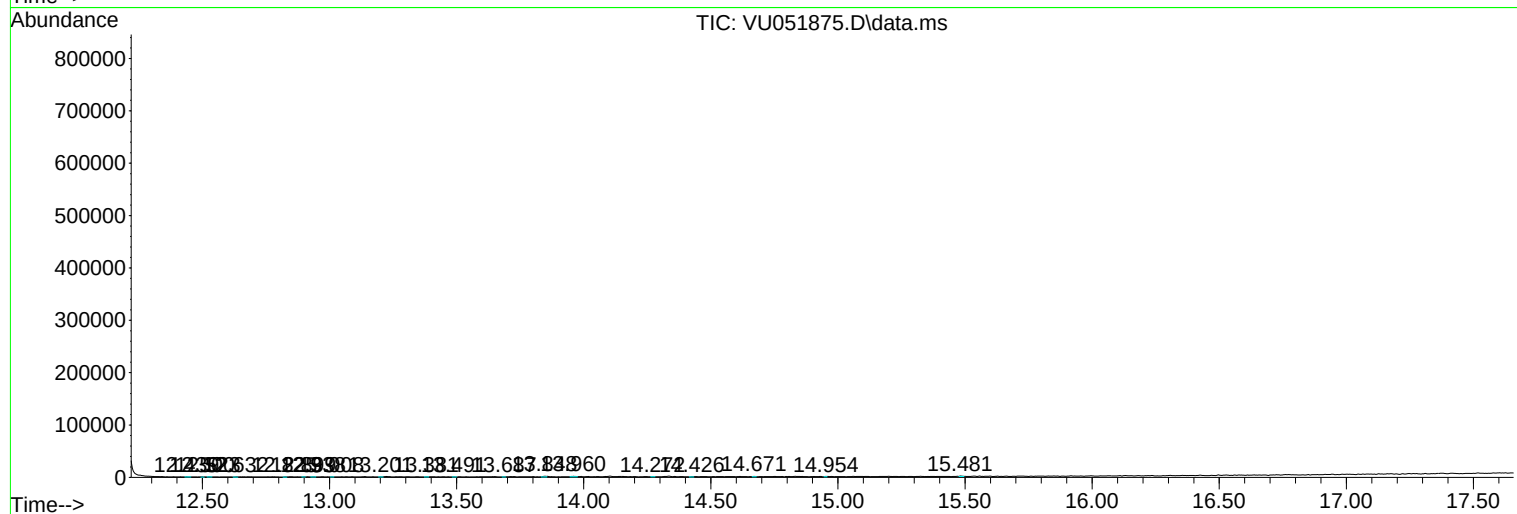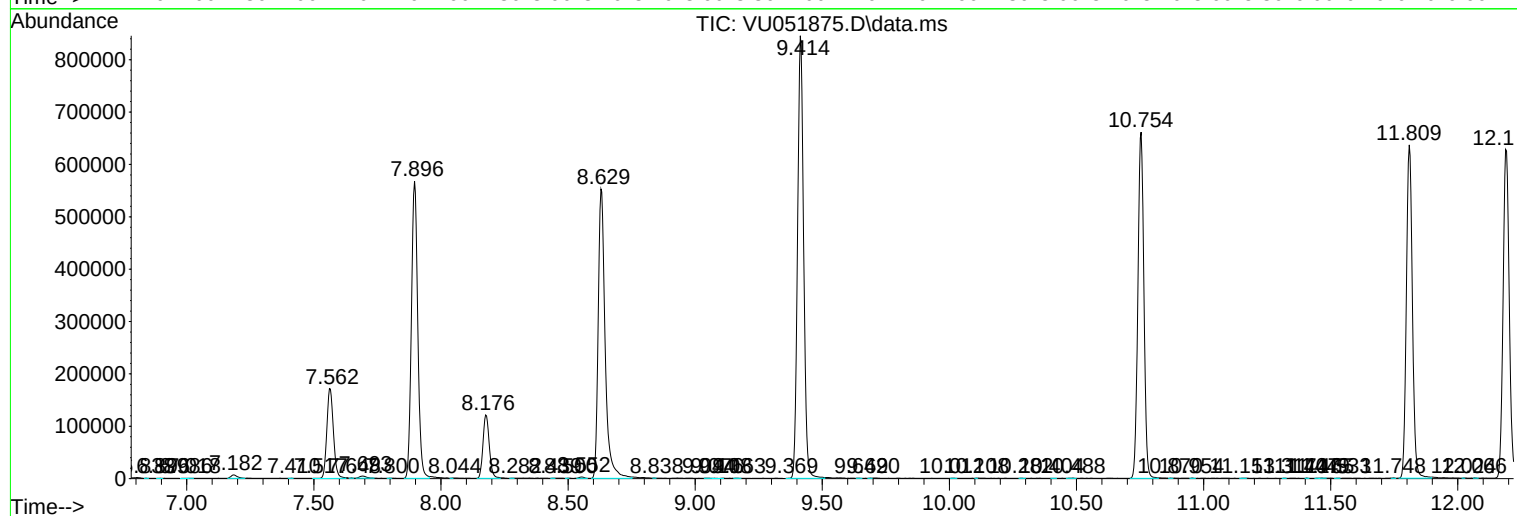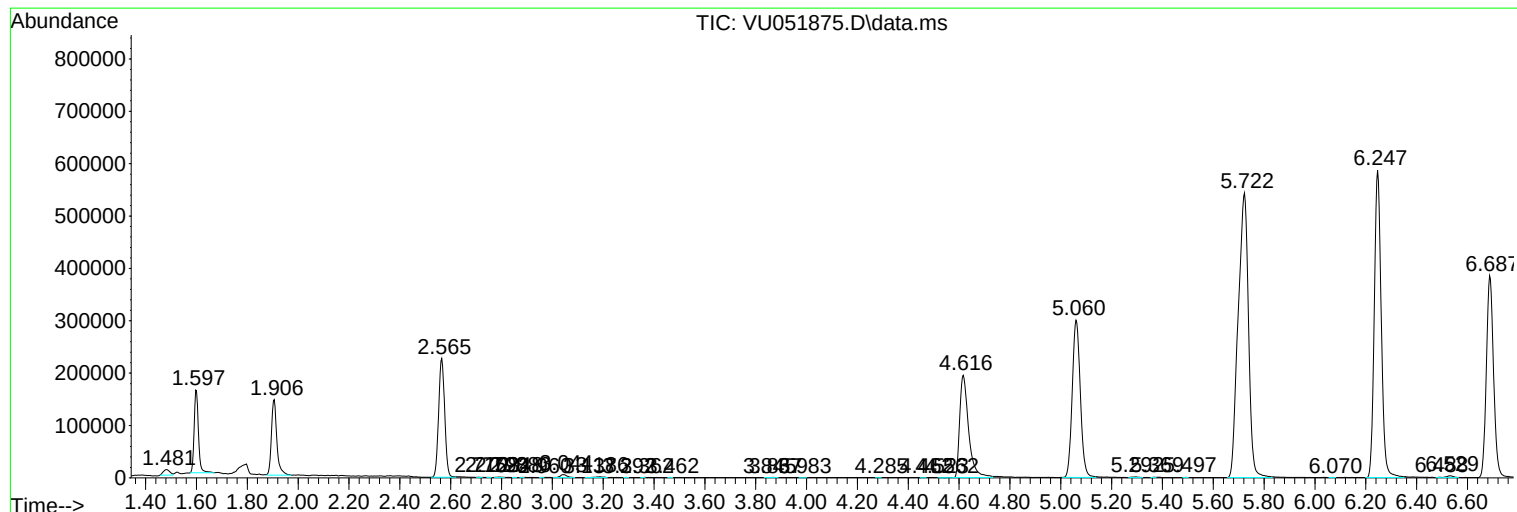

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111622\
Data File : VU051875.D
Acq On : 16 Nov 2022 11:31
Operator : JC/MD
Sample : VU1116WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK016

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111622\
Data File : VU051875.D
Acq On : 16 Nov 2022 11:31
Operator : JC/MD
Sample : VU1116WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK016

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc