

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111622\
 Data File : VU051876.D
 Acq On : 16 Nov 2022 11:55
 Operator : JC/MD
 Sample : VU1116WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK017

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

Signal : TIC: VU051876.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.481	35	44	52	rBV3	12367	22785	1.49%	0.180%
2	1.597	73	80	92	rBV	159329	178585	11.70%	1.411%
3	1.906	167	176	196	rVB	144547	209496	13.72%	1.655%
4	2.565	368	381	396	rBV	232044	378996	24.83%	2.995%
5	2.761	440	442	446	rBV3	329	225	0.01%	0.002%
6	2.787	446	450	457	rVB2	708	860	0.06%	0.007%
7	3.009	515	519	520	rBV	359	240	0.02%	0.002%
8	3.044	520	530	542	rVB3	5726	11505	0.75%	0.091%
9	3.186	562	574	588	rVB	3052	6453	0.42%	0.051%
10	3.330	616	619	623	rVB2	382	216	0.01%	0.002%
11	3.452	654	657	660	rVV	337	244	0.02%	0.002%
12	3.555	686	689	695	rVV2	403	345	0.02%	0.003%
13	3.780	756	759	763	rBV	282	205	0.01%	0.002%
14	3.848	777	780	785	rVB2	479	382	0.03%	0.003%
15	3.999	824	827	832	rBV2	297	257	0.02%	0.002%
16	4.266	907	910	916	rVB2	247	226	0.01%	0.002%
17	4.314	921	925	928	rVB2	325	273	0.02%	0.002%
18	4.333	928	931	936	rBV2	285	243	0.02%	0.002%
19	4.616	1007	1019	1048	rBV	202061	483686	31.69%	3.822%
20	4.919	1110	1113	1116	rBV2	308	225	0.01%	0.002%
21	5.060	1138	1157	1182	rBV	303407	664622	43.54%	5.252%
22	5.205	1200	1202	1208	rVB5	442	418	0.03%	0.003%
23	5.337	1239	1243	1248	rBV2	452	369	0.02%	0.003%
24	5.366	1248	1252	1253	rBV	647	508	0.03%	0.004%
25	5.456	1273	1280	1282	rBV3	264	239	0.02%	0.002%
26	5.722	1342	1363	1385	rBV2	542080	1526530	100.00%	12.063%
27	5.902	1417	1419	1427	rVB2	467	329	0.02%	0.003%
28	6.002	1446	1450	1451	rBV2	389	294	0.02%	0.002%
29	6.012	1451	1453	1457	rVB2	249	215	0.01%	0.002%
30	6.115	1480	1485	1487	rBV3	333	316	0.02%	0.002%
31	6.179	1502	1505	1510	rVB2	331	268	0.02%	0.002%
32	6.247	1510	1526	1549	rBV	594938	1134952	74.35%	8.968%
33	6.427	1579	1582	1589	rVB3	565	430	0.03%	0.003%
34	6.529	1604	1614	1624	rVV4	2767	4788	0.31%	0.038%
35	6.687	1647	1663	1691	rBV	389384	767395	50.27%	6.064%
36	6.809	1698	1701	1705	rVB4	676	601	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111622\
 Data File : VU051876.D
 Acq On : 16 Nov 2022 11:55
 Operator : JC/MD
 Sample : VU1116WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK017

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

37	6.845	1710	1712	1716	rVB2	357	217	0.01%	0.002%
38	6.976	1746	1753	1759	rBV2	436	556	0.04%	0.004%
39	7.185	1810	1818	1832	rBV2	6474	11684	0.77%	0.092%
40	7.320	1854	1860	1863	rVB2	232	218	0.01%	0.002%
41	7.484	1909	1911	1915	rVB	332	242	0.02%	0.002%
42	7.517	1915	1921	1923	rBV2	268	271	0.02%	0.002%
43	7.562	1923	1935	1959	rBV	173297	308468	20.21%	2.438%
44	7.690	1967	1975	1983	rBV2	3917	6288	0.41%	0.050%
45	7.800	2005	2009	2010	rBV	495	220	0.01%	0.002%
46	7.896	2026	2039	2064	rVV	568645	977798	64.05%	7.727%
47	8.176	2115	2126	2147	rBV	120990	206981	13.56%	1.636%
48	8.317	2167	2170	2173	rBV2	349	230	0.02%	0.002%
49	8.340	2173	2177	2183	rVB2	548	454	0.03%	0.004%
50	8.427	2200	2204	2208	rVB4	328	354	0.02%	0.003%
51	8.465	2213	2216	2219	rVV3	543	391	0.03%	0.003%
52	8.545	2237	2241	2250	rVB4	1827	2408	0.16%	0.019%
53	8.629	2255	2267	2301	rBV	577139	1062860	69.63%	8.399%
54	8.845	2332	2334	2337	rVB3	386	215	0.01%	0.002%
55	8.899	2346	2351	2354	rBV	421	441	0.03%	0.003%
56	8.996	2378	2381	2383	rBV	523	328	0.02%	0.003%
57	9.082	2406	2408	2412	rVB	310	223	0.01%	0.002%
58	9.118	2414	2419	2425	rVB2	527	575	0.04%	0.005%
59	9.153	2425	2430	2432	rBV2	274	303	0.02%	0.002%
60	9.234	2447	2455	2460	rBV2	522	595	0.04%	0.005%
61	9.333	2483	2486	2488	rBV	351	220	0.01%	0.002%
62	9.414	2497	2511	2534	rBV	866899	1404581	92.01%	11.099%
63	9.616	2571	2574	2579	rVB3	479	317	0.02%	0.003%
64	9.697	2596	2599	2602	rVV2	506	371	0.02%	0.003%
65	9.751	2613	2616	2619	rBV2	428	278	0.02%	0.002%
66	9.909	2659	2665	2667	rBV2	367	376	0.02%	0.003%
67	10.053	2707	2710	2715	rBV2	237	268	0.02%	0.002%
68	10.108	2724	2727	2730	rBV3	418	274	0.02%	0.002%
69	10.147	2733	2739	2741	rBV2	237	258	0.02%	0.002%
70	10.185	2748	2751	2755	rBV2	367	284	0.02%	0.002%
71	10.275	2776	2779	2784	rVB2	269	214	0.01%	0.002%
72	10.301	2784	2787	2795	rBV2	238	309	0.02%	0.002%
73	10.536	2857	2860	2863	rVV	246	210	0.01%	0.002%
74	10.751	2913	2927	2952	rBV	684397	1096221	71.81%	8.662%
75	10.963	2989	2993	2997	rBV2	252	248	0.02%	0.002%
76	11.108	3035	3038	3041	rVV2	360	210	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111622\
 Data File : VU051876.D
 Acq On : 16 Nov 2022 11:55
 Operator : JC/MD
 Sample : VU1116WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK017

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

77	11.143	3046	3049	3053	rVB3	406	295	0.02%	0.002%
78	11.420	3133	3135	3140	rVB2	488	371	0.02%	0.003%
79	11.465	3146	3149	3156	rVB3	378	426	0.03%	0.003%
80	11.497	3156	3159	3164	rVB	257	215	0.01%	0.002%
81	11.632	3198	3201	3205	rVB	329	215	0.01%	0.002%
82	11.709	3221	3225	3228	rVB2	336	254	0.02%	0.002%
83	11.741	3233	3235	3241	rBV3	601	549	0.04%	0.004%
84	11.809	3243	3256	3279	rBV	670225	1073337	70.31%	8.482%
85	12.137	3356	3358	3361	rBV	306	245	0.02%	0.002%
86	12.192	3361	3375	3400	rVV	661068	1087865	71.26%	8.596%
87	12.378	3429	3433	3436	rBV3	519	507	0.03%	0.004%
88	12.655	3516	3519	3526	rVV	332	248	0.02%	0.002%
89	12.687	3526	3529	3535	rVV2	372	378	0.02%	0.003%
90	13.031	3631	3636	3638	rBV	412	356	0.02%	0.003%
91	13.198	3685	3688	3693	rBV2	407	464	0.03%	0.004%
92	13.221	3693	3695	3703	rVB4	626	595	0.04%	0.005%
93	13.349	3732	3735	3738	rBV	555	332	0.02%	0.003%
94	13.844	3887	3889	3892	rBV3	490	304	0.02%	0.002%
95	14.098	3964	3968	3970	rBV3	613	414	0.03%	0.003%
96	14.333	4035	4041	4042	rBV2	793	802	0.05%	0.006%
97	14.838	4195	4198	4202	rBV2	603	600	0.04%	0.005%
98	14.966	4236	4238	4241	rBV2	529	288	0.02%	0.002%
99	14.999	4245	4248	4253	rBV3	610	639	0.04%	0.005%
100	15.635	4443	4446	4449	rVB2	859	548	0.04%	0.004%




Sum of corrected areas: 12654927

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111622\
Data File : VU051876.D
Acq On : 16 Nov 2022 11:55
Operator : JC/MD
Sample : VU1116WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK017

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

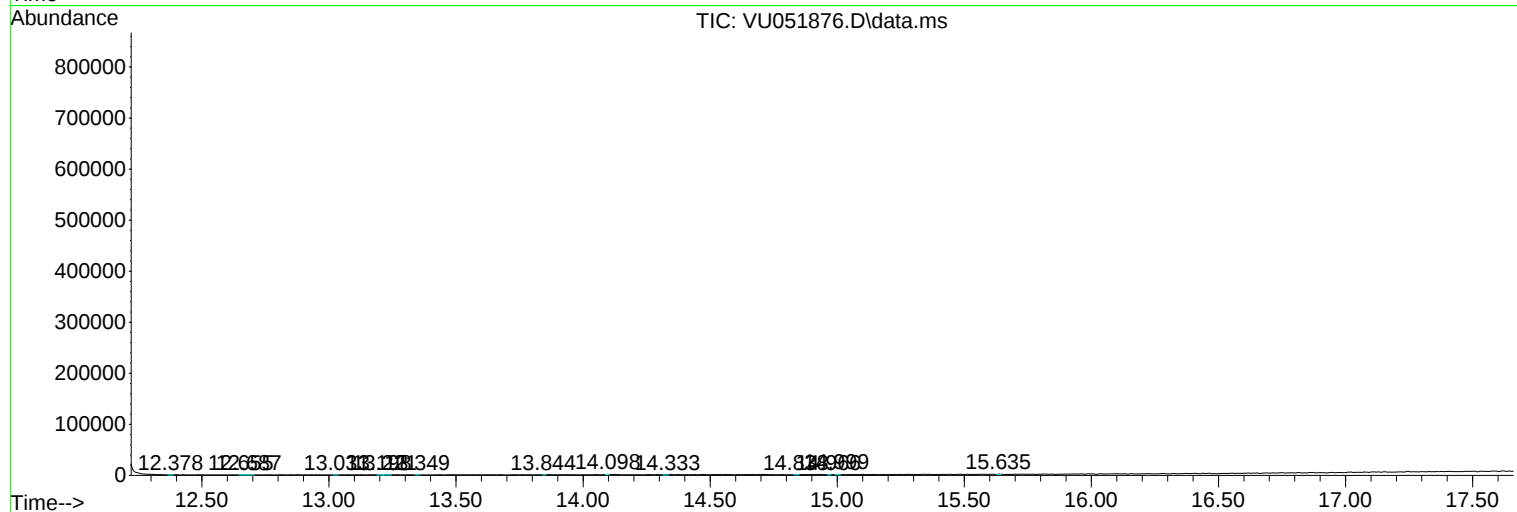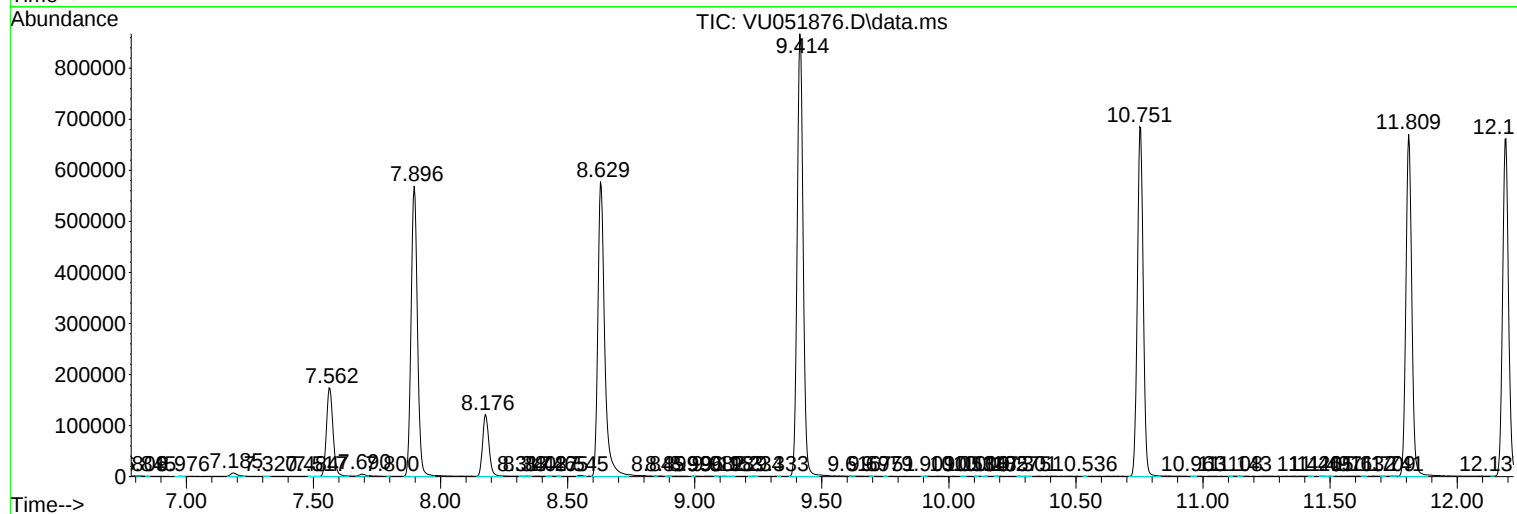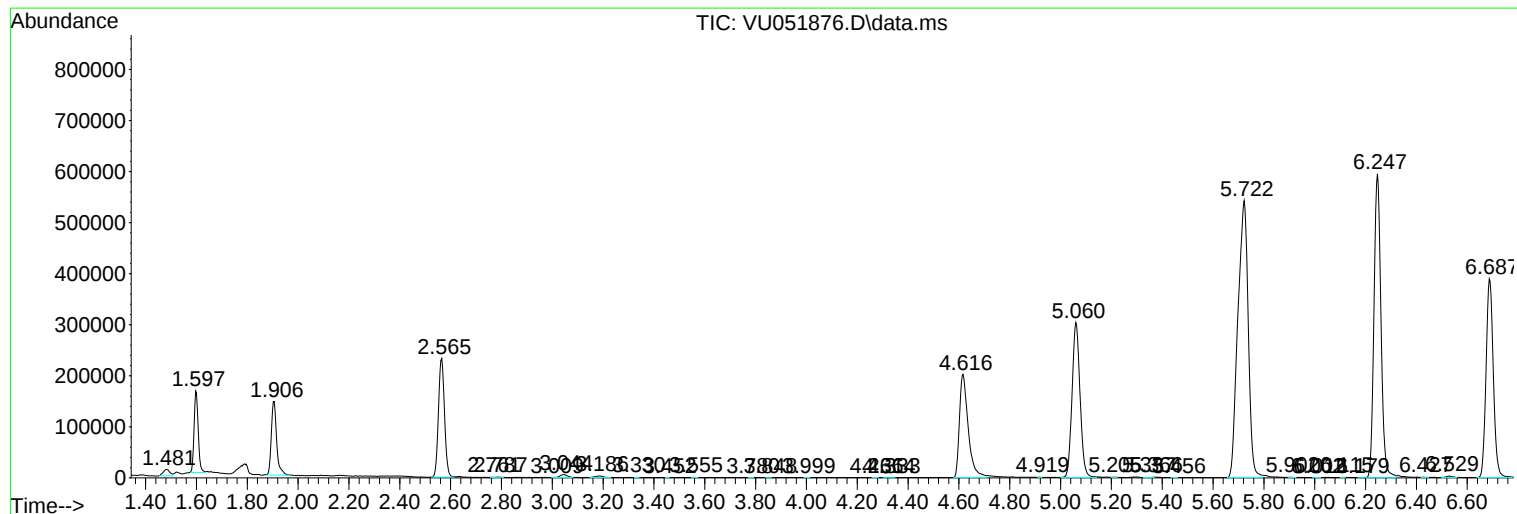

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111622\
Data File : VU051876.D
Acq On : 16 Nov 2022 11:55
Operator : JC/MD
Sample : VU1116WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK017

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111622\
Data File : VU051876.D
Acq On : 16 Nov 2022 11:55
Operator : JC/MD
Sample : VU1116WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK017

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------