


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111622\
Data File : VU051870.D
Acq On : 16 Nov 2022 09:24
Operator : JC/MD
Sample : BFB143
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB143

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Title : VOC Analysis
Last Update : Thu Nov 17 01:20:24 2022

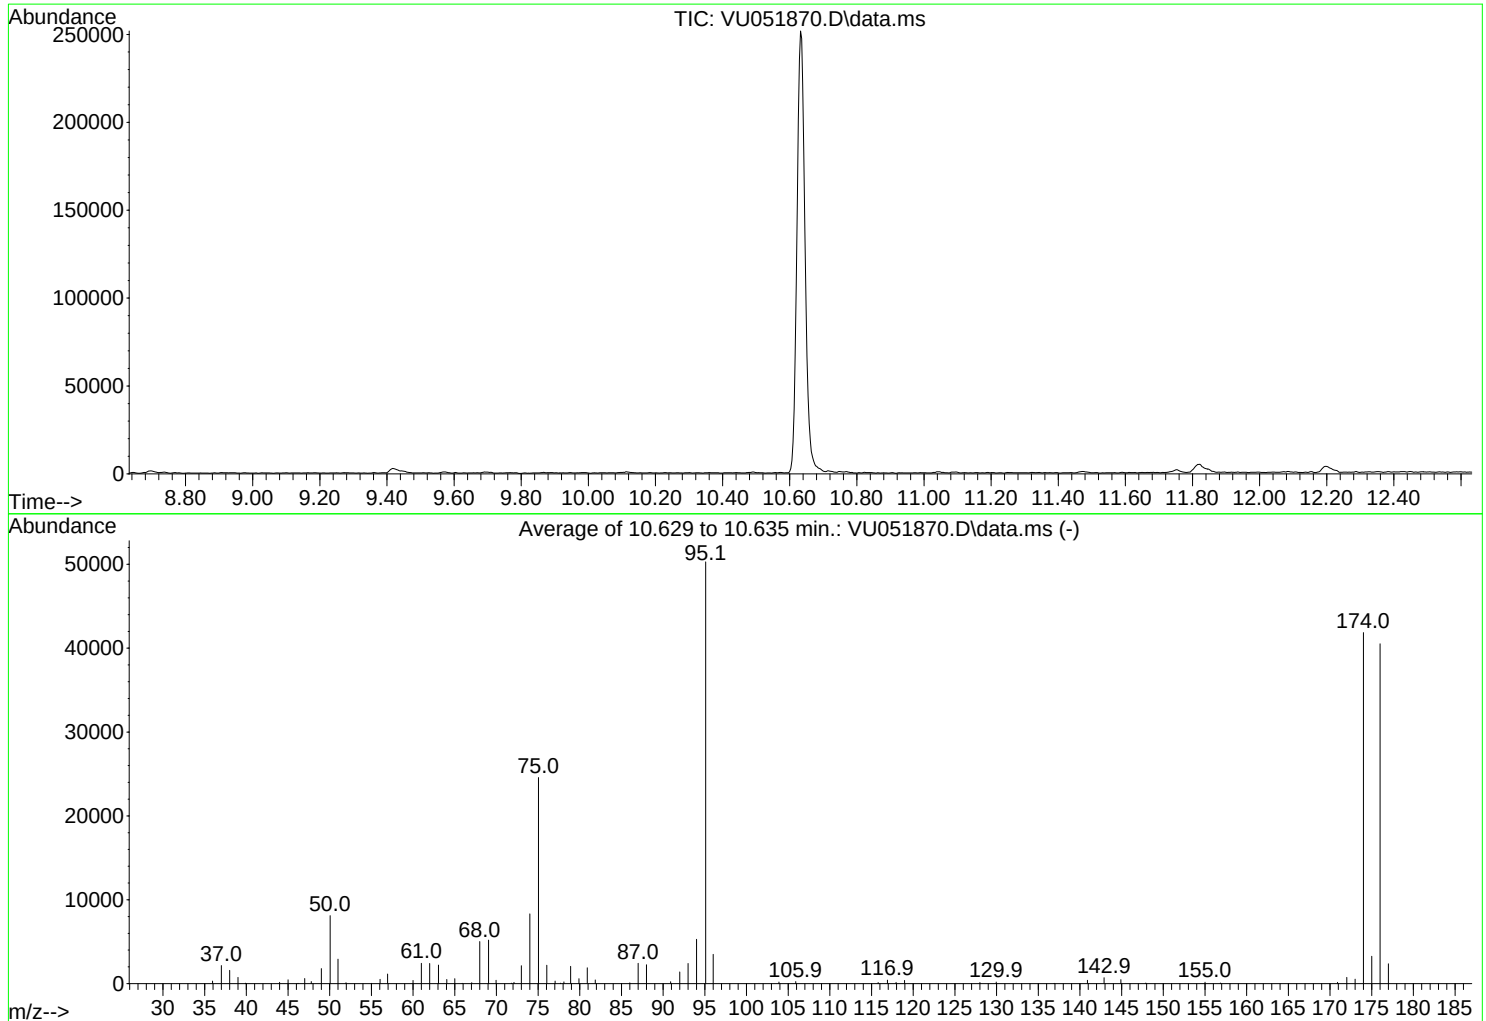

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.1	8118	PASS
75	95	30	80	48.9	24579	PASS
95	95	100	100	100.0	50293	PASS
96	95	5	9	6.9	3487	PASS
173	174	0.00	2	1.3	544	PASS
174	95	50	120	83.2	41856	PASS
175	174	5	9	7.8	3270	PASS
176	174	95	101	96.8	40520	PASS
177	176	5	9	5.8	2359	PASS

Scan 2878 (10.594 min): VU051870.D\data.ms
BFB143

m/z	Abundance
39.90	168.0
44.00	481.0

Instrument :
MSVOA_U
ClientSampleId :
BFB143

m/z	Abundance
36.00	317.0
37.00	2208.0
38.00	1580.0
39.00	746.0
39.90	265.0
44.00	698.0
45.00	407.0
47.00	611.0
47.80	261.0
49.00	1785.0
50.00	7787.0
51.00	2873.0
52.00	119.0
55.00	111.0
56.10	568.0
56.90	1194.0
59.90	372.0
61.00	2362.0
62.00	2414.0
63.00	2275.0
64.00	485.0
65.00	586.0
67.10	114.0
68.00	4903.0
69.00	5040.0
70.00	458.0
71.80	166.0
73.00	2200.0
74.00	8243.0
75.00	23976.0
76.00	2063.0
77.00	322.0
77.70	201.0
78.10	202.0
78.90	2056.0
79.90	564.0
80.90	1840.0
81.80	360.0
87.00	2459.0
88.00	2225.0
90.90	233.0
92.00	1414.0
93.00	2463.0
94.00	5221.0
95.10	48128.0
96.00	3369.0
103.80	170.0
105.90	287.0
115.80	146.0
116.90	388.0
118.00	152.0
119.00	364.0
127.90	121.0
129.90	215.0
140.90	381.0
142.90	693.0
144.90	471.0
155.00	167.0
156.80	105.0
170.80	147.0
172.00	657.0
173.00	621.0
174.00	38960.0
175.00	2967.0
176.00	38128.0
177.00	2314.0

Instrument :
MSVOA_U
ClientSampleId :
BFB143

m/z	Abundance
36.00	304.0
37.00	2217.0
38.00	1569.0
39.00	782.0
39.90	222.0
44.00	647.0
45.00	456.0
46.20	103.0
47.00	638.0
47.80	273.0
49.00	1852.0
50.10	8375.0
51.00	3001.0
51.90	123.0
56.10	549.0
56.90	1166.0
60.00	377.0
61.00	2492.0
62.00	2451.0
63.00	2304.0
64.00	533.0
65.00	596.0
67.10	127.0
68.00	5116.0
69.10	5389.0
69.90	433.0
72.10	209.0
73.00	2212.0
74.00	8595.0
75.10	25272.0
76.00	2294.0
77.00	313.0
78.10	224.0
78.90	2113.0
79.90	603.0
80.90	1923.0
81.80	474.0
86.00	128.0
87.00	2463.0
88.00	2326.0
90.90	230.0
92.00	1420.0
93.00	2525.0
94.00	5342.0
95.10	51824.0
96.00	3590.0
103.90	197.0
105.90	275.0
115.80	132.0
116.90	451.0
118.00	143.0
119.00	386.0
128.00	132.0
130.00	191.0
140.90	407.0
142.90	720.0
144.90	490.0
147.90	112.0
155.00	180.0
156.90	105.0
170.90	146.0
172.00	770.0
173.00	551.0
174.00	42872.0
175.00	3441.0
176.00	41592.0
177.00	2436.0

Instrument :
MSVOA_U
ClientSampleId :
BFB143

m/z	Abundance
35.90	317.0
37.00	2019.0
38.00	1614.0
39.00	735.0
39.90	185.0
44.00	586.0
45.00	505.0
47.00	565.0
47.80	240.0
49.00	1768.0
50.10	8191.0
51.00	2863.0
51.90	121.0
56.00	458.0
57.00	1063.0
60.10	387.0
61.00	2419.0
62.00	2339.0
63.10	2091.0
64.10	501.0
65.00	570.0
65.90	125.0
67.00	125.0
68.00	5024.0
69.00	5132.0
70.00	330.0
72.10	252.0
73.00	2022.0
74.00	8146.0
75.10	24488.0
76.10	2240.0
77.10	303.0
78.10	193.0
78.90	2036.0
79.90	605.0
80.90	1933.0
81.90	509.0
86.00	151.0
87.00	2337.0
88.00	2214.0
90.90	198.0
92.00	1362.0
93.00	2245.0
94.00	5297.0
95.10	50928.0
96.00	3502.0
104.00	217.0
105.90	212.0
115.80	106.0
116.90	447.0
117.90	138.0
118.90	401.0
128.10	133.0
129.90	161.0
136.90	114.0
140.90	394.0
142.90	691.0
144.90	460.0
147.90	107.0
155.00	144.0
171.00	156.0
172.00	794.0
173.00	460.0
174.00	43736.0
175.00	3401.0
176.00	41840.0
177.00	2326.0

Instrument :
MSVOA_U
ClientSampleId :
BFB143