

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111623\
 Data File : VU056407.D
 Acq On : 16 Nov 2023 15:07
 Operator : MD/SY
 Sample : 05373-01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDM7

Quant Time: Nov 17 01:38:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 17 01:31:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	291445	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	288701	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	115856	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	85124	3.905	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.000%
7) Chloroethane-d5	1.907	69	79963	4.784	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.600%
11) 1,1-Dichloroethene-d2	2.560	65	40787	4.240	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.800%
20) 2-Butanone-d5	4.615	46	220529	50.734	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.460%
24) Chloroform-d	5.055	84	198346	4.704	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.000%
26) 1,2-Dichloroethane-d4	5.695	65	102761	5.274	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.400%
32) Benzene-d6	5.721	84	396202	4.606	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.200%
36) 1,2-Dichloropropane-d6	6.685	67	123912	4.780	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.600%
41) Toluene-d8	7.894	98	332391	4.376	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.600%
43) trans-1,3-Dichloroprop...	8.177	79	43543	4.379	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.600%
46) 2-Hexanone-d5	8.627	63	186362	47.697	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.400%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	81653	4.408	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.200%
66) 1,2-Dichlorobenzene-d4	12.190	152	110164	5.147	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.000%
Target Compounds					Qvalue	
25) Chloroform	5.084	83	31953	0.811	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111623\
Data File : VU056407.D
Acq On : 16 Nov 2023 15:07
Operator : MD/SY
Sample : 05373-01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCDM7

Quant Time: Nov 17 01:38:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 17 01:31:28 2023
Response via : Initial Calibration

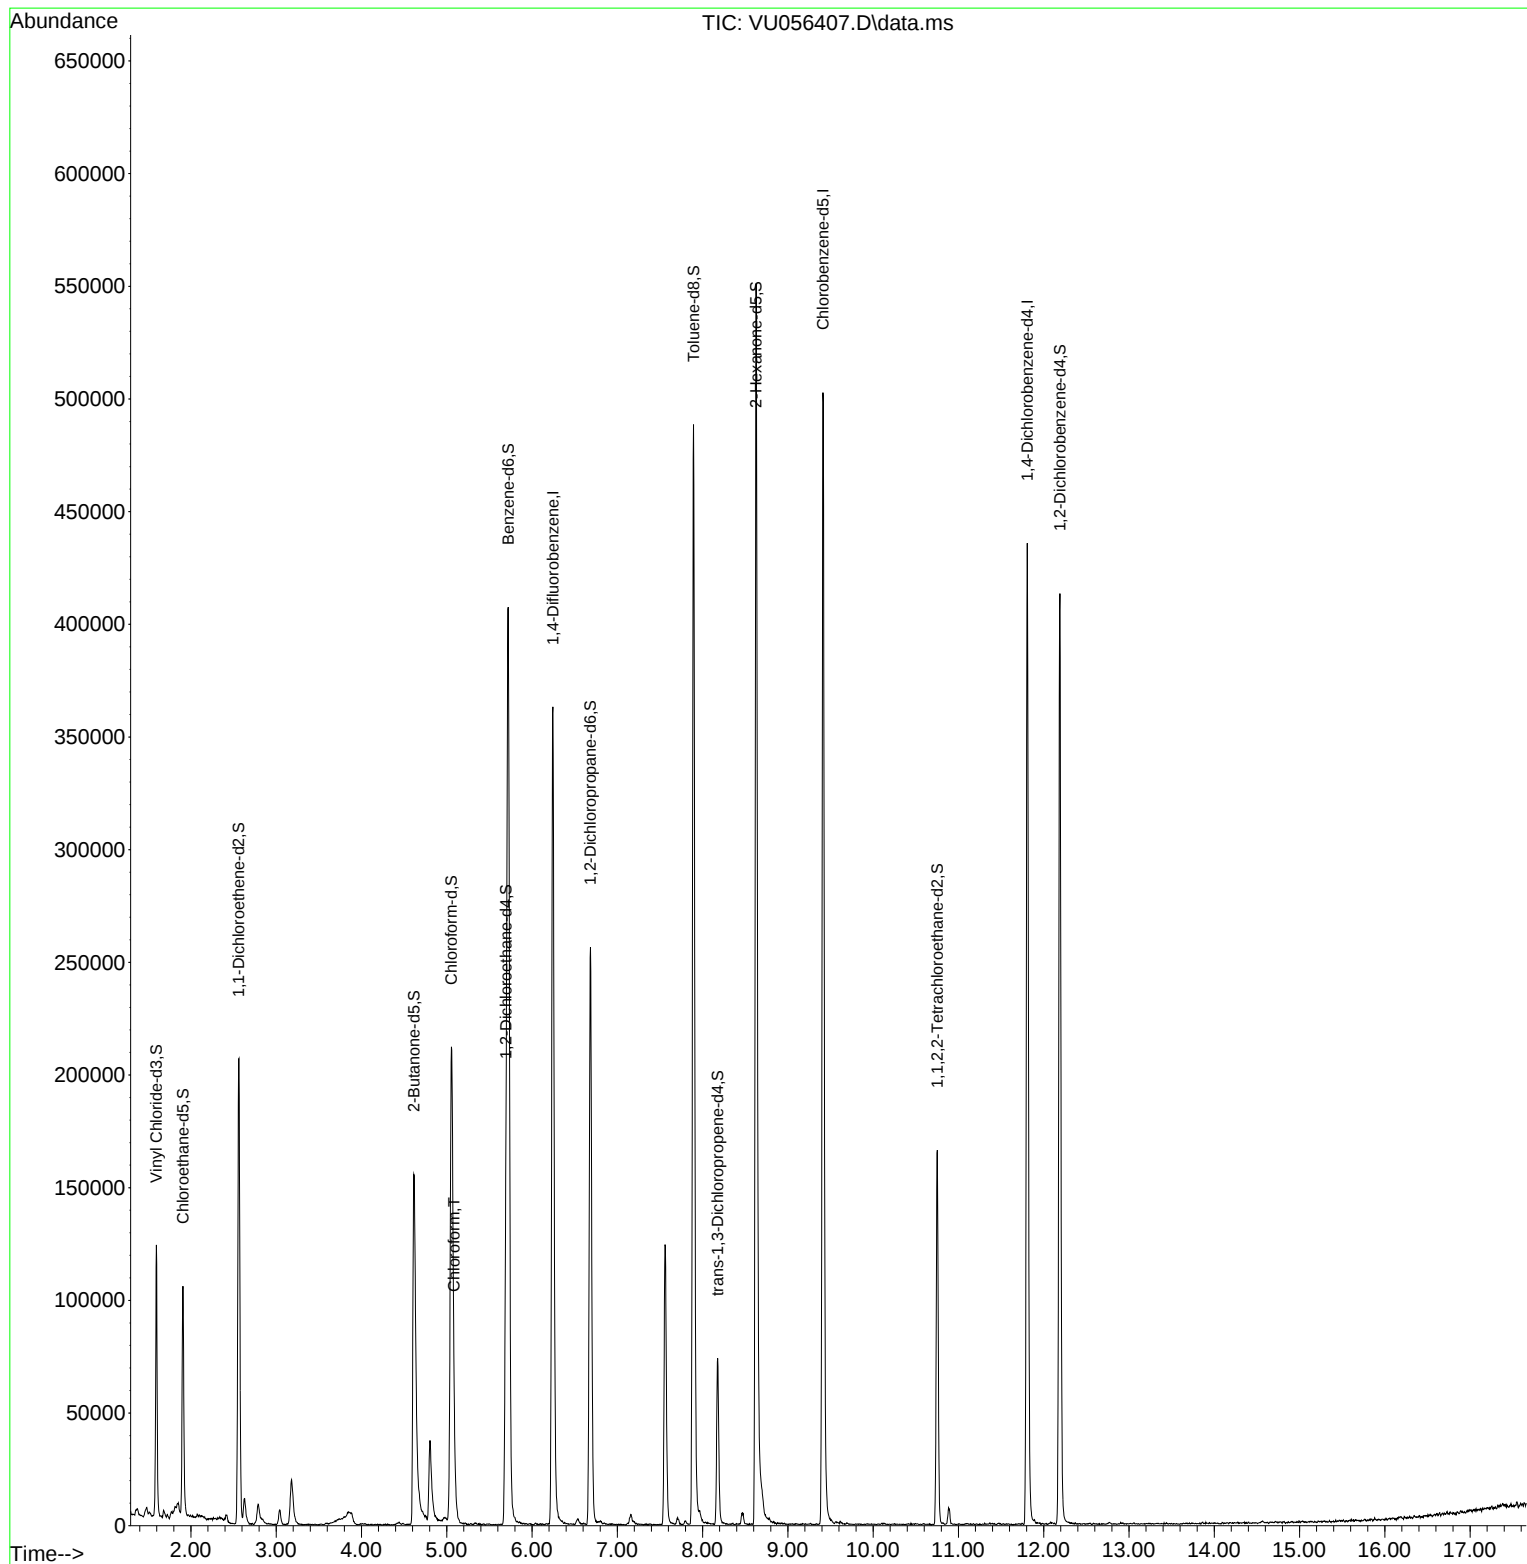

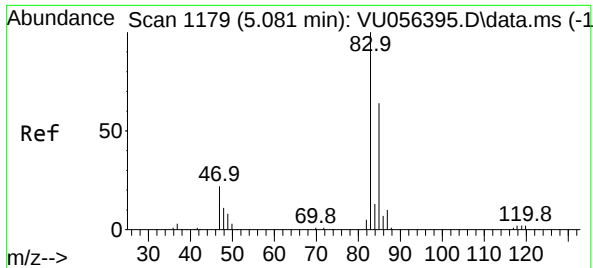

#25
 Chloroform
 Concen: 0.811 ug/L
 RT: 5.084 min Scan# 11
 Delta R.T. 0.003 min
 Lab File: VU056407.D
 Acq: 16 Nov 2023 15:07

Instrument :
 MSVOA_U
 ClientSampleId :
 GCDM7

Tgt Ion: 83 Resp: 31953
 Ion Ratio Lower Upper
 83 100
 85 63.5 47.0 87.2

