

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111623\
 Data File : VU056396.D
 Acq On : 16 Nov 2023 10:15
 Operator : MD/SY
 Sample : VU1116WBL01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK075

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056396.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	106	rVB	124447	143890	14.49%	1.707%
2	1.907	184	192	208	rVB	96838	135459	13.64%	1.607%
3	2.563	382	396	413	rBV	209072	346736	34.91%	4.114%
4	3.042	534	545	559	rVB3	8848	17309	1.74%	0.205%
5	3.181	573	588	607	rBV2	21922	54237	5.46%	0.644%
6	4.621	1019	1036	1077	rBV	140932	399764	40.25%	4.744%
7	5.058	1156	1172	1195	rBV	197245	448494	45.15%	5.322%
8	5.721	1354	1378	1410	rBV3	383199	993280	100.00%	11.786%
9	6.245	1528	1541	1575	rBV	352979	699318	70.40%	8.298%
10	6.685	1665	1678	1710	rBV	236947	471177	47.44%	5.591%
11	7.563	1935	1951	1976	rBV	112854	209864	21.13%	2.490%
12	7.894	2036	2054	2084	rBV	453153	808242	81.37%	9.591%
13	8.177	2131	2142	2160	rBV2	69577	122133	12.30%	1.449%
14	8.631	2271	2283	2314	rBV	494562	940563	94.69%	11.161%
15	9.412	2513	2526	2552	rBV	497971	879755	88.57%	10.439%
16	10.753	2931	2943	2958	rBV	171351	275104	27.70%	3.264%
17	10.891	2977	2986	2994	rVB3	7172	10513	1.06%	0.125%
18	11.807	3259	3271	3293	rBV	474285	786346	79.17%	9.331%
19	12.190	3373	3390	3418	rBV	402199	685253	68.99%	8.131%




Sum of corrected areas: 8427437

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111623\
Data File : VU056396.D
Acq On : 16 Nov 2023 10:15
Operator : MD/SY
Sample : VU1116WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK075

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

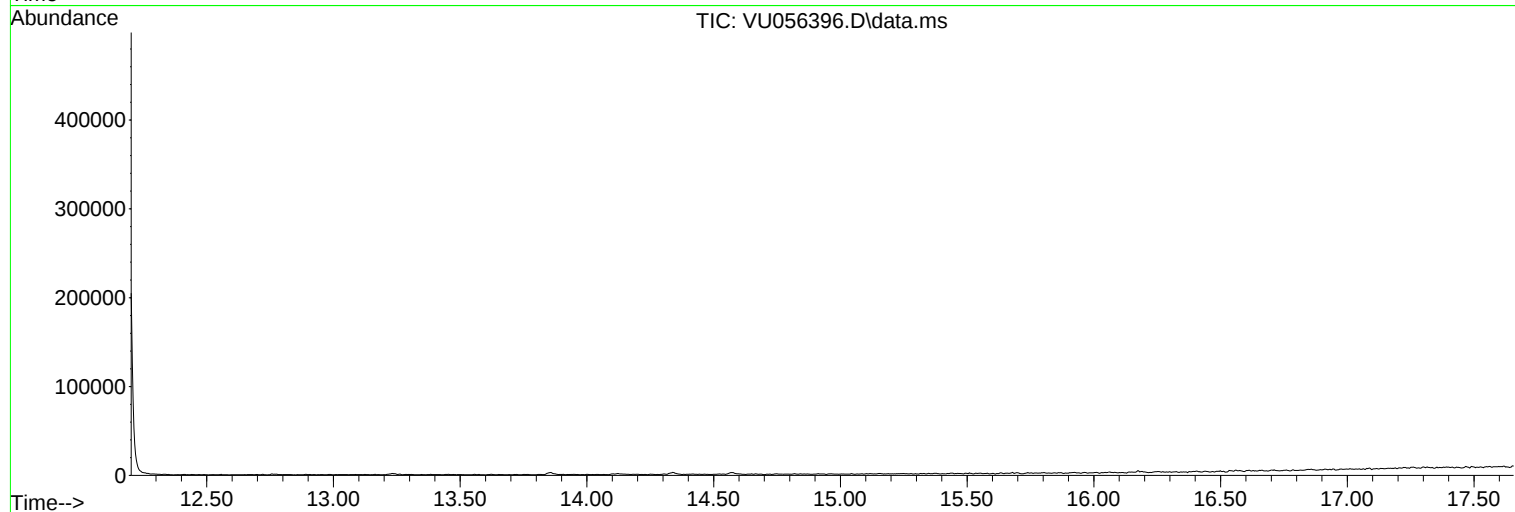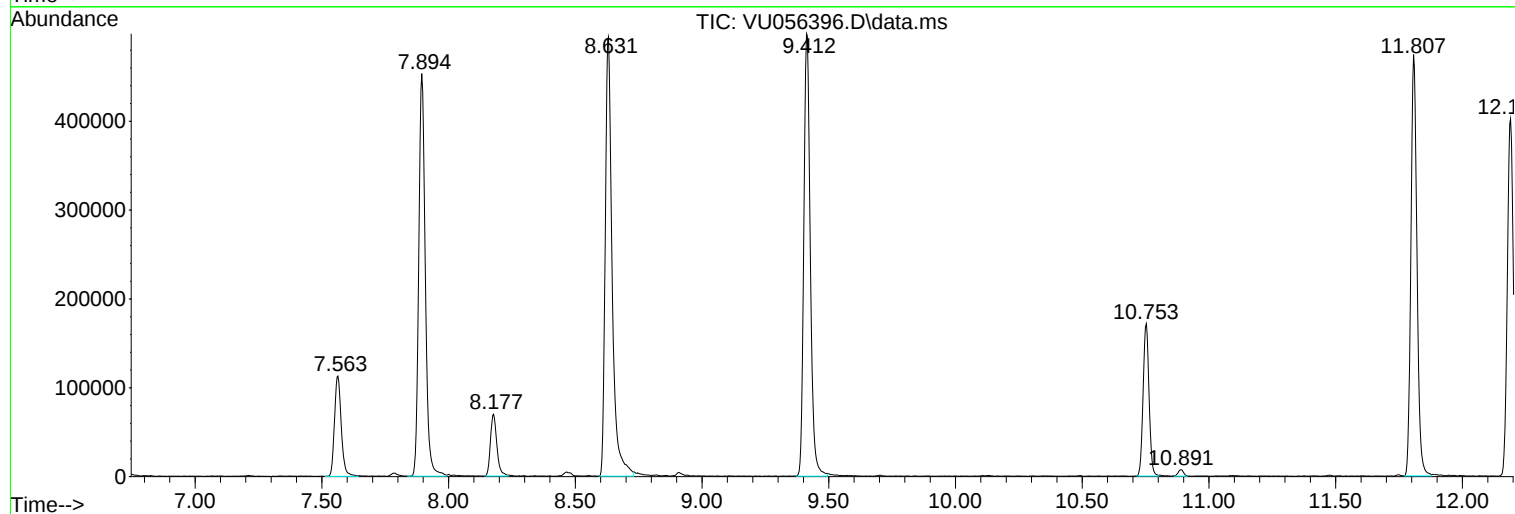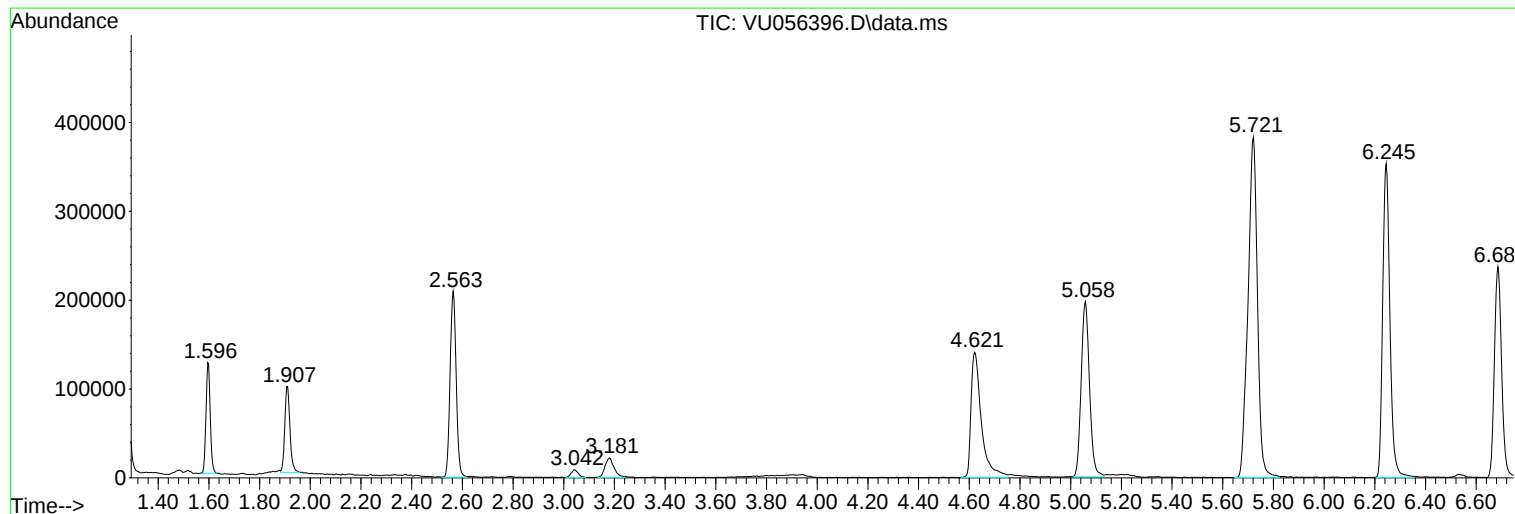

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111623\
Data File : VU056396.D
Acq On : 16 Nov 2023 10:15
Operator : MD/SY
Sample : VU1116WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK075

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111623\
Data File : VU056396.D
Acq On : 16 Nov 2023 10:15
Operator : MD/SY
Sample : VU1116WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK075

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc