
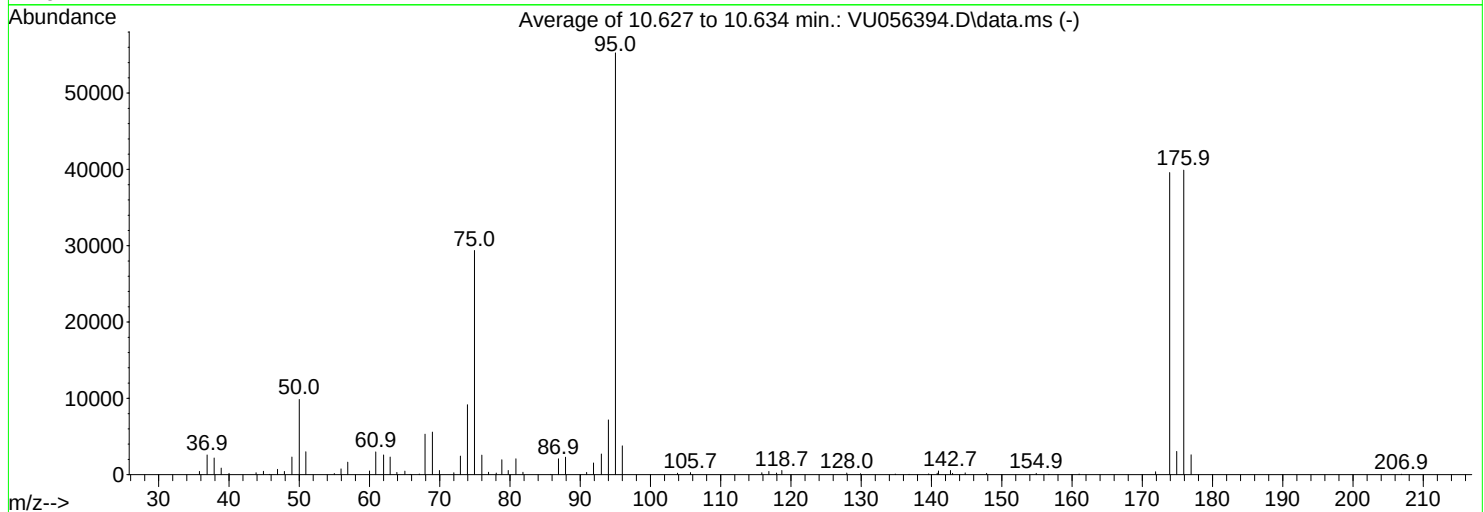


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111623\
Data File : VU056394.D
Acq On : 16 Nov 2023 08:41
Operator : MD/SY
Sample : BFB075
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB075

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Nov 17 04:03:21 2023

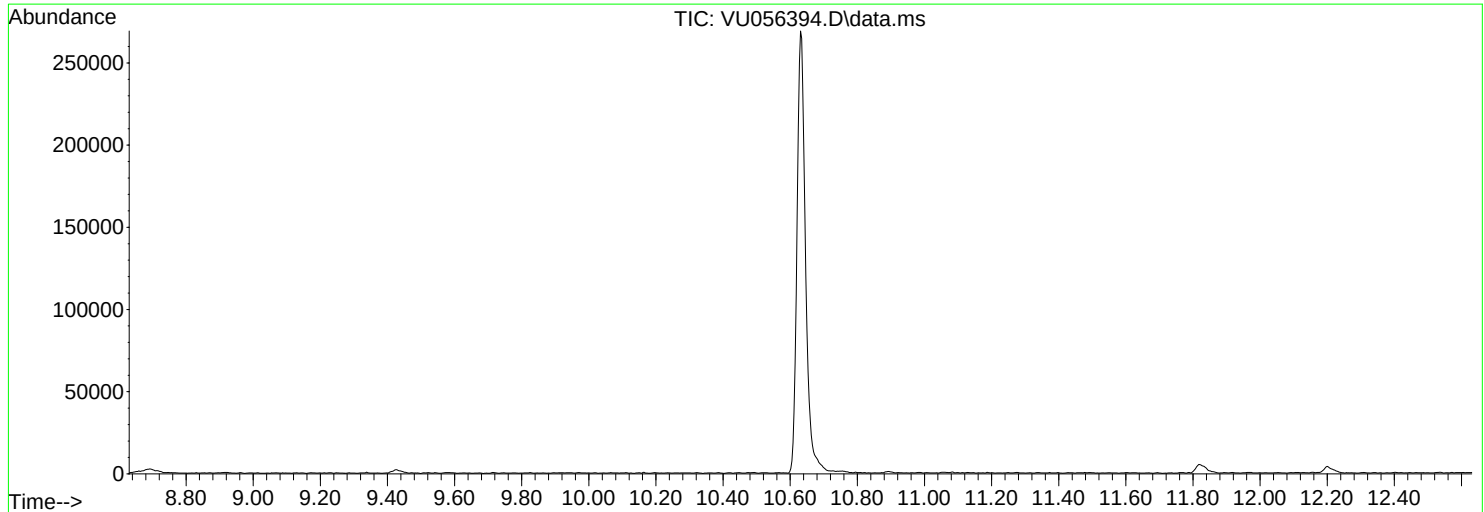

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	9866	PASS
75	95	30	80	53.2	29384	PASS
95	95	100	100	100.0	55277	PASS
96	95	5	9	6.8	3783	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.6	39589	PASS
175	174	5	9	7.7	3042	PASS
176	174	95	101	100.8	39912	PASS
177	176	5	9	6.5	2593	PASS

m/z	Abundance
39.80	164.0
43.90	427.0

Instrument :
MSVOA_U
ClientSampleId :
BFB075

m/z	Abundance
35.80	451.0
36.90	2559.0
37.90	2045.0
38.90	891.0
39.70	191.0
40.00	181.0
43.80	638.0
44.90	403.0
45.80	119.0
46.90	599.0
47.90	345.0
49.00	2266.0
50.00	8997.0
51.00	2773.0
55.00	125.0
56.00	778.0
56.90	1699.0
59.90	488.0
60.90	2800.0
62.00	2430.0
62.90	2193.0
63.80	304.0
65.00	347.0
67.10	139.0
67.90	5295.0
69.00	5407.0
69.90	568.0
72.00	187.0
72.90	2360.0
73.90	8564.0
75.00	28696.0
76.00	2559.0
77.00	316.0
78.00	152.0
78.80	1930.0
79.70	496.0
80.80	1982.0
81.90	320.0
86.90	2031.0
87.90	2340.0
90.90	354.0
91.90	1607.0
93.00	2373.0
94.00	6838.0
95.00	54072.0
96.00	3638.0
103.90	156.0
105.70	361.0
115.80	192.0
116.90	389.0
117.90	183.0
118.70	520.0
128.00	163.0
129.90	135.0
140.80	555.0
142.70	582.0
144.80	191.0
147.80	130.0
154.90	220.0
156.70	102.0
171.90	422.0
173.90	37368.0
174.90	2807.0
175.90	37264.0
176.90	2512.0

Instrument :
MSVOA_U
ClientSampleId :
BFB075

m/z	Abundance
35.80	433.0
36.90	2603.0
37.90	2226.0
38.90	882.0
40.00	170.0
43.80	689.0
44.90	456.0
46.90	739.0
47.90	444.0
48.90	2395.0
50.00	10111.0
51.00	3143.0
55.00	143.0
55.90	761.0
56.90	1719.0
60.00	498.0
60.90	3122.0
62.00	2669.0
63.00	2398.0
63.90	288.0
65.10	465.0
67.10	146.0
67.90	5492.0
69.00	5810.0
69.90	568.0
72.00	258.0
73.00	2492.0
73.90	9463.0
75.00	30208.0
76.00	2565.0
77.00	295.0
78.00	232.0
78.80	2032.0
79.80	540.0
80.80	2091.0
81.90	329.0
86.90	2129.0
87.90	2346.0
90.90	311.0
91.90	1581.0
93.00	2841.0
94.00	7455.0
95.00	56872.0
96.00	3948.0
103.90	181.0
105.70	273.0
115.80	263.0
116.80	427.0
118.00	220.0
118.70	592.0
127.90	238.0
129.90	137.0
134.90	113.0
139.60	149.0
141.00	692.0
142.70	544.0
144.80	256.0
147.80	178.0
154.90	175.0
161.00	121.0
171.90	398.0
173.90	40824.0
174.90	3205.0
175.90	41224.0
177.00	2689.0
206.90	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB075

m/z	Abundance
35.80	371.0
36.90	2582.0
37.90	2262.0
38.90	790.0
40.00	178.0
43.90	683.0
44.90	469.0
46.90	721.0
47.90	455.0
48.90	2290.0
50.00	10489.0
50.90	3072.0
55.00	165.0
55.90	747.0
56.90	1469.0
60.10	468.0
60.90	3007.0
62.00	2647.0
63.00	2321.0
64.00	300.0
65.10	544.0
65.80	120.0
67.90	5131.0
68.90	5549.0
70.00	523.0
72.00	303.0
73.00	2447.0
74.00	9470.0
74.90	29248.0
76.00	2527.0
76.90	330.0
78.10	268.0
78.90	1908.0
79.80	593.0
80.90	2189.0
81.80	309.0
85.80	148.0
86.90	2070.0
87.90	2199.0
90.90	208.0
91.90	1390.0
93.00	2873.0
94.00	7254.0
95.00	54888.0
96.00	3764.0
103.80	224.0
105.70	187.0
115.90	281.0
116.80	471.0
118.00	256.0
118.70	530.0
127.90	209.0
129.90	133.0
134.80	130.0
136.80	148.0
139.60	143.0
141.00	780.0
142.70	503.0
143.00	503.0
144.80	237.0
147.90	206.0
154.90	134.0
161.00	137.0
171.90	347.0
173.90	40576.0
174.90	3114.0
175.90	41248.0
176.90	2579.0
206.90	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB075