

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111624\
 Data File : VU061767.D
 Acq On : 17 Nov 2024 01:23
 Operator : MD/SY
 Sample : P4829-09
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E29W1

Quant Time: Nov 18 04:21:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 18 04:15:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	163714	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	155538	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	67742	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	36995	3.497	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	70.000%
7) Chloroethane-d5	1.908	69	41031	4.544	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.800%
11) 1,1-Dichloroethene-d2	2.560	65	17339	3.653	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.000%
20) 2-Butanone-d5	4.621	46	112800	50.242	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.480%
24) Chloroform-d	5.052	84	90841	4.321	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.400%
26) 1,2-Dichloroethane-d4	5.692	65	47357	4.693	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.800%
32) Benzene-d6	5.718	84	186395	4.332	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.600%
36) 1,2-Dichloropropane-d6	6.682	67	58969	4.647	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.000%
41) Toluene-d8	7.891	98	163746	4.083	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.600%
43) trans-1,3-Dichloroprop...	8.174	79	17849	3.818	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.400%
46) 2-Hexanone-d5	8.628	63	89698	48.558	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.120%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	47626	4.760	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.200%
66) 1,2-Dichlorobenzene-d4	12.187	152	58833	4.876	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.600%
Target Compounds					Qvalue	
13) Acetone	2.637	43	27919	19.738	ug/L	99
16) Methylene chloride	3.039	84	3891	0.342	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111624\
Data File : VU061767.D
Acq On : 17 Nov 2024 01:23
Operator : MD/SY
Sample : P4829-09
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E29W1


Quant Time: Nov 18 04:21:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 18 04:15:29 2024
Response via : Initial Calibration

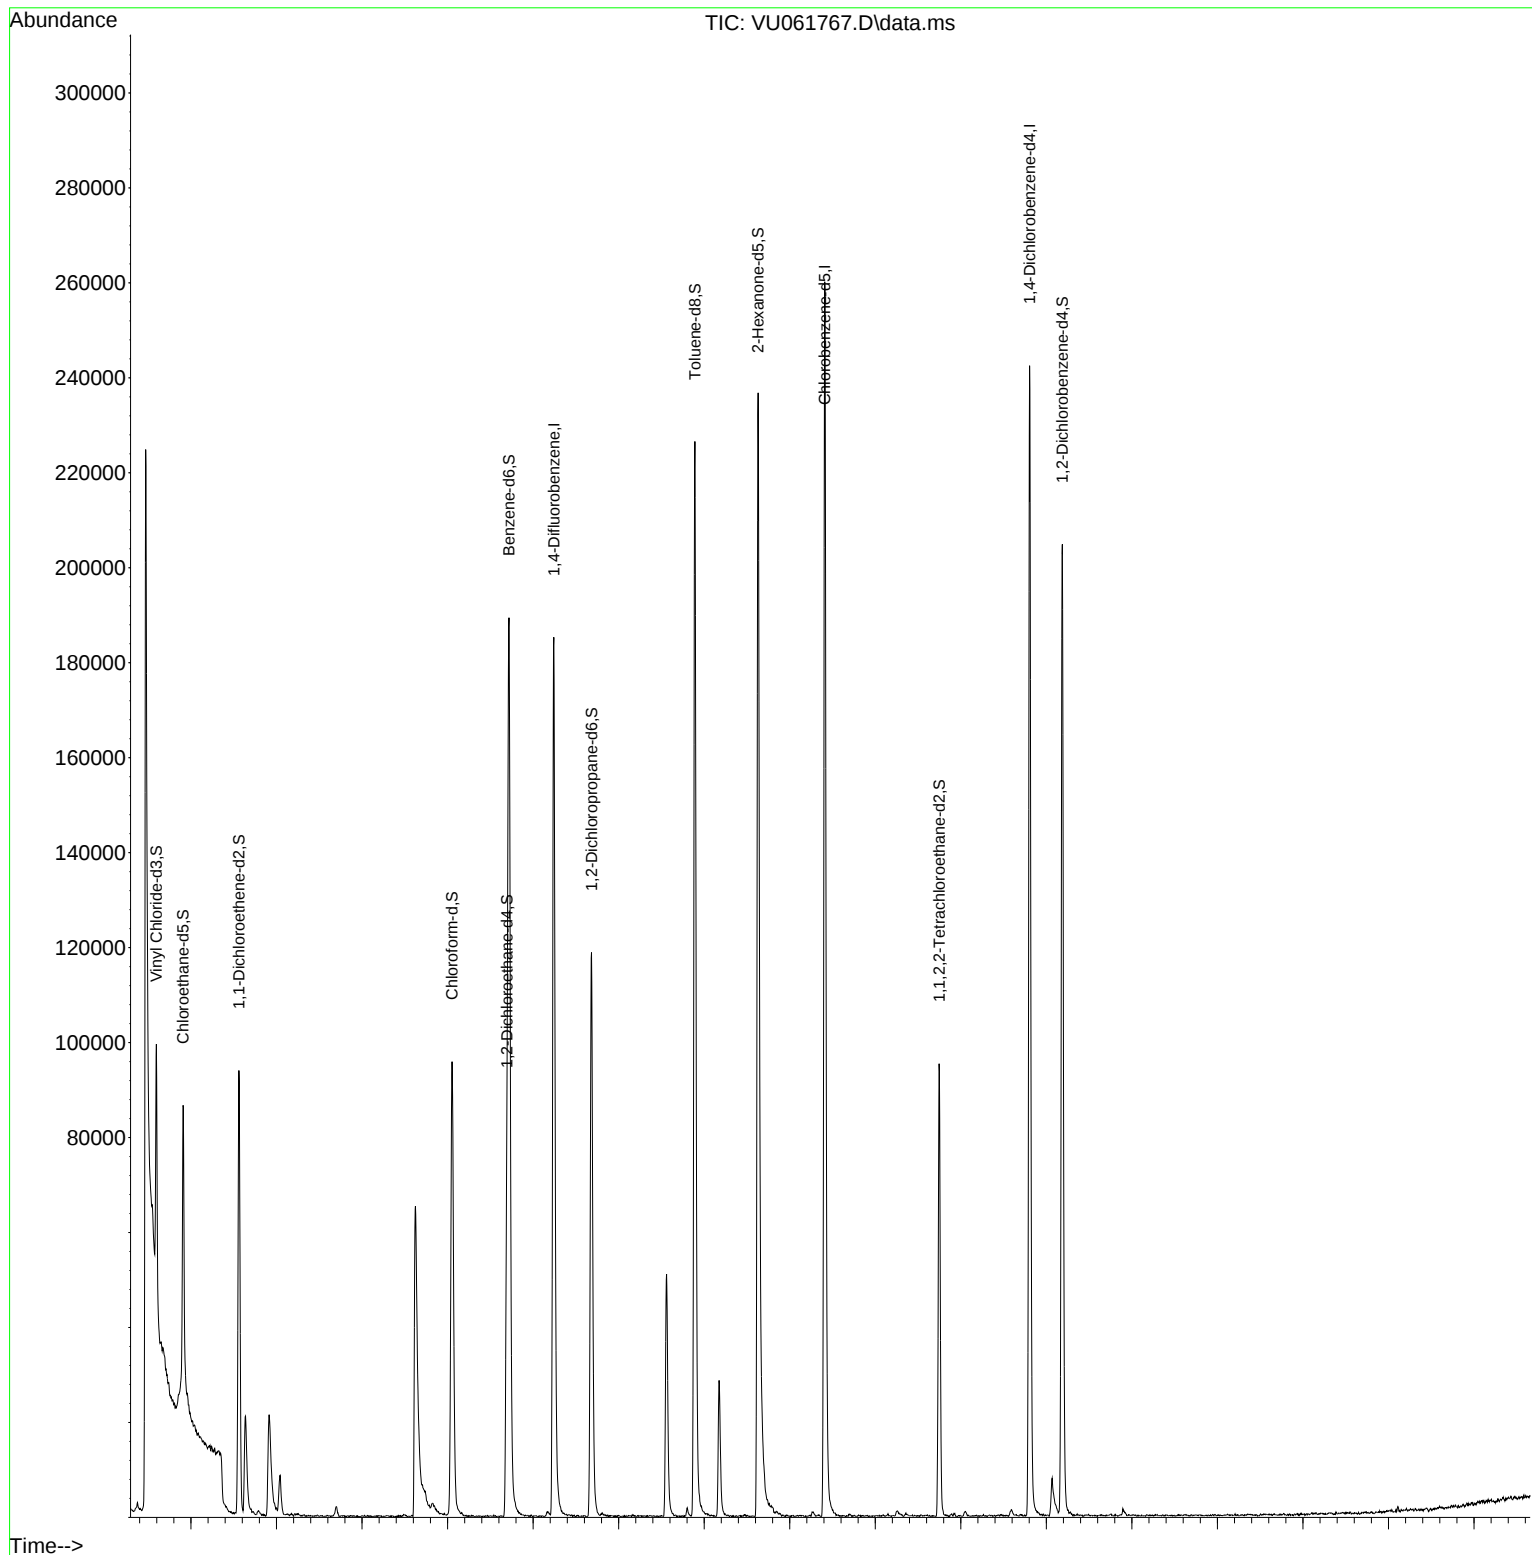

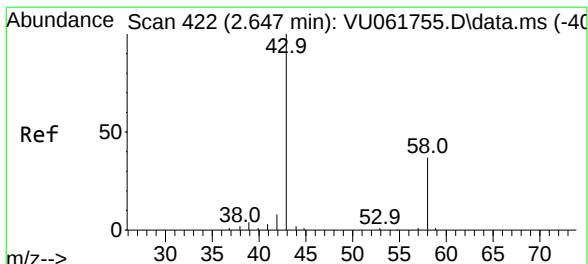




#13
 Acetone
 Concen: 19.738 ug/L
 RT: 2.637 min Scan# 41
 Delta R.T. -0.010 min
 Lab File: VU061767.D
 Acq: 17 Nov 2024 01:23

Instrument :
 MSVOA_U
 ClientSampleId :
 E29W1

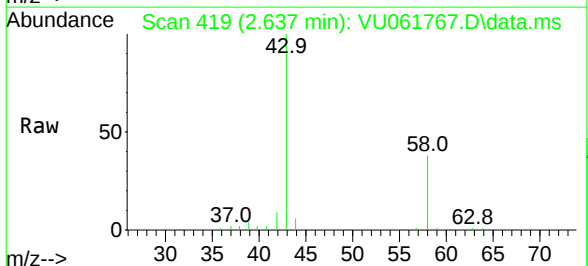

Tgt Ion: 43 Resp: 27919

Ion	Ratio	Lower	Upper
43	100		
58	35.3	0.0	69.8

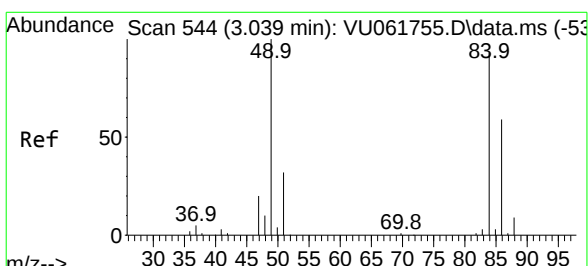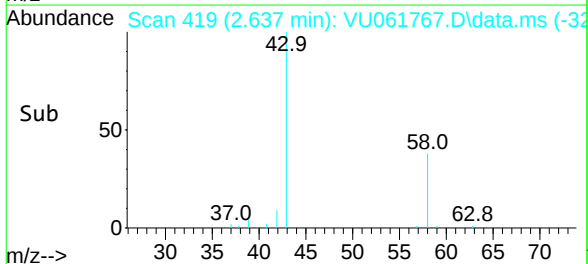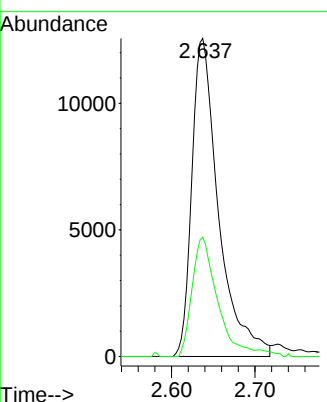

#16
 Methylene chloride
 Concen: 0.342 ug/L
 RT: 3.039 min Scan# 544
 Delta R.T. 0.000 min
 Lab File: VU061767.D
 Acq: 17 Nov 2024 01:23

Tgt Ion: 84 Resp: 3891

Ion	Ratio	Lower	Upper
84	100		
86	59.8	45.1	83.7
49	125.7	76.3	141.7

