

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111624\
 Data File : VU061769.D
 Acq On : 17 Nov 2024 02:12
 Operator : MD/SY
 Sample : P4829-11
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E29W5

Quant Time: Nov 18 04:22:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Nov 18 04:15:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	166292	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	158891	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	71897	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	38418	3.576	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.600%
7) Chloroethane-d5	1.911	69	40269	4.390	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.800%
11) 1,1-Dichloroethene-d2	2.563	65	18348	3.806	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.200%
20) 2-Butanone-d5	4.624	46	114750	50.318	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.640%
24) Chloroform-d	5.052	84	91505	4.285	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.600%
26) 1,2-Dichloroethane-d4	5.692	65	48480	4.730	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.600%
32) Benzene-d6	5.717	84	188313	4.284	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.600%
36) 1,2-Dichloropropane-d6	6.679	67	58978	4.549	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.000%
41) Toluene-d8	7.891	98	166693	4.069	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.400%
43) trans-1,3-Dichloroprop...	8.177	79	18508	3.876	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.600%
46) 2-Hexanone-d5	8.631	63	92097	48.805	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.600%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	49242	4.818	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.400%
66) 1,2-Dichlorobenzene-d4	12.187	152	60825	4.750	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.000%
Target Compounds						
13) Acetone	2.640	43	28838	20.071	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111624\
Data File : VU061769.D
Acq On : 17 Nov 2024 02:12
Operator : MD/SY
Sample : P4829-11
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E29W5


Quant Time: Nov 18 04:22:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Nov 18 04:15:29 2024
Response via : Initial Calibration

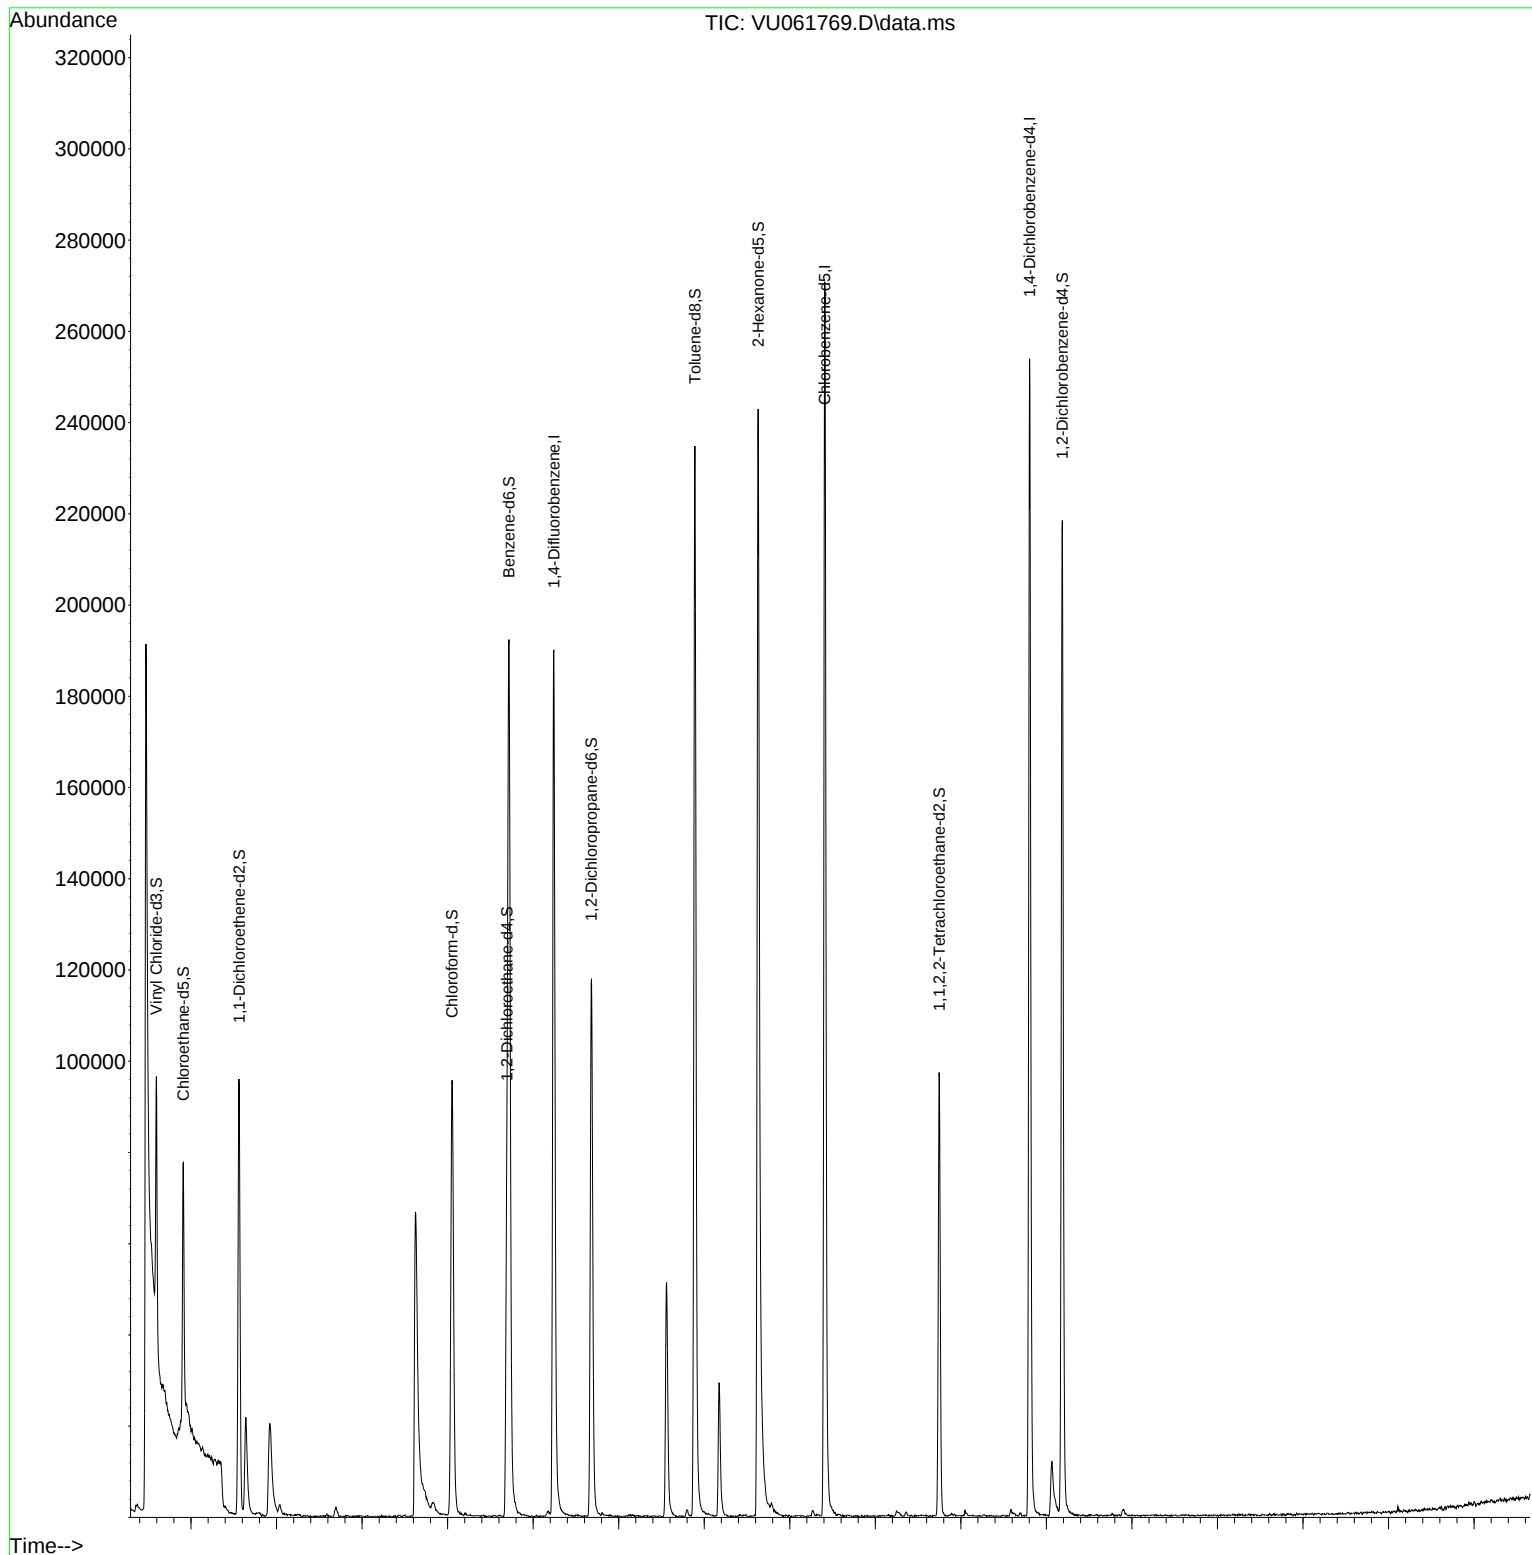

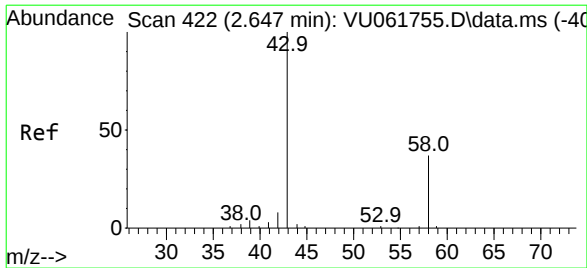

#13
Acetone
Concen: 20.071 ug/L
RT: 2.640 min Scan# 42
Delta R.T. -0.006 min
Lab File: VU061769.D
Acq: 17 Nov 2024 02:12

Instrument :
MSVOA_U
ClientSampleId :
E29W5

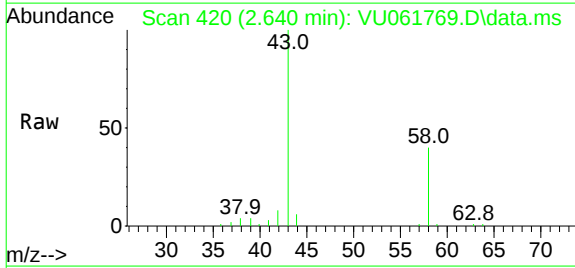

Tgt Ion: 43 Resp: 28838
Ion Ratio Lower Upper
43 100
58 37.5 0.0 69.8

