
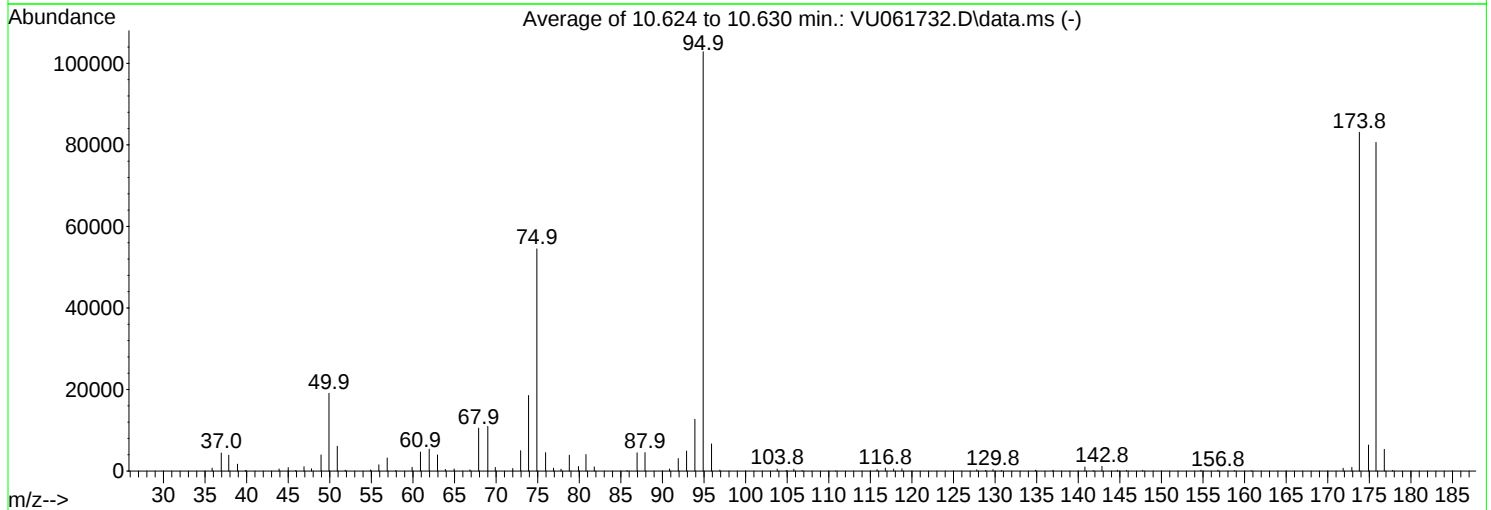


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111624\
Data File : VU061732.D
Acq On : 16 Nov 2024 08:38
Operator : MD/SY
Sample : BFB028
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB028

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Nov 18 04:15:29 2024

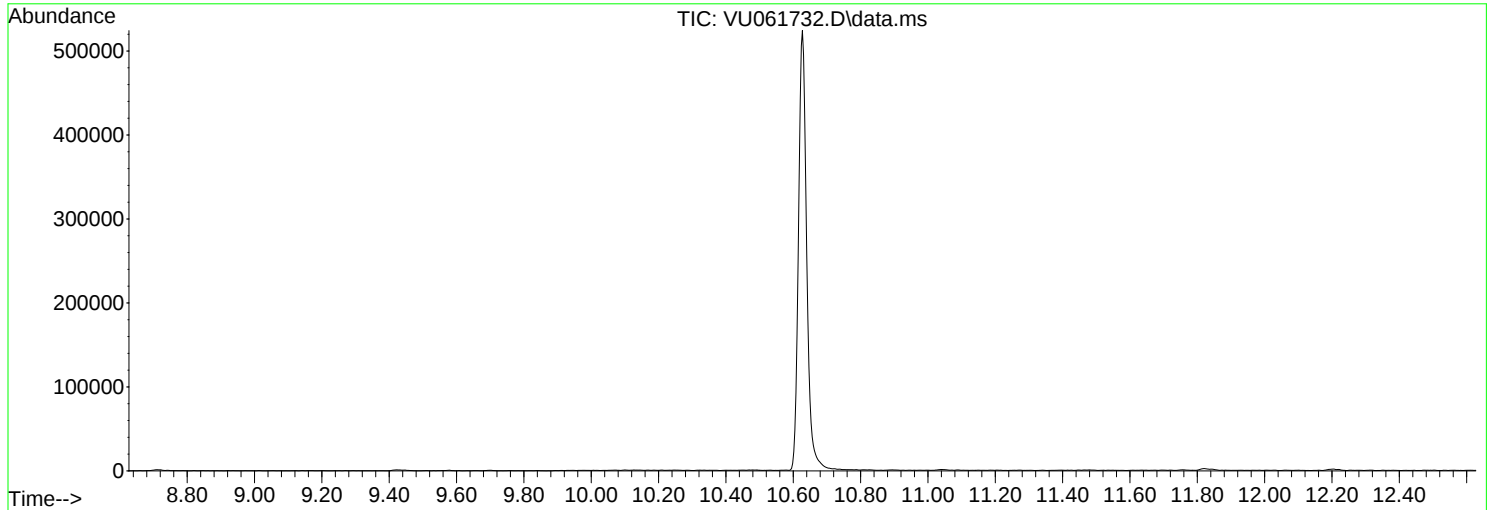

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	19085	PASS
75	95	30	80	53.0	54496	PASS
95	95	100	100	100.0	102848	PASS
96	95	5	9	6.5	6666	PASS
173	174	0.00	2	1.1	900	PASS
174	95	50	120	80.8	83104	PASS
175	174	5	9	7.7	6399	PASS
176	174	95	101	97.0	80629	PASS
177	176	5	9	6.6	5320	PASS

m/z	Abundance
35.90	408.0
37.80	138.0
43.90	308.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

m/z	Abundance
35.90	1181.0
37.00	4594.0
37.90	4159.0
38.90	1724.0
39.80	210.0
43.90	795.0
45.00	909.0
45.90	146.0
46.90	1167.0
47.80	554.0
48.90	4100.0
49.90	19344.0
50.90	6212.0
51.90	229.0
54.90	249.0
55.90	1577.0
56.90	3173.0
57.80	140.0
59.90	977.0
60.90	4786.0
61.90	5432.0
62.90	3865.0
63.90	377.0
65.00	533.0
66.80	294.0
67.90	10634.0
69.00	10888.0
69.90	845.0
72.00	660.0
72.90	5009.0
73.90	18632.0
74.90	54896.0
76.00	4709.0
76.90	768.0
77.80	457.0
78.80	3973.0
79.90	1149.0
80.80	4123.0
81.80	1047.0
85.70	150.0
86.90	4567.0
87.90	4363.0
90.80	489.0
91.90	3036.0
92.90	4999.0
93.90	12827.0
94.90	102272.0
95.90	6812.0
96.90	290.0
103.80	484.0
104.90	153.0
105.80	494.0
106.80	143.0
115.80	382.0
116.80	745.0
117.80	490.0
118.80	623.0
127.80	298.0
128.90	167.0
129.80	384.0
130.80	158.0
134.80	207.0
137.00	191.0
140.80	1013.0
141.80	133.0
142.80	1102.0
144.70	215.0
145.80	153.0
147.80	214.0
154.70	249.0
156.80	237.0
158.80	113.0
160.90	125.0
171.90	632.0
172.90	885.0
173.80	80808.0
174.90	6328.0
175.80	79168.0
176.80	5317.0
177.80	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

m/z	Abundance
35.90	1184.0
36.90	4620.0
37.90	4125.0
38.90	1751.0
39.80	189.0
44.00	857.0
45.00	890.0
45.90	142.0
46.90	1085.0
47.80	605.0
49.00	4048.0
49.90	19768.0
50.90	6282.0
51.80	217.0
54.90	289.0
55.90	1586.0
56.90	3358.0
57.90	110.0
59.90	968.0
60.90	4795.0
62.00	5573.0
63.00	4043.0
63.90	418.0
65.00	550.0
66.80	339.0
67.90	10909.0
69.00	11250.0
69.90	939.0
72.00	655.0
72.90	5120.0
73.90	19176.0
74.90	56232.0
76.00	4630.0
76.90	705.0
77.80	490.0
78.80	4022.0
79.90	1140.0
80.80	4221.0
81.80	1048.0
85.80	173.0
87.00	4608.0
87.90	4697.0
90.90	544.0
91.90	3135.0
92.90	5052.0
93.90	13132.0
94.90	105984.0
95.90	6842.0
96.90	232.0
103.80	517.0
104.90	165.0
105.80	476.0
106.80	147.0
115.80	410.0
116.80	766.0
117.80	523.0
118.80	568.0
127.80	328.0
128.80	187.0
129.70	399.0
130.70	167.0
134.80	222.0
137.00	208.0
140.80	1026.0
141.80	122.0
142.90	1209.0
144.70	228.0
145.80	158.0
147.80	194.0
154.70	227.0
156.80	246.0
158.80	114.0
160.80	115.0
171.80	706.0
172.90	976.0
173.80	85800.0
174.90	6648.0
175.80	83024.0
176.80	5477.0
177.80	186.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

m/z	Abundance
35.90	1036.0
36.90	4109.0
37.90	3835.0
38.90	1613.0
39.90	133.0
44.00	858.0
45.00	774.0
45.90	136.0
46.90	968.0
47.80	579.0
48.90	3713.0
49.90	18144.0
50.90	5798.0
51.80	218.0
54.90	287.0
55.90	1467.0
56.90	3119.0
58.00	100.0
59.90	895.0
60.90	4452.0
62.00	5190.0
62.90	3960.0
63.90	405.0
64.90	517.0
66.90	342.0
67.90	10060.0
69.00	10756.0
69.90	919.0
72.00	580.0
73.00	4873.0
73.90	17824.0
74.90	52360.0
75.90	4277.0
76.90	605.0
77.80	444.0
78.80	3748.0
79.90	1056.0
80.80	3840.0
81.80	1008.0
85.80	144.0
87.00	4291.0
87.90	4528.0
90.90	530.0
91.90	3047.0
92.90	4726.0
93.90	12142.0
94.90	100288.0
95.90	6344.0
96.90	175.0
103.80	490.0
104.90	158.0
105.80	446.0
106.80	130.0
110.80	100.0
115.80	391.0
116.80	697.0
117.80	514.0
118.80	530.0
127.80	372.0
128.80	204.0
129.70	367.0
130.70	174.0
134.90	223.0
136.90	213.0
140.80	977.0
141.80	100.0
142.80	1181.0
144.70	220.0
145.80	146.0
147.70	193.0
154.80	179.0
156.80	213.0
158.80	133.0
160.70	127.0
171.80	741.0
172.90	840.0
173.80	82704.0
174.90	6222.0
175.80	79696.0
176.80	5167.0
177.80	231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028