


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU111718\
 Data File : VU028217.D
 Acq On : 17 Nov 2018 09:23
 Operator : MD/SY
 Sample : BFB55
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB55

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111718WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Nov 19 02:51:07 2018

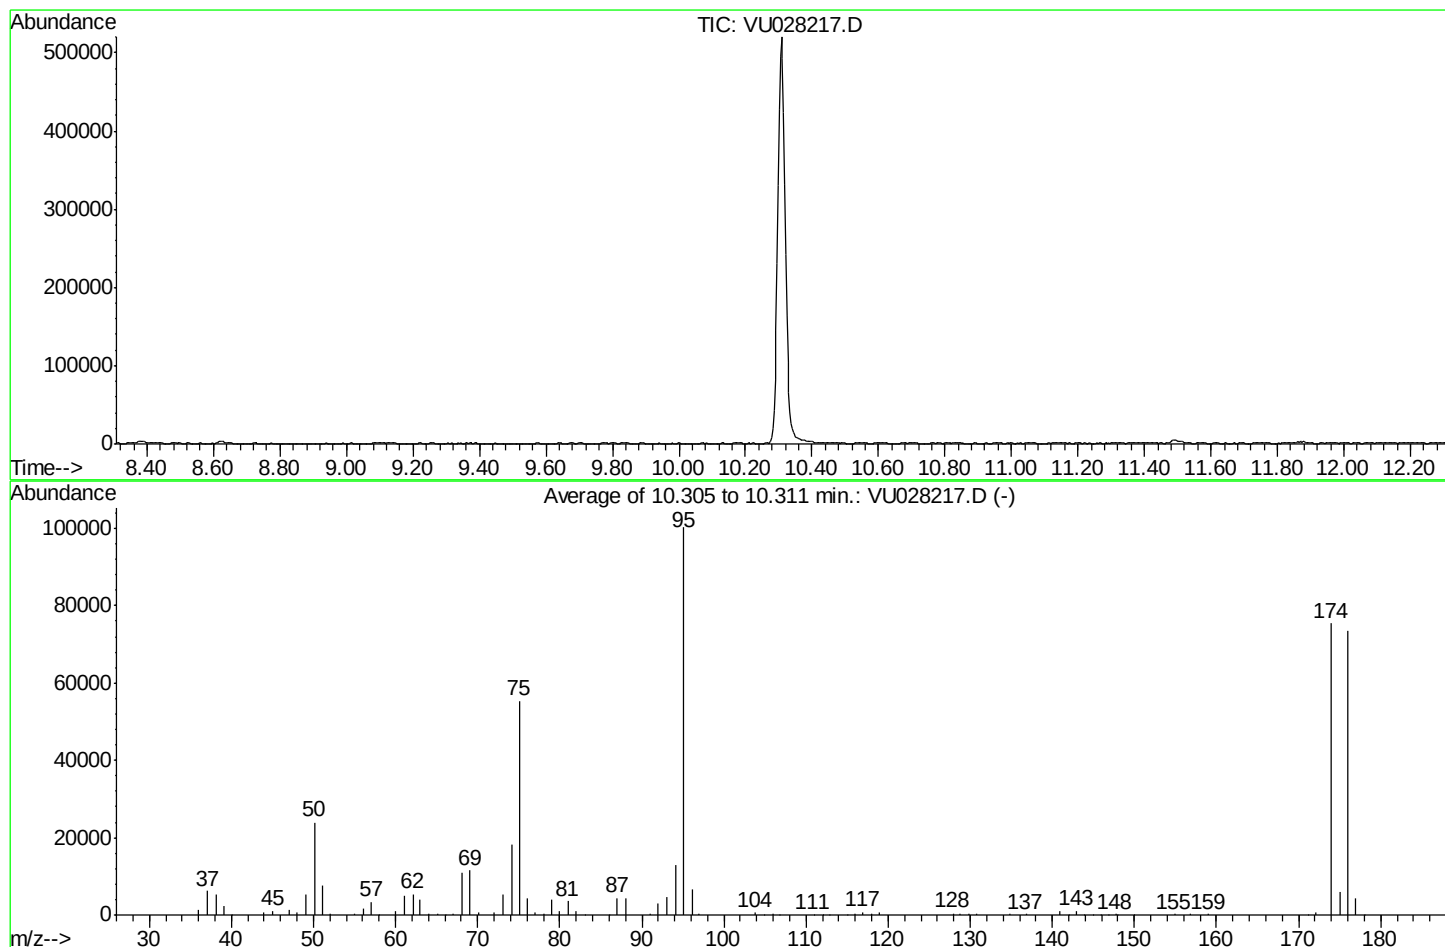

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.9	23952	PASS
75	95	30	80	55.2	55384	PASS
95	95	100	100	100.0	100250	PASS
96	95	5	9	6.6	6612	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.1	75330	PASS
175	174	5	9	7.9	5970	PASS
176	174	95	101	97.4	73344	PASS
177	176	5	9	6.0	4392	PASS

Scan 2827 (10.263 min): VU028217.D
BFB55

m/z	Abundance
40.00	305.0
44.00	645.0
206.90	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55

m/z	Abundance
36.00	1330.0
37.10	6063.0
38.10	5318.0
39.10	2123.0
40.00	326.0
44.00	1220.0
45.00	1126.0
47.00	1325.0
48.00	608.0
49.10	4918.0
50.10	23040.0
51.10	7107.0
52.00	433.0
55.10	356.0
56.10	1785.0
57.10	3342.0
57.90	144.0
60.00	1113.0
61.10	4882.0
62.10	5307.0
63.00	3587.0
64.00	346.0
65.10	400.0
66.00	118.0
67.10	355.0
68.10	10822.0
69.10	11174.0
70.10	676.0
72.00	612.0
73.10	4966.0
74.10	18320.0
75.10	53800.0
76.10	4281.0
77.00	541.0
78.00	500.0
79.00	3550.0
80.00	1036.0
81.00	3392.0
82.00	893.0
83.00	129.0
87.00	4166.0
88.00	4410.0
90.90	457.0
92.00	3047.0
93.00	4688.0
94.10	12897.0
95.10	97472.0
96.10	6585.0
96.90	200.0
103.90	457.0
104.90	156.0
106.00	404.0
110.90	117.0
112.90	104.0
115.00	106.0
115.90	438.0
117.00	644.0
118.00	423.0
118.90	670.0
128.00	408.0
128.80	283.0
129.90	330.0
130.80	211.0
134.90	177.0
136.80	251.0
141.00	1105.0
143.00	1077.0
143.90	165.0
145.00	117.0
146.00	155.0
147.80	229.0
154.90	151.0
156.90	195.0
159.10	178.0
172.10	659.0
174.00	75256.0
175.00	5997.0
176.00	72832.0
177.00	4465.0
178.00	130.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55

m/z	Abundance
36.00	1345.0
37.10	6369.0
38.10	5596.0
39.10	2359.0
40.00	341.0
44.00	1300.0
45.00	1182.0
47.00	1576.0
48.00	730.0
49.10	5445.0
50.10	24848.0
51.10	7752.0
52.00	388.0
55.10	436.0
56.10	1899.0
57.10	3598.0
57.90	137.0
60.00	1147.0
61.00	5241.0
62.10	5499.0
63.00	3970.0
64.00	296.0
65.10	466.0
66.00	159.0
67.00	345.0
68.10	11413.0
69.10	11983.0
70.10	827.0
72.00	595.0
73.10	5418.0
74.10	18832.0
75.10	57216.0
76.10	4464.0
77.00	654.0
78.00	497.0
79.00	4094.0
80.00	1138.0
81.00	3674.0
81.90	891.0
83.00	169.0
87.00	4441.0
88.00	4483.0
90.90	403.0
92.00	3144.0
93.00	4696.0
94.10	13370.0
95.10	103448.0
96.10	6820.0
97.00	217.0
103.80	529.0
105.00	180.0
106.00	442.0
106.80	110.0
110.90	122.0
112.90	106.0
114.90	107.0
115.90	436.0
116.90	708.0
118.00	465.0
119.00	685.0
127.90	472.0
128.80	249.0
129.80	341.0
130.80	224.0
134.90	208.0
136.80	242.0
140.90	1135.0
142.00	123.0
143.00	1189.0
143.90	178.0
145.00	144.0
146.00	148.0
146.90	101.0
147.70	244.0
149.90	112.0
154.90	231.0
156.80	211.0
159.00	211.0
172.10	596.0
174.00	77992.0
175.00	6144.0
176.00	75864.0
177.00	4555.0
178.00	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55

m/z	Abundance
36.00	1148.0
37.10	6260.0
38.10	5284.0
39.10	2388.0
40.10	322.0
44.00	1316.0
45.10	1070.0
47.00	1519.0
48.00	737.0
49.10	5399.0
50.10	23968.0
51.10	7630.0
52.00	349.0
55.00	433.0
56.00	1774.0
57.10	3403.0
57.90	122.0
60.10	1066.0
61.00	5075.0
62.10	5174.0
63.00	4105.0
64.00	276.0
65.10	491.0
66.00	112.0
67.00	277.0
68.10	10907.0
69.10	11526.0
70.10	895.0
72.00	492.0
73.00	5586.0
74.10	17800.0
75.10	55136.0
76.10	4202.0
77.00	805.0
78.10	457.0
79.00	4006.0
80.00	1070.0
81.00	3631.0
81.90	817.0
83.00	153.0
86.10	110.0
87.00	4611.0
88.00	4026.0
91.10	358.0
92.00	2835.0
93.10	4338.0
94.10	12752.0
95.10	99832.0
96.10	6432.0
97.00	168.0
103.80	588.0
105.00	165.0
106.00	440.0
106.80	115.0
110.90	126.0
112.10	110.0
114.90	104.0
115.90	373.0
116.90	696.0
118.00	436.0
119.00	556.0
127.90	399.0
128.70	224.0
129.80	340.0
130.80	146.0
134.80	234.0
136.80	180.0
140.90	1082.0
142.00	148.0
143.00	1120.0
143.90	126.0
145.00	152.0
145.90	119.0
146.80	108.0
147.70	195.0
148.00	183.0
154.90	261.0
156.80	146.0
159.00	233.0
171.10	139.0
172.00	529.0
174.00	72744.0
175.00	5770.0
176.00	71336.0
177.00	4158.0
178.00	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB55