

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU111720\
 Data File : VU041272.D
 Acq On : 17 Nov 2020 11:44
 Operator : SY/MD
 Sample : L4759-07
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4426

Quant Time: Nov 17 22:51:32 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Nov 17 22:32:58 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	67533	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	70942	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	29293	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	23397	4.71	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.20%
7) Chloroethane-d5	1.92	69	20215	4.76	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.20%
11) 1,1-Dichloroethene-d2	2.58	63	35681	3.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.60%
20) 2-Butanone-d5	4.65	46	95002	46.38	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.76%
24) Chloroform-d	5.08	84	53302	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.20%
26) 1,2-Dichloroethane-d4	5.72	65	32989	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.00%
32) Benzene-d6	5.74	84	94354	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
36) 1,2-Dichloropropane-d6	6.70	67	34296	5.20	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.00%
41) Toluene-d8	7.91	98	77028	4.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.60%
43) trans-1,3-Dichloropropene-	8.19	79	12129	4.27	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.40%
46) 2-Hexanone-d5	8.64	63	66307	43.76	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.52%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	29249	4.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.40%
64) 1,2-Dichlorobenzene-d4	12.19	152	30232	5.29	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.80%


Target Compounds					Ovalue
13) Acetone	2.66	43	3860	2.841 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU111720\
Data File : VU041272.D
Acq On : 17 Nov 2020 11:44
Operator : SY/MD
Sample : L4759-07
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4426

Quant Time: Nov 17 22:51:32 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 17 22:32:58 2020
Response via : Initial Calibration

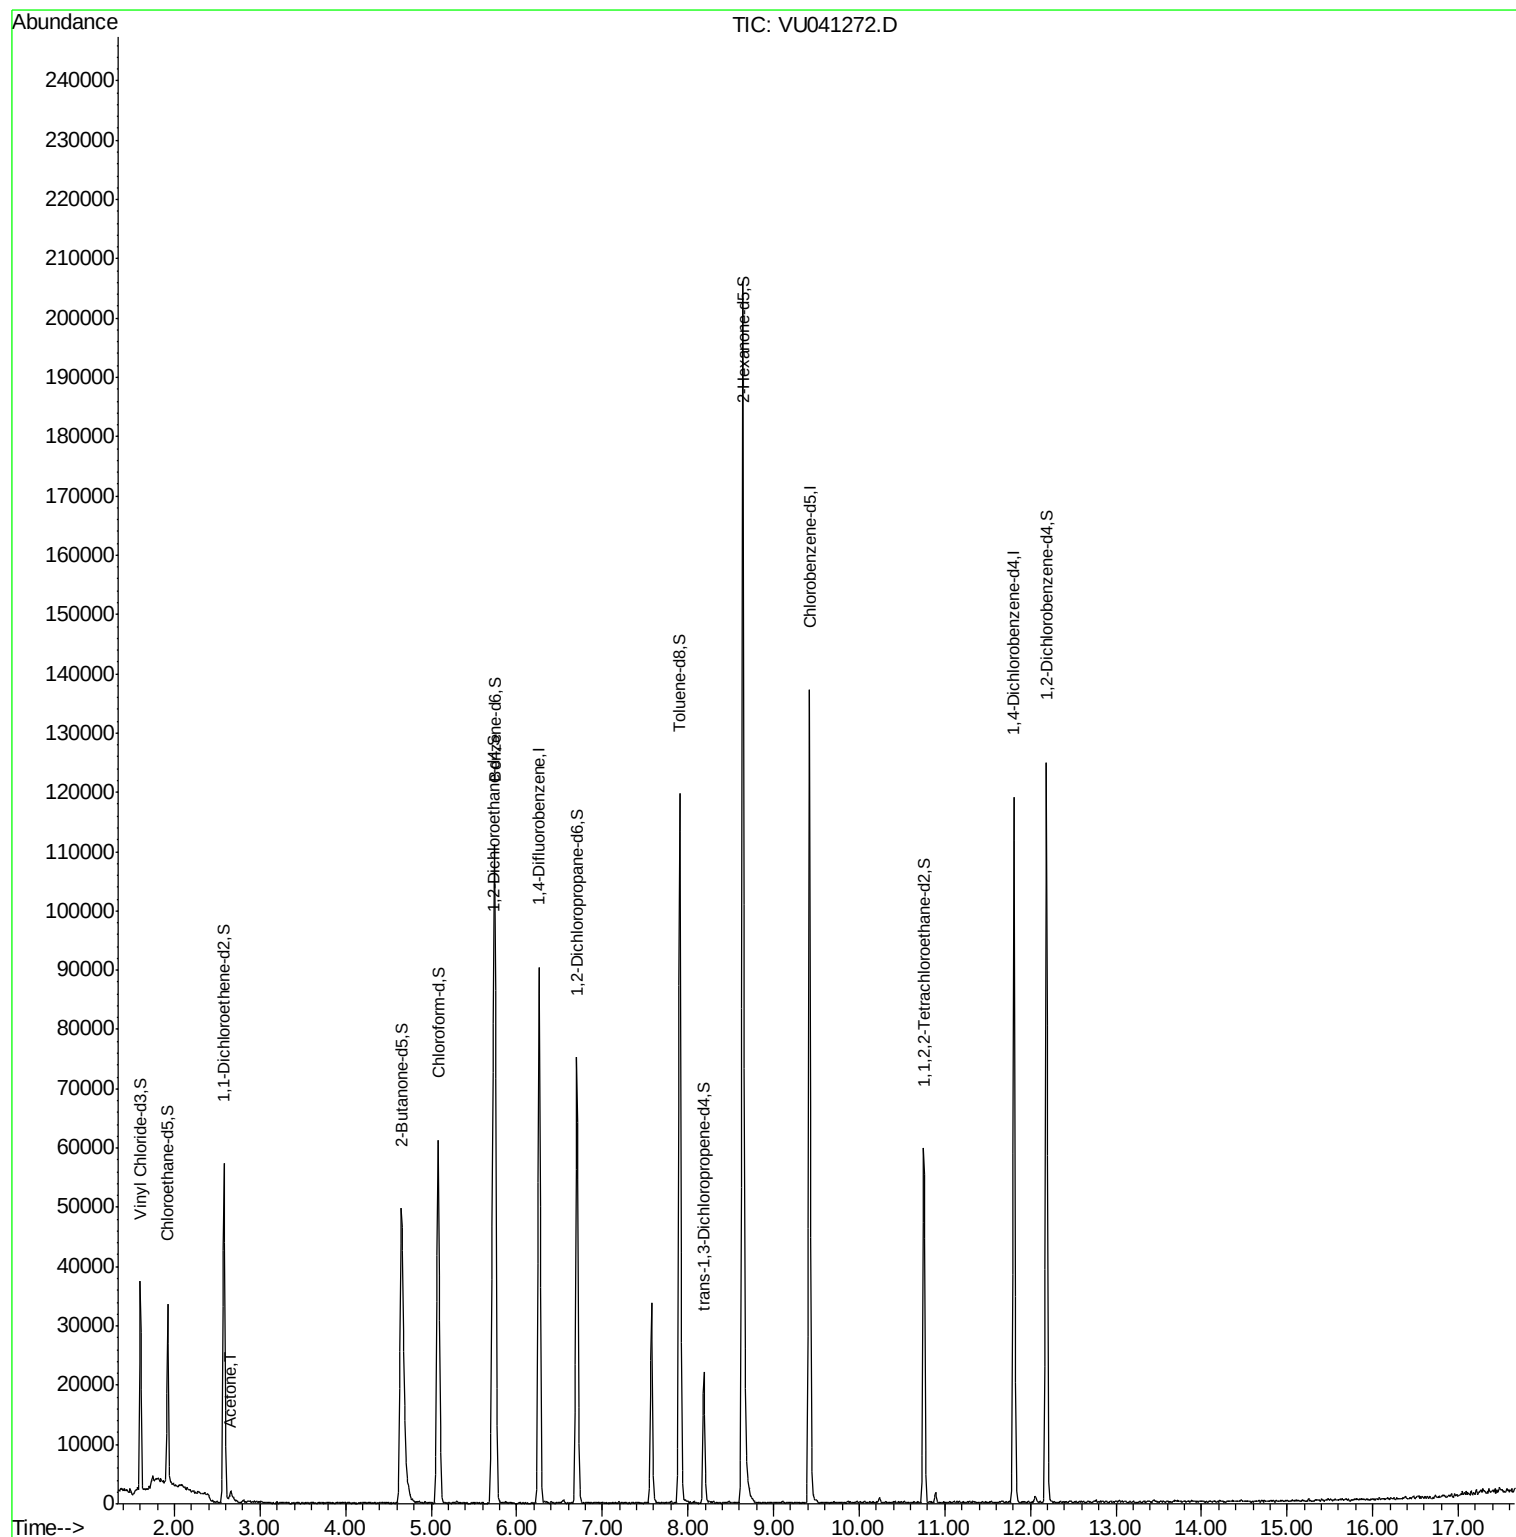

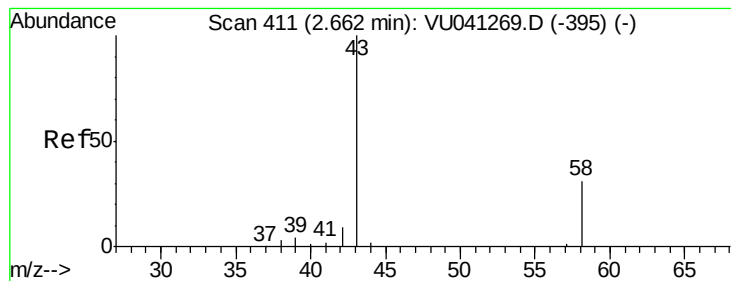

#13
 Acetone
 Concen: 2.841 ug/L
 RT: 2.66 min Scan# 412
 Delta R.T. 0.00 min
 Lab File: VU041272.D
 Acq: 17 Nov 2020 11:44

Instrument :
 MSVOA_U
 ClientSampleId :
 H4426

Tot Ion: 43 Resp: 3860
 Ion Ratio Lower Upper
 43 100
 58 17.5 0.0 25.4

