

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU111720\
 Data File : VU041293.D
 Acq On : 17 Nov 2020 22:15
 Operator : SY/MD
 Sample : L4759-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4387

Quant Time: Nov 18 00:29:35 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Nov 18 00:06:52 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	63074	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	64220	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	23233	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	23407	5.04	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.80%
7) Chloroethane-d5	1.92	69	20210	5.09	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.80%
11) 1,1-Dichloroethene-d2	2.58	63	34238	3.57	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.40%
20) 2-Butanone-d5	4.66	46	86433	45.18	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.36%
24) Chloroform-d	5.08	84	48828	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.20%
26) 1,2-Dichloroethane-d4	5.72	65	31267	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.40%
32) Benzene-d6	5.74	84	87676	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.20%
36) 1,2-Dichloropropane-d6	6.70	67	29916	5.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.20%
41) Toluene-d8	7.91	98	69510	4.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.20%
43) trans-1,3-Dichloropropene-	8.19	79	11330	4.41	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.20%
46) 2-Hexanone-d5	8.64	63	60175	43.87	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.74%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	25168	4.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.00%
64) 1,2-Dichlorobenzene-d4	12.19	152	24133	5.32	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.40%


Target Compounds					Ovalue
13) Acetone	2.67	43	3418	2.693 ug/L	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU111720\
Data File : VU041293.D
Acq On : 17 Nov 2020 22:15
Operator : SY/MD
Sample : L4759-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4387

Quant Time: Nov 18 00:29:35 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 18 00:06:52 2020
Response via : Initial Calibration

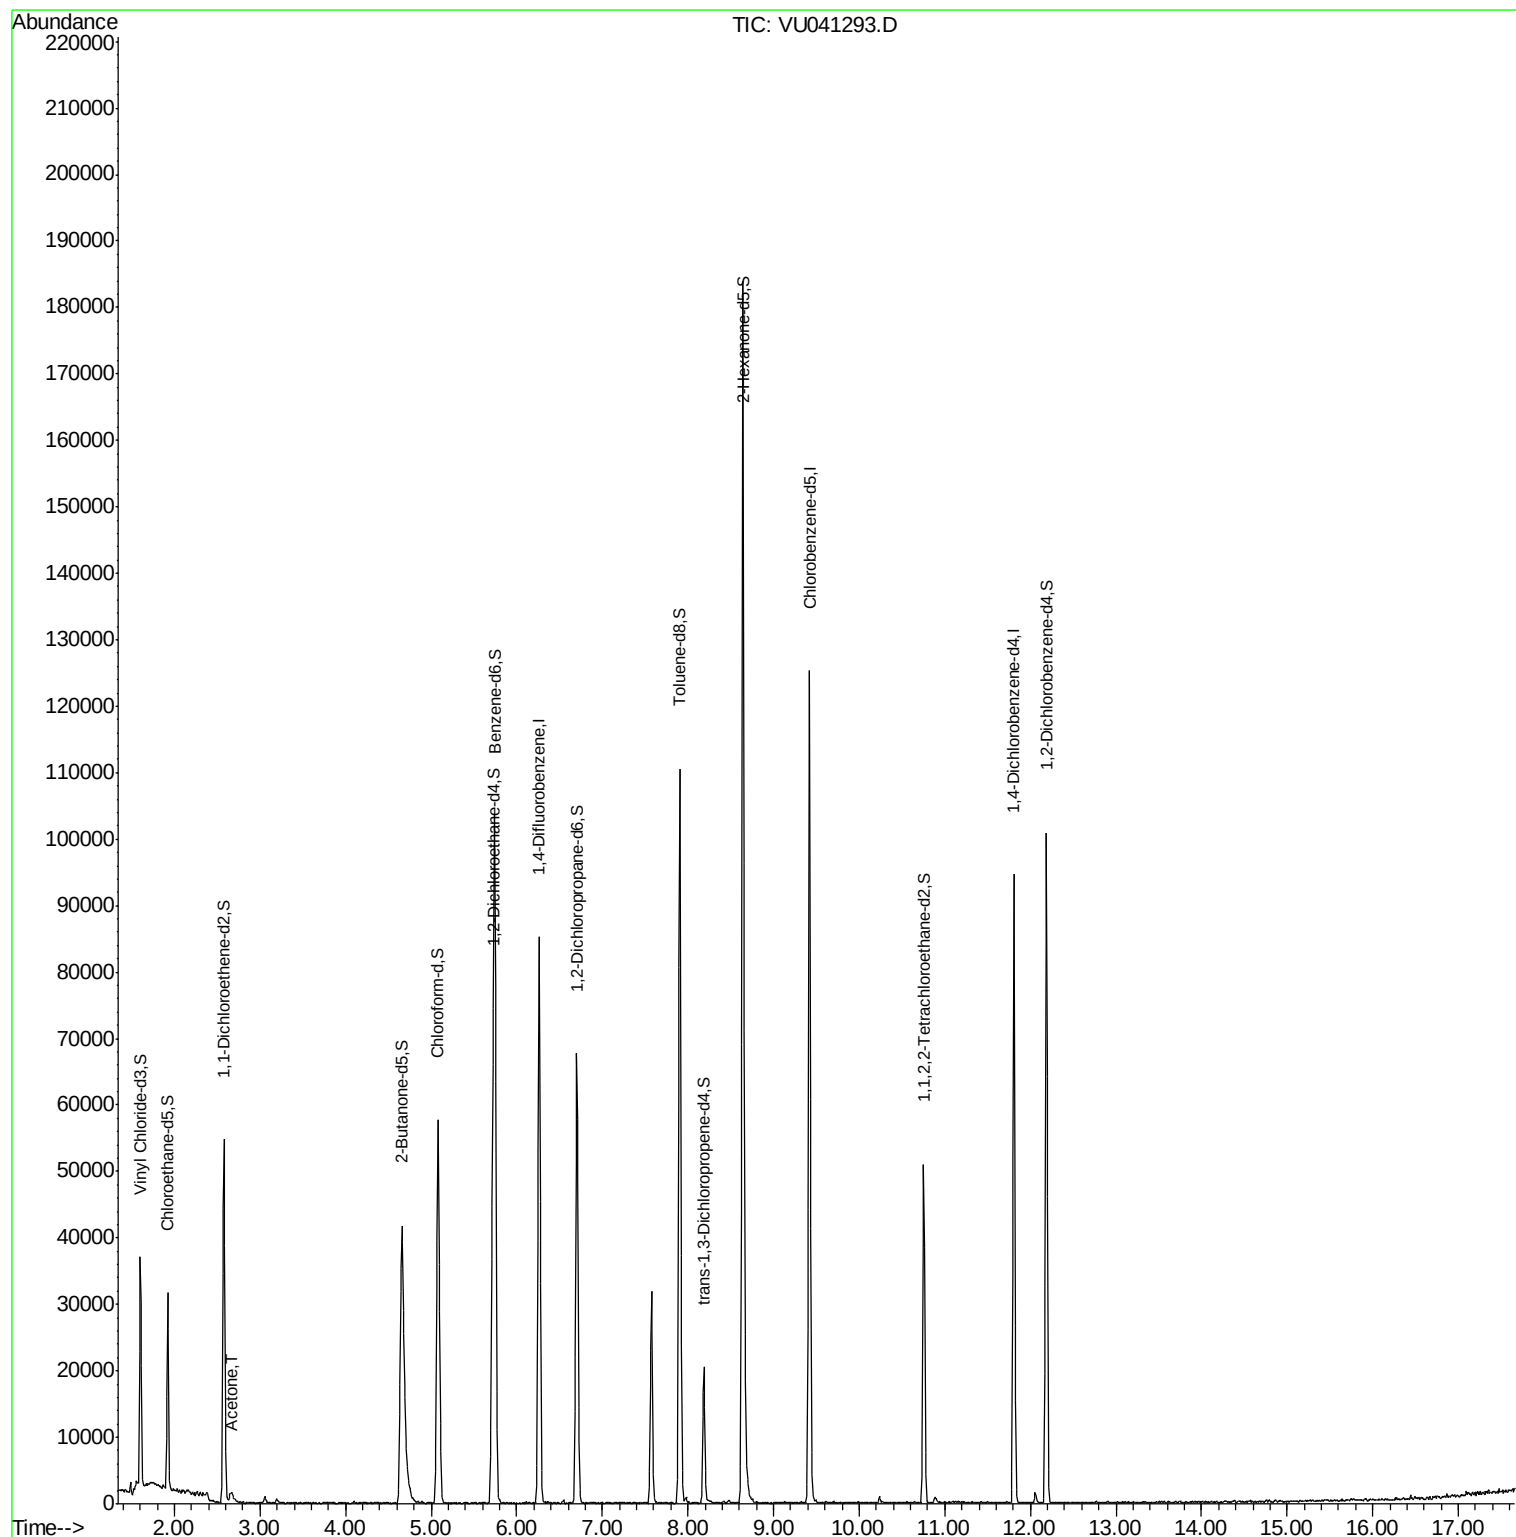

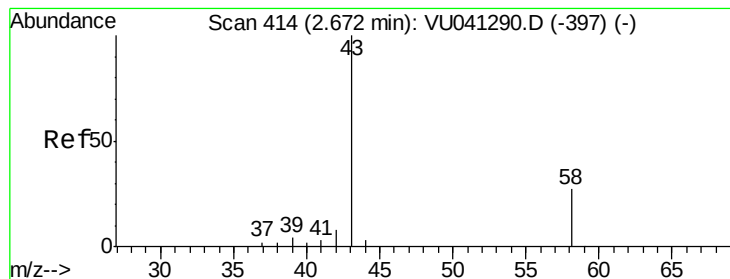

#13

Acetone

Concen: 2.693 ug/L

RT: 2.67 min Scan# 414

Delta R.T. -0.00 min

Lab File: VU041293.D

Acq: 17 Nov 2020 22:15

Instrument :
MSVOA_U
ClientSampleId :
H4387

Tot Ion: 43 Resp: 3418

Ion Ratio Lower Upper

43 100

58 22.5 0.0 25.4

