

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111721\
 Data File : VU045837.D
 Acq On : 17 Nov 2021 14:01
 Operator : SY/MD
 Sample : M4686-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG1Z5

Quant Time: Nov 18 02:20:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 18 02:11:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	92894	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	98463	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	44785	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	22112	3.004	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	60.000%
7) Chloroethane-d5	1.919	69	20119	3.755	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	75.200%
11) 1,1-Dichloroethene-d2	2.572	65	10259	3.323	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.400%
20) 2-Butanone-d5	4.642	46	109468	55.502	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.000%
24) Chloroform-d	5.067	84	50537	4.121	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.400%
26) 1,2-Dichloroethane-d4	5.706	65	31268	4.346	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.000%
32) Benzene-d6	5.732	84	98229	3.623	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	72.400%
36) 1,2-Dichloropropane-d6	6.694	67	35027	4.099	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.000%
41) Toluene-d8	7.902	98	82417	3.360	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	67.200%#
43) trans-1,3-Dichloroprop...	8.179	79	13219	3.810	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.200%
46) 2-Hexanone-d5	8.636	63	75358	48.262	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.520%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	33453	4.634	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.600%
66) 1,2-Dichlorobenzene-d4	12.195	152	35826	4.659	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.200%
Target Compounds						Qvalue
3) Chloromethane	1.520	50	1097	0.137	ug/L	90
9) Trichlorofluoromethane	2.144	101	1157	0.111	ug/L	97
17) Methyl tert-butyl Ether	3.369	73	2160	0.144	ug/L #	91
22) cis-1,2-Dichloroethene	4.671	96	4884	0.731	ug/L	91
34) Trichloroethene	6.546	95	63688	8.994	ug/L	98
47) Tetrachloroethene	8.555	164	12039	2.429	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111721\
Data File : VU045837.D
Acq On : 17 Nov 2021 14:01
Operator : SY/MD
Sample : M4686-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG1Z5

Quant Time: Nov 18 02:20:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 18 02:11:55 2021
Response via : Initial Calibration




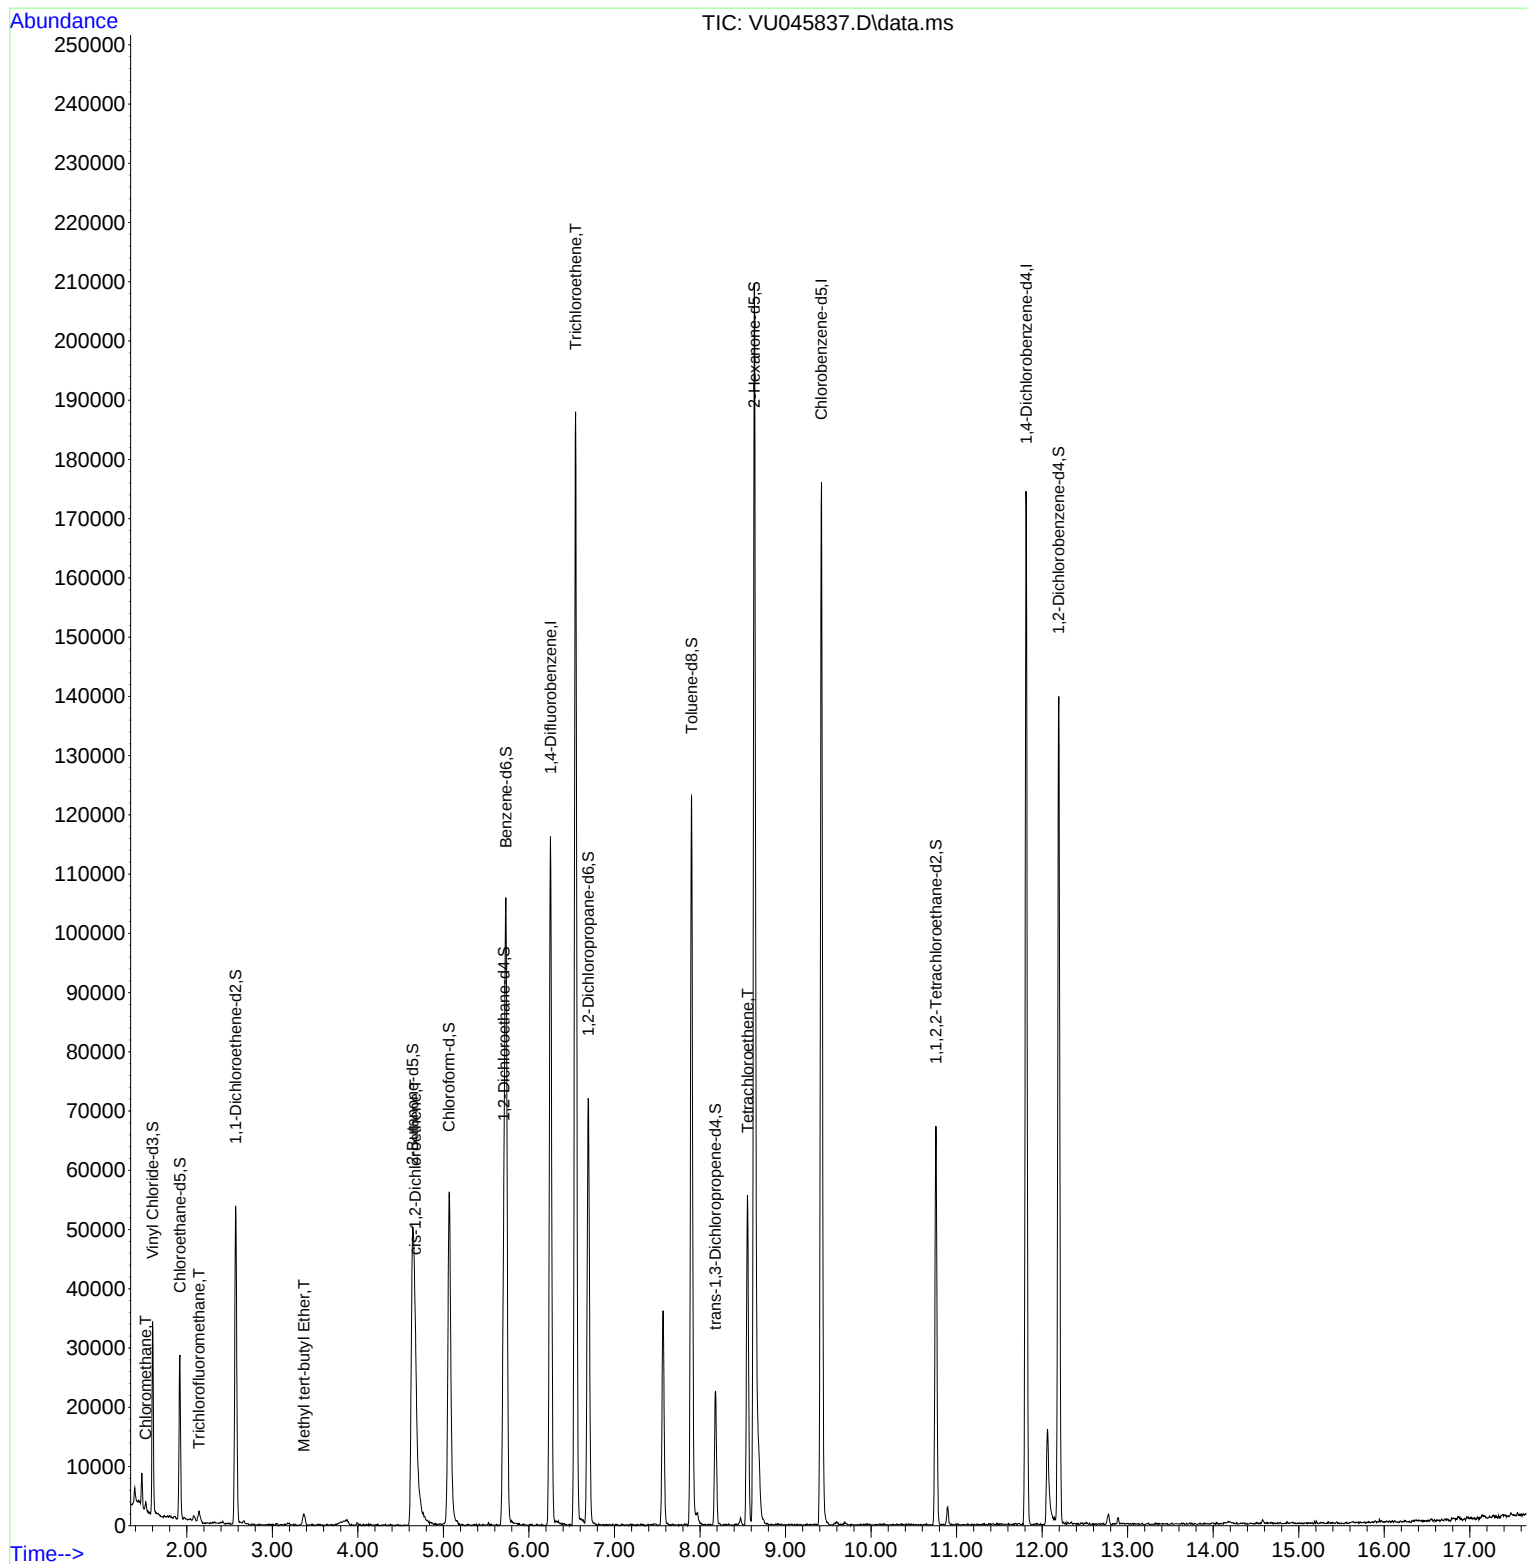


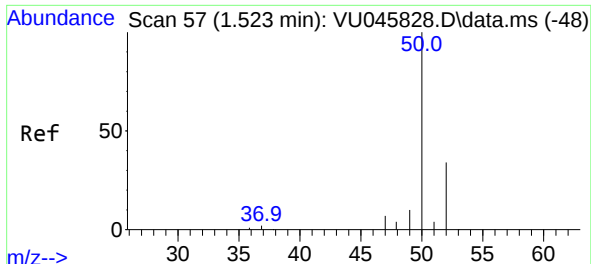

#3
Chloromethane
Concen: 0.137 ug/L
RT: 1.520 min Scan# 50
Delta R.T. -0.003 min
Lab File: VU045837.D
Acq: 17 Nov 2021 14:01




Instrument :
MSVOA_U
ClientSampleId :
BG1Z5


Tgt Ion: 50 Resp: 1097
Ion Ratio Lower Upper
50 100
52 27.5 23.0 42.8

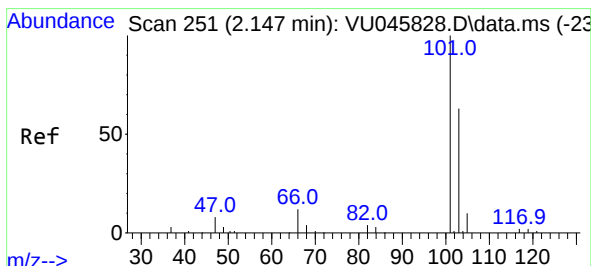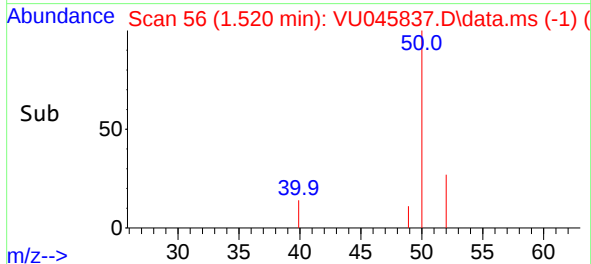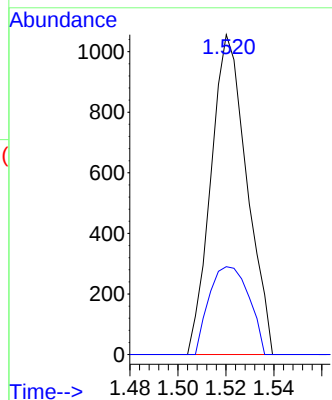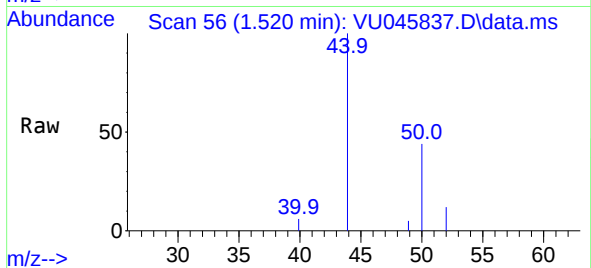

#9
Trichlorofluoromethane
Concen: 0.111 ug/L
RT: 2.144 min Scan# 250
Delta R.T. -0.003 min
Lab File: VU045837.D
Acq: 17 Nov 2021 14:01

Tgt Ion: 101 Resp: 1157
Ion Ratio Lower Upper
101 100
103 67.1 51.5 77.3


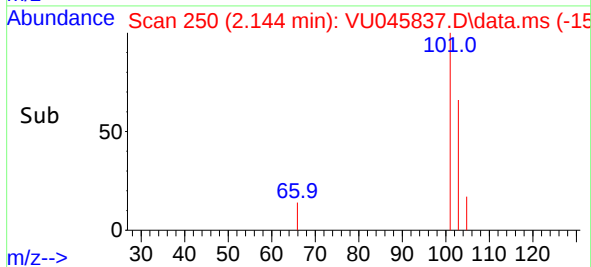
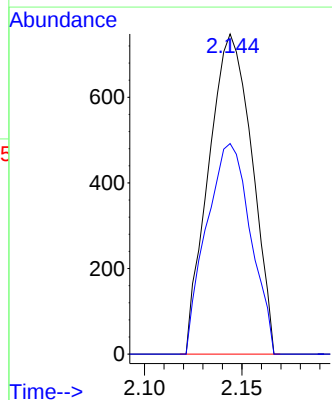
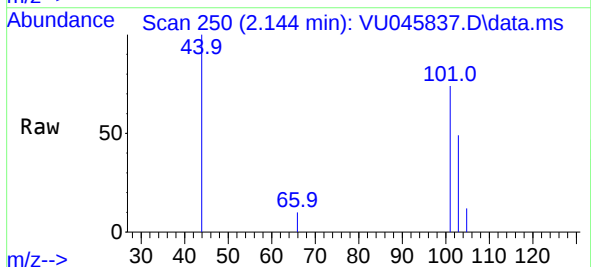


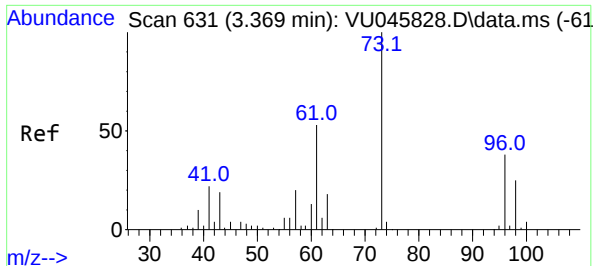

#17
Methyl tert-butyl Ether
Concen: 0.144 ug/L
RT: 3.369 min Scan# 61
Delta R.T. 0.000 min
Lab File: VU045837.D
Acq: 17 Nov 2021 14:01




Instrument :
MSVOA_U
ClientSampleId :
BG1Z5


Tgt Ion: 73 Resp: 2160
Ion Ratio Lower Upper
73 100
43 19.0 14.8 22.2
57 13.8 17.4 26.0#

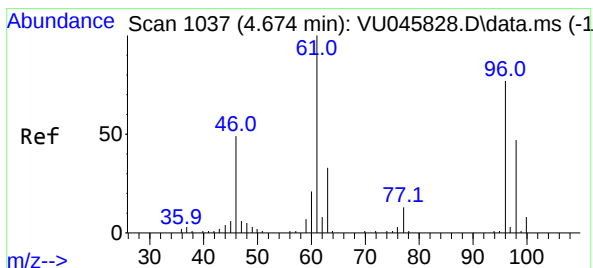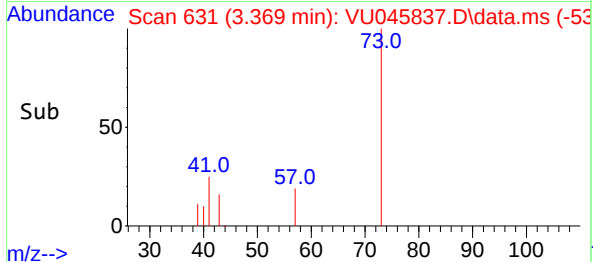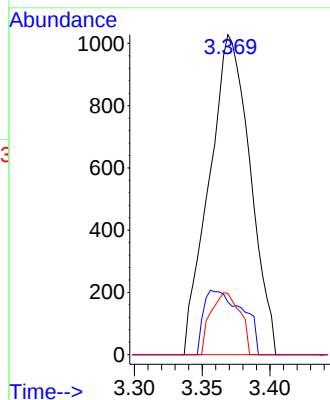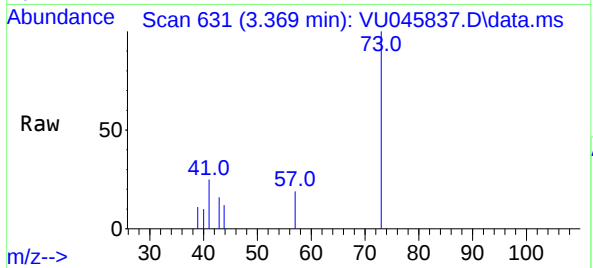

#22
cis-1,2-Dichloroethene
Concen: 0.731 ug/L
RT: 4.671 min Scan# 1036
Delta R.T. -0.003 min
Lab File: VU045837.D
Acq: 17 Nov 2021 14:01

Tgt Ion: 96 Resp: 4884
Ion Ratio Lower Upper
96 100
61 117.8 88.5 164.3
98 54.8 44.4 82.5

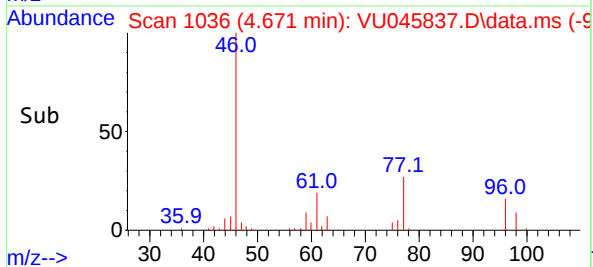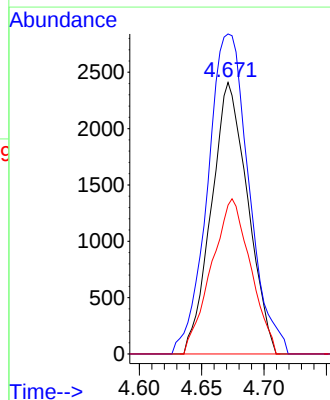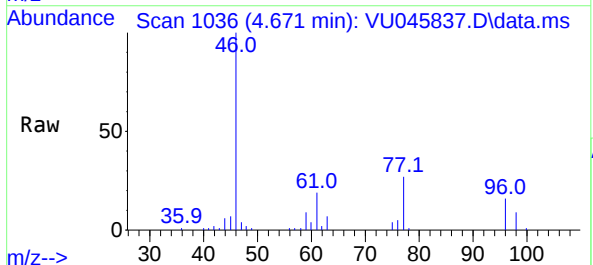




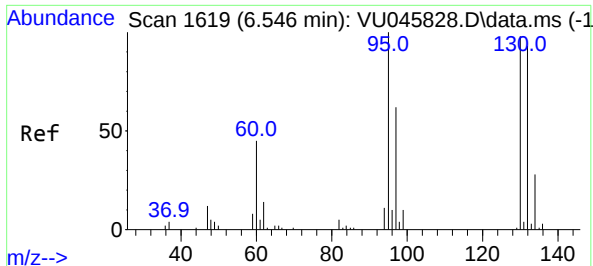


#34
Trichloroethene
Concen: 8.994 ug/L
RT: 6.546 min Scan# 1619
Delta R.T. 0.000 min
Lab File: VU045837.D
Acq: 17 Nov 2021 14:01

Instrument :
MSVOA_U
ClientSampleId :
BG1Z5

Tgt Ion: 95 Resp: 63688

Ion	Ratio	Lower	Upper
95	100		
97	62.8	46.5	86.5
132	92.1	65.1	120.9
130	95.8	67.3	124.9

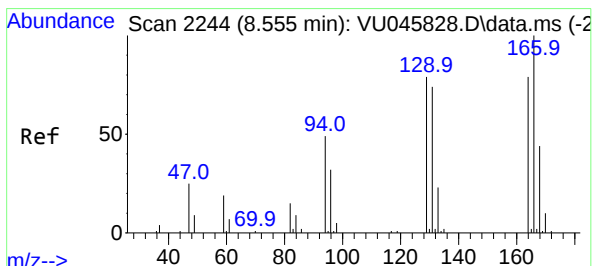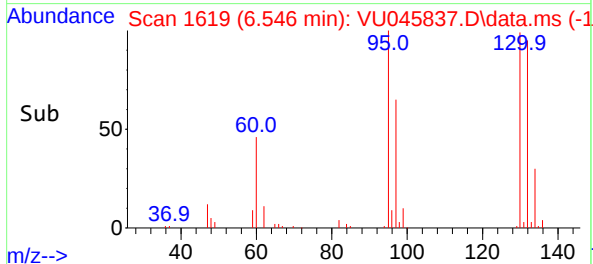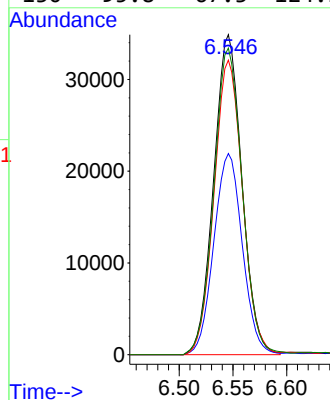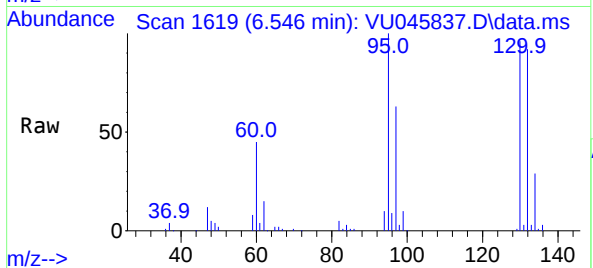

#47
Tetrachloroethene
Concen: 2.429 ug/L
RT: 8.555 min Scan# 2244
Delta R.T. 0.000 min
Lab File: VU045837.D
Acq: 17 Nov 2021 14:01

Tgt Ion: 164 Resp: 12039

Ion	Ratio	Lower	Upper
164	100		
129	96.4	71.8	133.4
131	97.1	68.5	127.3
166	126.8	94.1	174.8

