

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111721\
 Data File : VU045847.D
 Acq On : 17 Nov 2021 18:04
 Operator : SY/MD
 Sample : M4664-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4633

Quant Time: Nov 18 02:22:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 18 02:11:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	95072	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	101145	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	44982	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	38977	5.175	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	103.400%
7) Chloroethane-d5	1.919	69	28909	5.272	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.400%
11) 1,1-Dichloroethene-d2	2.572	65	15299	4.843	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	96.800%
20) 2-Butanone-d5	4.639	46	95399	47.260	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.520%
24) Chloroform-d	5.067	84	53840	4.290	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.800%
26) 1,2-Dichloroethane-d4	5.703	65	35703	4.849	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.000%
32) Benzene-d6	5.732	84	122509	4.398	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.000%
36) 1,2-Dichloropropane-d6	6.694	67	38732	4.412	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.200%
41) Toluene-d8	7.902	98	103791	4.119	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.400%
43) trans-1,3-Dichloroprop...	8.182	79	14110	3.959	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.200%
46) 2-Hexanone-d5	8.636	63	64770	40.381	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.760%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	32949	4.443	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.800%
66) 1,2-Dichlorobenzene-d4	12.195	152	38484	4.983	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.600%
Target Compounds						
13) Acetone	2.658	43	8293	6.980	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111721\
Data File : VU045847.D
Acq On : 17 Nov 2021 18:04
Operator : SY/MD
Sample : M4664-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4633

Quant Time: Nov 18 02:22:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 18 02:11:55 2021
Response via : Initial Calibration

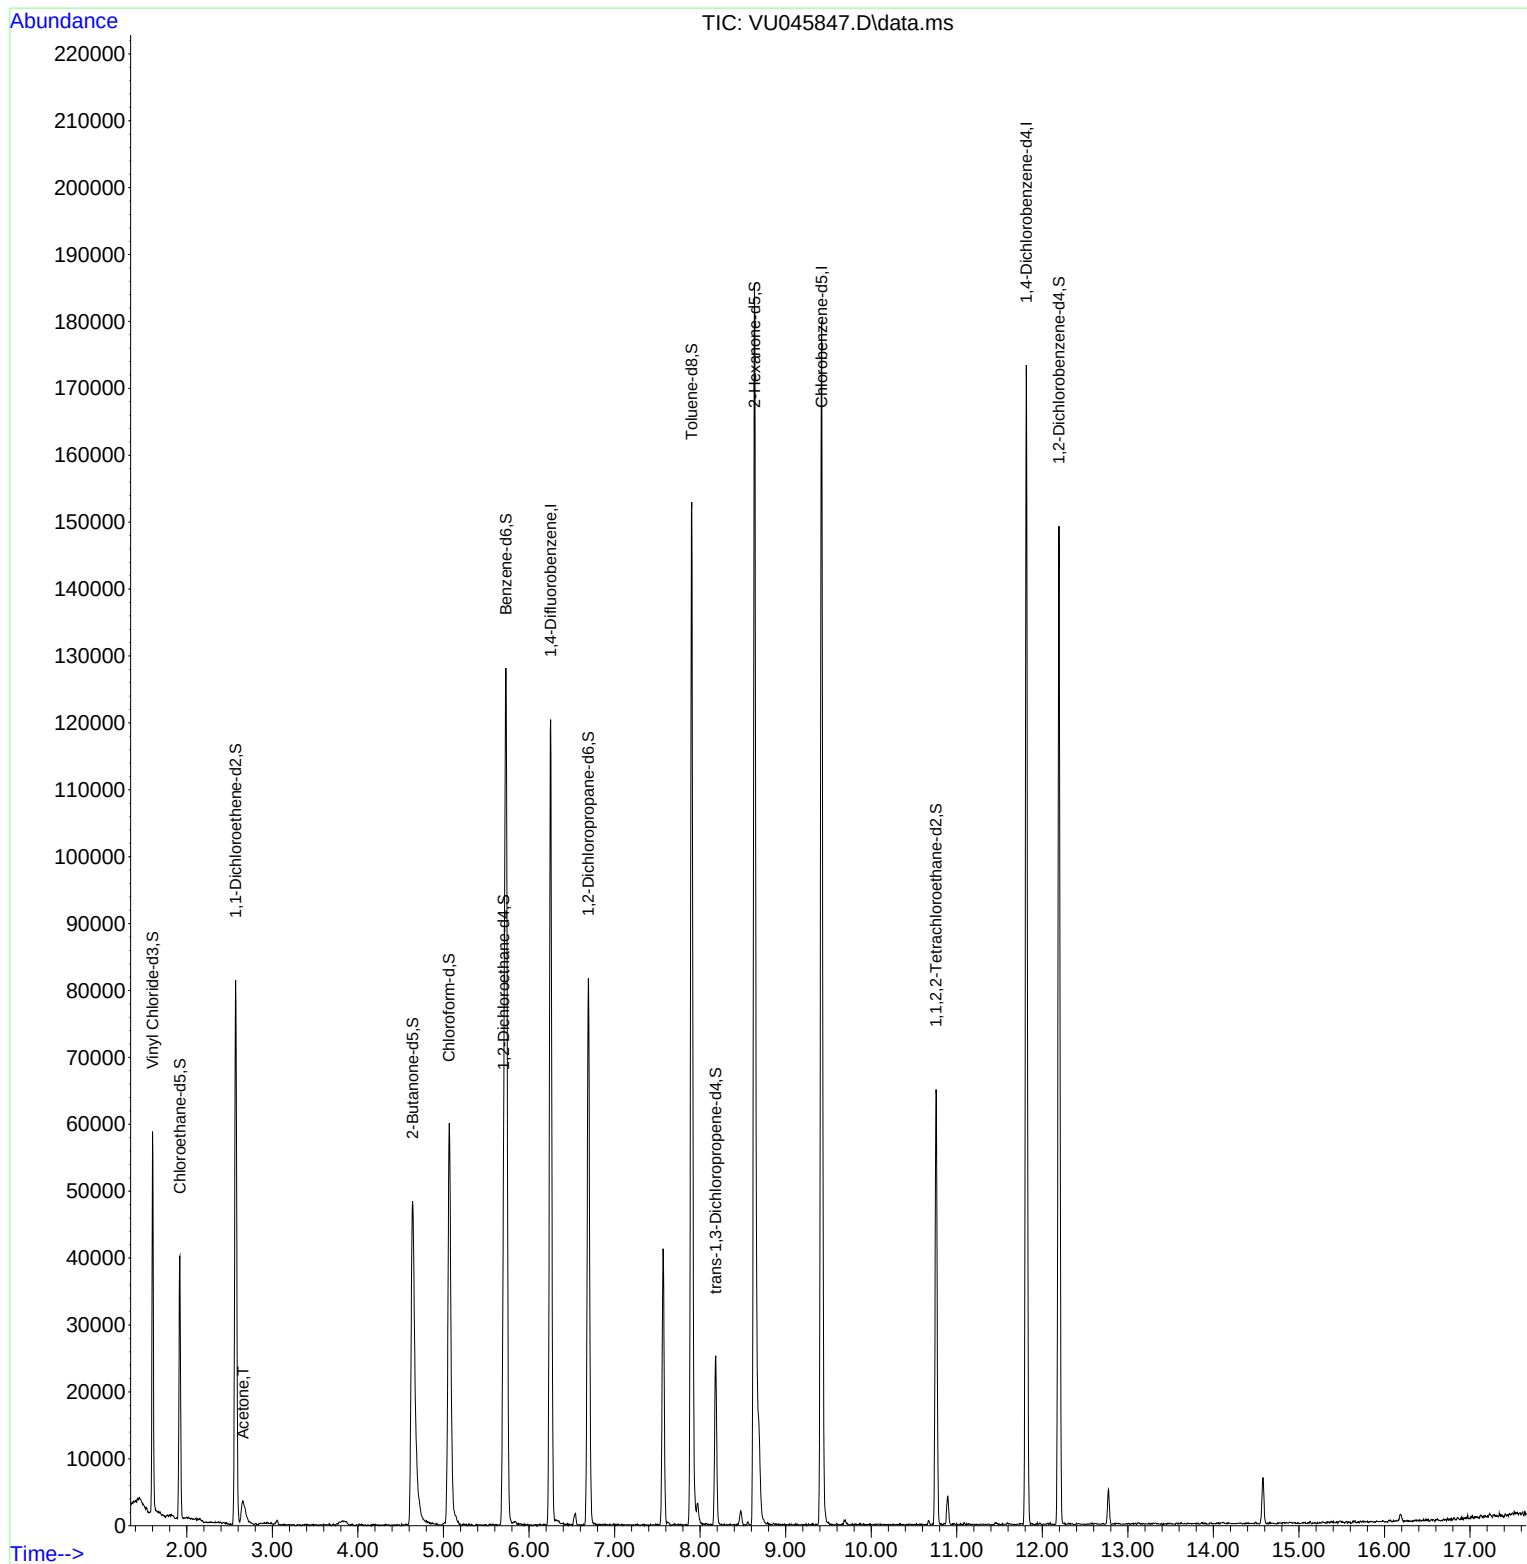

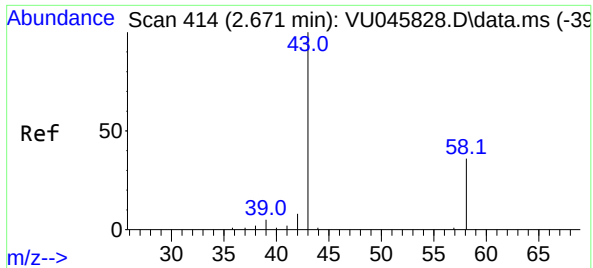

#13
Acetone
Concen: 6.980 ug/L
RT: 2.658 min Scan# 41
Delta R.T. -0.013 min
Lab File: VU045847.D
Acq: 17 Nov 2021 18:04

Instrument :
MSVOA_U
ClientSampleId :
H4633

Tgt Ion: 43 Resp: 8293
Ion Ratio Lower Upper
43 100
58 35.0 0.0 71.6

