

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111721\
 Data File : VU045852.D
 Acq On : 17 Nov 2021 20:04
 Operator : SY/MD
 Sample : M4664-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4676

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU045852.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	72	82	94	rBV	605851	690777	84.18%	15.626%
2	1.915	173	179	192	rVB	41668	55982	6.82%	1.266%
3	1.999	201	205	218	rVB	18829	23818	2.90%	0.539%
4	2.571	372	383	400	rVB	85088	137135	16.71%	3.102%
5	3.362	618	629	641	rBV4	11836	24477	2.98%	0.554%
6	4.671	1011	1036	1068	rBV2	322885	820593	100.00%	18.563%
7	5.066	1137	1159	1178	rBV	67371	150969	18.40%	3.415%
8	5.394	1250	1261	1272	rVB5	4140	8268	1.01%	0.187%
9	5.729	1343	1365	1394	rBV2	136657	365742	44.57%	8.274%
10	6.253	1513	1528	1544	rBV	123319	229357	27.95%	5.188%
11	6.546	1607	1619	1628	rBV3	4974	8876	1.08%	0.201%
12	6.693	1652	1665	1685	rBV	84992	162852	19.85%	3.684%
13	7.568	1926	1937	1959	rVB	42496	73691	8.98%	1.667%
14	7.902	2028	2041	2055	rBV	160979	280911	34.23%	6.355%
15	8.182	2117	2128	2142	rBV	25936	42552	5.19%	0.963%
16	8.635	2257	2269	2301	rBV	192965	392371	47.82%	8.876%
17	9.420	2499	2513	2530	rBV	184039	304225	37.07%	6.882%
18	10.758	2918	2929	2947	rBV	67221	107477	13.10%	2.431%
19	11.812	3245	3257	3277	rBV	179196	287054	34.98%	6.494%
20	12.195	3364	3376	3393	rVB	158512	253433	30.88%	5.733%




Sum of corrected areas: 4420560

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111721\
Data File : VU045852.D
Acq On : 17 Nov 2021 20:04
Operator : SY/MD
Sample : M4664-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4676

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

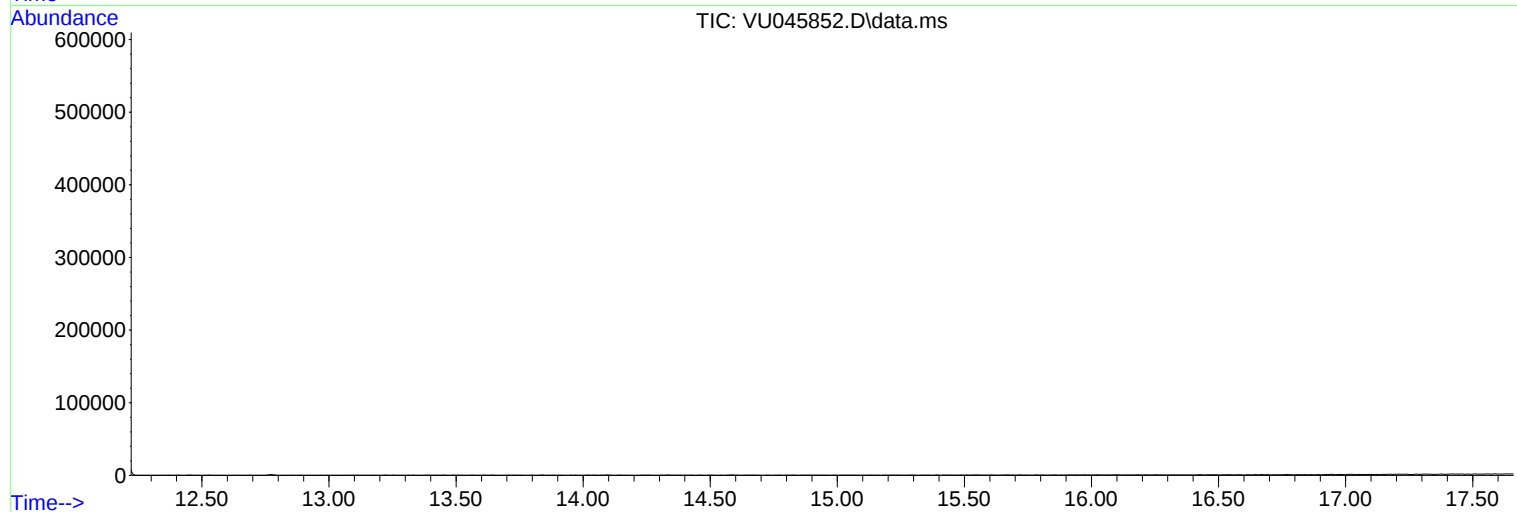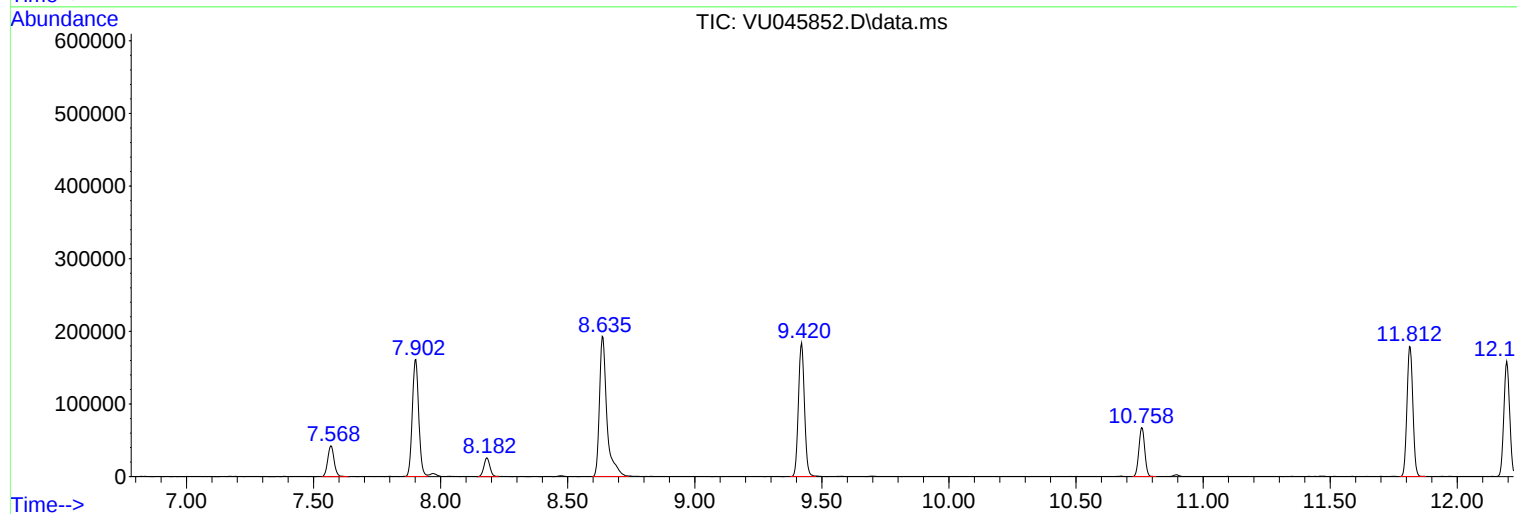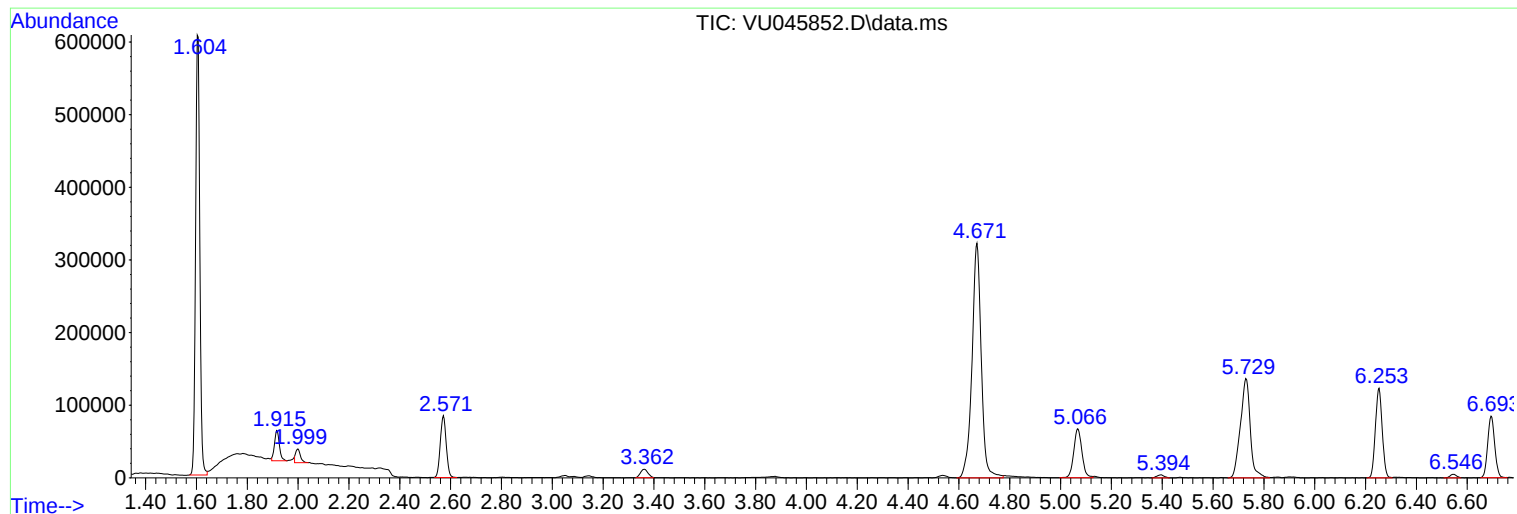

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111721\
Data File : VU045852.D
Acq On : 17 Nov 2021 20:04
Operator : SY/MD
Sample : M4664-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4676










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.999	0.52 ug/L	23818	1,4-Difluorobenzene	6.253

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Butane, 2-methyl-	72	C5H12	000078-78-4	72
2		Butane, 2-methyl-	72	C5H12	000078-78-4	72
3		3-Buten-1-ol	72	C4H8O	000627-27-0	32
4		Pentane	72	C5H12	000109-66-0	28
5		Pentane	72	C5H12	000109-66-0	25

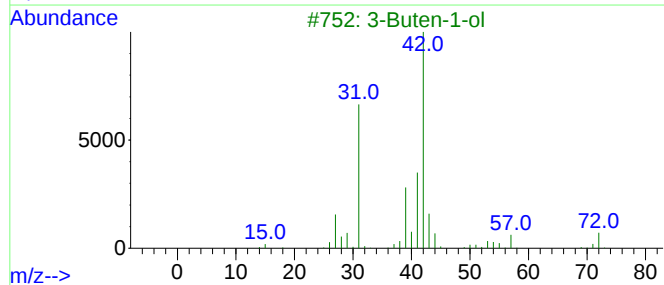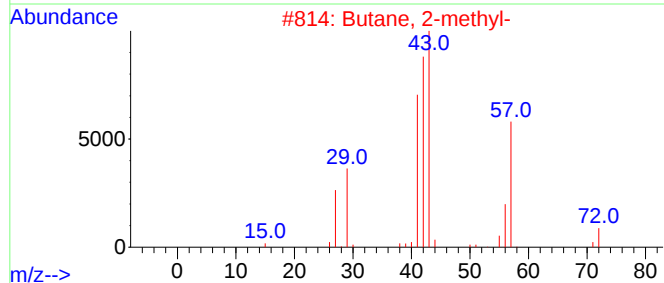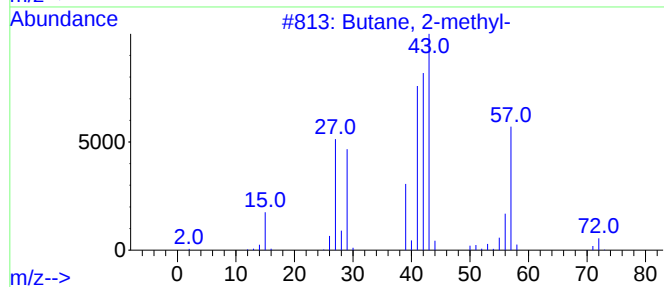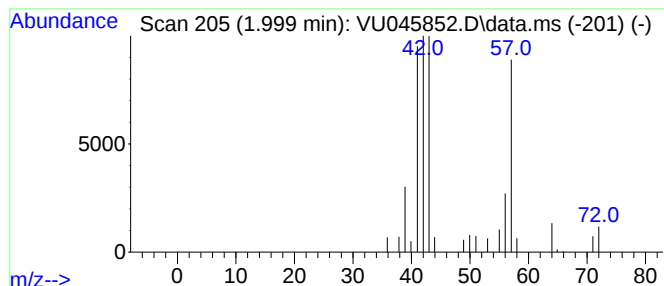

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111721\
Data File : VU045852.D
Acq On : 17 Nov 2021 20:04
Operator : SY/MD
Sample : M4664-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4676

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	1.999	0.5	ug/L	23818	1	6.253	229357	5.0