
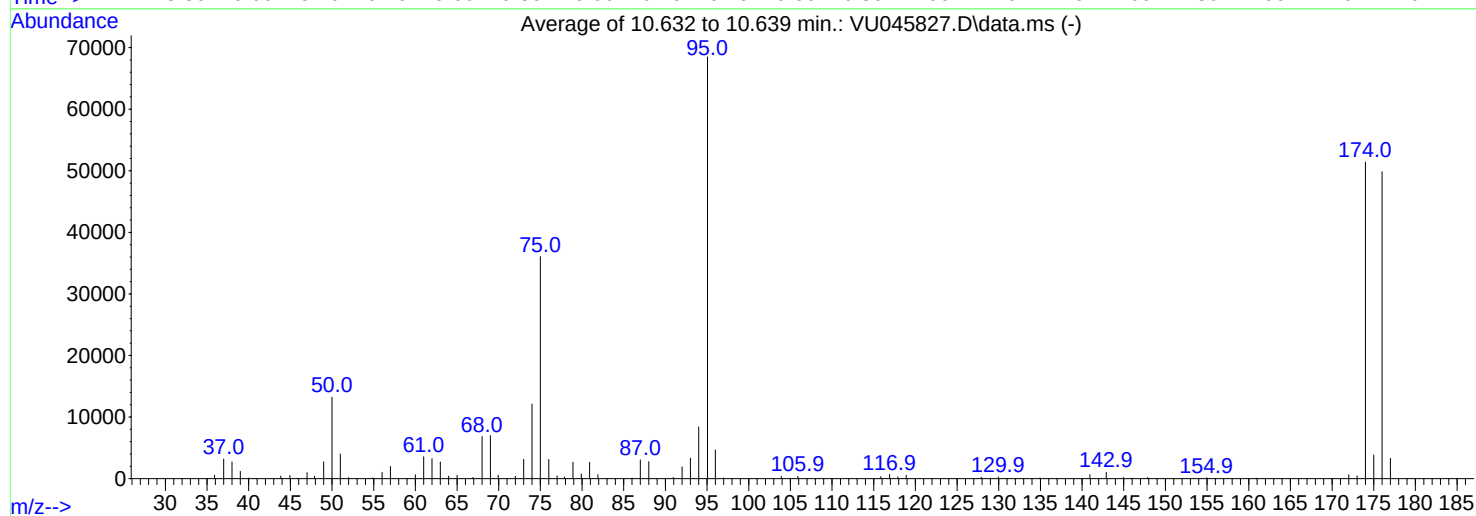


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111721\
 Data File : VU045827.D
 Acq On : 17 Nov 2021 09:26
 Operator : SY/MD
 Sample : BFB027
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB027

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Nov 22 03:50:15 2021

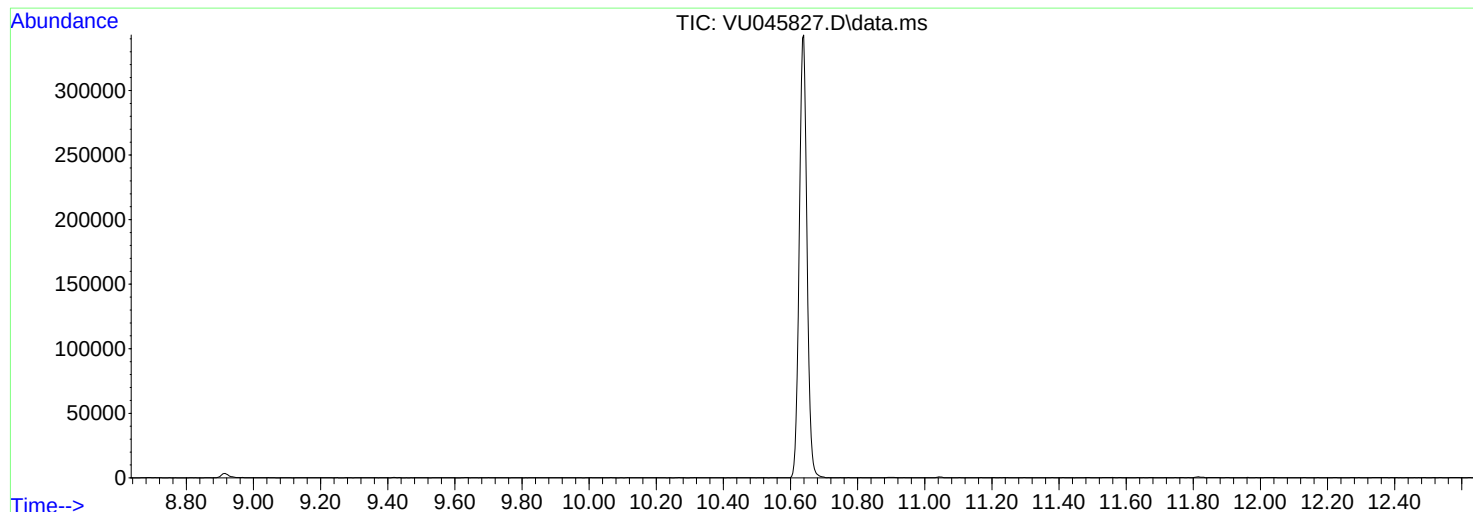

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	13238	PASS
75	95	30	80	52.7	36083	PASS
95	95	100	100	100.0	68507	PASS
96	95	5	9	6.8	4670	PASS
173	174	0.00	2	0.9	444	PASS
174	95	50	120	75.0	51392	PASS
175	174	5	9	7.5	3840	PASS
176	174	95	101	97.0	49845	PASS
177	176	5	9	6.7	3315	PASS

m/z	Abundance
35.90	570.0
37.00	3194.0
38.00	2754.0
39.00	1197.0
40.00	103.0
43.90	548.0
44.90	552.0
45.80	112.0
47.00	976.0
47.90	451.0
49.00	2829.0
50.00	13781.0
51.00	4048.0
52.00	178.0
54.90	176.0
56.00	1116.0
57.00	2022.0
60.00	657.0
61.00	3595.0
62.00	3382.0
63.00	2716.0
64.00	402.0
65.00	496.0
66.90	235.0
68.00	6811.0
69.00	7095.0
69.90	627.0
72.00	372.0
73.00	3255.0
74.00	12523.0
75.00	37664.0
76.00	3072.0
77.00	406.0
77.80	242.0
78.90	2822.0
79.90	813.0
80.90	2725.0
81.90	670.0
86.00	102.0
87.00	3436.0
88.00	2809.0
90.90	230.0
92.00	2016.0
93.00	3412.0
94.00	8752.0
95.10	70432.0
96.00	4869.0
97.00	110.0
103.90	347.0
104.90	100.0
105.90	425.0
115.90	333.0
116.90	654.0
117.90	307.0
118.90	497.0
127.90	251.0
129.00	109.0
129.90	301.0
130.90	105.0
134.90	109.0
137.00	116.0
140.90	711.0
142.90	1049.0
145.00	205.0
145.90	108.0
147.90	182.0
154.90	164.0
160.90	106.0
172.00	604.0
173.00	421.0
174.00	54528.0
175.00	4045.0
176.00	52432.0
177.00	3355.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

m/z	Abundance
43.80	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

m/z	Abundance
35.90	581.0
37.00	3093.0
38.00	2539.0
39.00	1133.0
40.00	106.0
43.90	492.0
45.00	462.0
47.00	943.0
47.90	330.0
49.00	2591.0
50.00	12265.0
51.00	3857.0
52.00	159.0
54.90	151.0
56.00	942.0
57.00	1862.0
60.00	607.0
61.00	3451.0
62.00	3077.0
63.00	2596.0
64.00	429.0
65.00	563.0
66.90	191.0
68.00	6608.0
69.00	6644.0
70.00	490.0
72.00	392.0
73.00	2964.0
74.00	11455.0
75.00	33360.0
76.00	3057.0
77.00	467.0
78.00	273.0
78.90	2448.0
79.90	754.0
80.90	2517.0
81.90	623.0
87.00	2566.0
88.00	2612.0
91.00	201.0
92.00	1775.0
93.00	3074.0
94.00	7812.0
95.00	64216.0
96.00	4290.0
97.00	139.0
103.90	381.0
105.90	336.0
115.80	323.0
116.90	659.0
117.90	248.0
118.90	562.0
127.90	208.0
130.00	266.0
135.00	116.0
141.00	589.0
142.90	1026.0
144.90	217.0
147.90	194.0
155.00	141.0
172.00	629.0
173.00	466.0
174.00	46776.0
175.00	3514.0
176.00	45656.0
177.00	3167.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

m/z	Abundance
35.90	599.0
37.00	3268.0
38.00	2819.0
39.00	1221.0
40.00	112.0
43.90	550.0
44.90	522.0
45.80	108.0
47.00	1017.0
47.90	404.0
49.00	2802.0
50.00	13667.0
51.00	4126.0
52.00	186.0
54.90	167.0
56.00	1073.0
57.00	2035.0
60.00	632.0
61.00	3677.0
62.00	3313.0
63.00	2778.0
64.00	437.0
65.00	569.0
66.90	200.0
68.00	7071.0
69.00	7225.0
69.90	587.0
72.00	408.0
73.00	3217.0
74.00	12462.0
75.00	37224.0
76.00	3257.0
77.00	451.0
77.90	288.0
78.90	2762.0
79.90	812.0
80.90	2748.0
81.90	662.0
86.00	103.0
87.00	3103.0
88.00	2843.0
91.00	232.0
92.00	1977.0
93.00	3468.0
94.00	8652.0
95.00	70872.0
96.00	4851.0
97.00	134.0
103.90	362.0
104.90	100.0
105.90	393.0
115.80	331.0
116.90	703.0
117.90	294.0
118.90	572.0
127.90	240.0
129.00	108.0
130.00	319.0
135.00	121.0
141.00	669.0
142.90	1047.0
144.90	231.0
145.90	121.0
147.90	200.0
154.90	156.0
160.90	113.0
172.00	667.0
173.00	446.0
174.00	52872.0
175.00	3960.0
176.00	51448.0
177.00	3423.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027