

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111722\
 Data File : VU051887.D
 Acq On : 17 Nov 2022 11:29
 Operator : JC/MD
 Sample : VU1117WBL03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK020

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

Signal : TIC: VU051887.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	37	44	52	rBV2	9993	14771	1.05%	0.123%
2	1.597	73	80	92	rBV	145982	162134	11.49%	1.355%
3	1.896	165	173	197	rVB	132766	195473	13.85%	1.633%
4	2.462	346	349	352	rBV2	499	447	0.03%	0.004%
5	2.494	357	359	364	rBV2	422	399	0.03%	0.003%
6	2.562	368	380	397	rBV	216080	351588	24.91%	2.938%
7	2.781	443	448	458	rVB3	896	1426	0.10%	0.012%
8	3.044	519	530	543	rBV2	7852	15358	1.09%	0.128%
9	3.186	559	574	592	rVB	15987	39698	2.81%	0.332%
10	3.510	670	675	678	rBV	307	261	0.02%	0.002%
11	3.803	763	766	772	rVB2	290	302	0.02%	0.003%
12	3.845	776	779	785	rVB2	302	299	0.02%	0.002%
13	3.916	795	801	803	rBV2	330	272	0.02%	0.002%
14	4.301	919	921	928	rVB2	349	337	0.02%	0.003%
15	4.388	944	948	953	rBV	283	269	0.02%	0.002%
16	4.543	991	996	1000	rBV2	263	307	0.02%	0.003%
17	4.616	1004	1019	1047	rBV	186695	456316	32.33%	3.813%
18	4.906	1104	1109	1114	rBV3	503	524	0.04%	0.004%
19	4.964	1124	1127	1130	rVB2	487	296	0.02%	0.002%
20	5.060	1139	1157	1179	rBV	286666	626050	44.35%	5.231%
21	5.292	1218	1229	1231	rBV5	1157	1625	0.12%	0.014%
22	5.366	1247	1252	1254	rBV2	774	654	0.05%	0.005%
23	5.462	1275	1282	1285	rBV	296	278	0.02%	0.002%
24	5.600	1322	1325	1332	rVB	319	321	0.02%	0.003%
25	5.719	1338	1362	1382	rBV2	506649	1411546	100.00%	11.794%
26	5.915	1421	1423	1429	rBV2	360	326	0.02%	0.003%
27	6.028	1455	1458	1464	rVB3	477	477	0.03%	0.004%
28	6.057	1464	1467	1470	rBV2	433	277	0.02%	0.002%
29	6.247	1511	1526	1547	rBV	555124	1061396	75.19%	8.868%
30	6.526	1606	1613	1625	rVB10	2483	5343	0.38%	0.045%
31	6.575	1625	1628	1631	rVB2	591	350	0.02%	0.003%
32	6.687	1649	1663	1689	rBV	362493	707646	50.13%	5.913%
33	6.832	1706	1708	1713	rVB2	600	474	0.03%	0.004%
34	6.867	1714	1719	1722	rBV	386	407	0.03%	0.003%
35	7.079	1781	1785	1793	rBV2	891	1149	0.08%	0.010%
36	7.118	1793	1797	1801	rVB	425	344	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111722\
 Data File : VU051887.D
 Acq On : 17 Nov 2022 11:29
 Operator : JC/MD
 Sample : VU1117WBL03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK020

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

37	7.186	1809	1818	1837	rVB4	6688	13048	0.92%	0.109%
38	7.513	1915	1920	1922	rBV2	281	274	0.02%	0.002%
39	7.562	1922	1935	1965	rVV	161708	287884	20.39%	2.405%
40	7.690	1965	1975	1984	rBV4	4311	7657	0.54%	0.064%
41	7.784	1998	2004	2006	rBV3	1009	1025	0.07%	0.009%
42	7.896	2025	2039	2060	rBV	523383	902174	63.91%	7.538%
43	8.131	2109	2112	2115	rVB2	475	301	0.02%	0.003%
44	8.176	2115	2126	2147	rBV	117659	197629	14.00%	1.651%
45	8.250	2147	2149	2155	rVB4	668	608	0.04%	0.005%
46	8.468	2211	2217	2221	rVV4	360	437	0.03%	0.004%
47	8.552	2236	2243	2249	rVB6	1313	1982	0.14%	0.017%
48	8.632	2255	2268	2300	rBV2	525826	995968	70.56%	8.322%
49	8.809	2321	2323	2330	rVB2	628	472	0.03%	0.004%
50	8.883	2344	2346	2348	rVB2	616	253	0.02%	0.002%
51	8.915	2348	2356	2358	rBV3	861	916	0.06%	0.008%
52	8.970	2370	2373	2377	rBV4	460	390	0.03%	0.003%
53	9.115	2414	2418	2422	rVB2	363	290	0.02%	0.002%
54	9.150	2425	2429	2431	rBV2	403	276	0.02%	0.002%
55	9.218	2446	2450	2451	rBV	392	263	0.02%	0.002%
56	9.230	2452	2454	2461	rVB2	394	373	0.03%	0.003%
57	9.295	2470	2474	2480	rVB3	303	340	0.02%	0.003%
58	9.330	2480	2485	2487	rBV2	368	274	0.02%	0.002%
59	9.414	2497	2511	2533	rBV	819889	1329234	94.17%	11.106%
60	9.684	2590	2595	2597	rBV	256	272	0.02%	0.002%
61	9.751	2613	2616	2621	rBV3	286	287	0.02%	0.002%
62	9.845	2642	2645	2650	rBV2	387	343	0.02%	0.003%
63	9.870	2650	2653	2656	rVB2	379	265	0.02%	0.002%
64	9.893	2656	2660	2663	rBV	283	237	0.02%	0.002%
65	10.095	2719	2723	2728	rBV3	321	393	0.03%	0.003%
66	10.250	2767	2771	2774	rBV2	311	244	0.02%	0.002%
67	10.295	2781	2785	2787	rBV	369	302	0.02%	0.003%
68	10.494	2842	2847	2851	rBV3	291	294	0.02%	0.002%
69	10.751	2911	2927	2948	rBV	667573	1074555	76.13%	8.978%
70	10.938	2979	2985	2990	rBV2	246	293	0.02%	0.002%
71	11.144	3047	3049	3056	rVB3	391	378	0.03%	0.003%
72	11.465	3146	3149	3151	rBV	348	246	0.02%	0.002%
73	11.526	3165	3168	3174	rVB2	329	275	0.02%	0.002%
74	11.684	3214	3217	3220	rBV2	354	273	0.02%	0.002%
75	11.745	3232	3236	3242	rVB3	524	481	0.03%	0.004%
76	11.809	3244	3256	3276	rBV	641059	1031809	73.10%	8.621%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111722\
 Data File : VU051887.D
 Acq On : 17 Nov 2022 11:29
 Operator : JC/MD
 Sample : VU1117WBL03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK020

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

77	12.057	3330	3333	3338	rBV3	350	339	0.02%	0.003%
78	12.189	3362	3374	3401	rVV	646835	1045615	74.08%	8.737%
79	12.349	3421	3424	3426	rBV2	699	426	0.03%	0.004%
80	12.417	3442	3445	3448	rBV3	418	296	0.02%	0.002%
81	12.478	3459	3464	3465	rBV3	684	627	0.04%	0.005%
82	12.967	3613	3616	3619	rBV2	504	338	0.02%	0.003%
83	13.227	3692	3697	3707	rBV4	902	1759	0.12%	0.015%
84	13.291	3712	3717	3719	rBV2	450	356	0.03%	0.003%
85	13.346	3731	3734	3737	rBV	565	345	0.02%	0.003%
86	13.433	3757	3761	3764	rBV2	413	405	0.03%	0.003%
87	13.610	3812	3816	3819	rBV3	448	364	0.03%	0.003%
88	13.780	3866	3869	3875	rVB2	497	374	0.03%	0.003%
89	13.825	3880	3883	3885	rBV2	410	292	0.02%	0.002%
90	13.841	3886	3888	3890	rBV2	621	344	0.02%	0.003%
91	14.092	3962	3966	3967	rBV	800	555	0.04%	0.005%
92	14.262	4016	4019	4022	rBV2	370	265	0.02%	0.002%
93	14.333	4036	4041	4043	rBV3	1107	846	0.06%	0.007%
94	14.349	4043	4046	4050	rVB3	870	665	0.05%	0.006%
95	14.471	4082	4084	4088	rBV2	416	334	0.02%	0.003%
96	14.722	4160	4162	4165	rVB2	532	249	0.02%	0.002%
97	15.436	4382	4384	4387	rBV2	589	306	0.02%	0.003%
98	15.632	4443	4445	4447	rBV2	582	262	0.02%	0.002%
99	15.693	4462	4464	4466	rBV	705	410	0.03%	0.003%
100	15.889	4523	4525	4527	rBV3	806	352	0.02%	0.003%




Sum of corrected areas: 11968279

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111722\
Data File : VU051887.D
Acq On : 17 Nov 2022 11:29
Operator : JC/MD
Sample : VU1117WBL03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK020

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

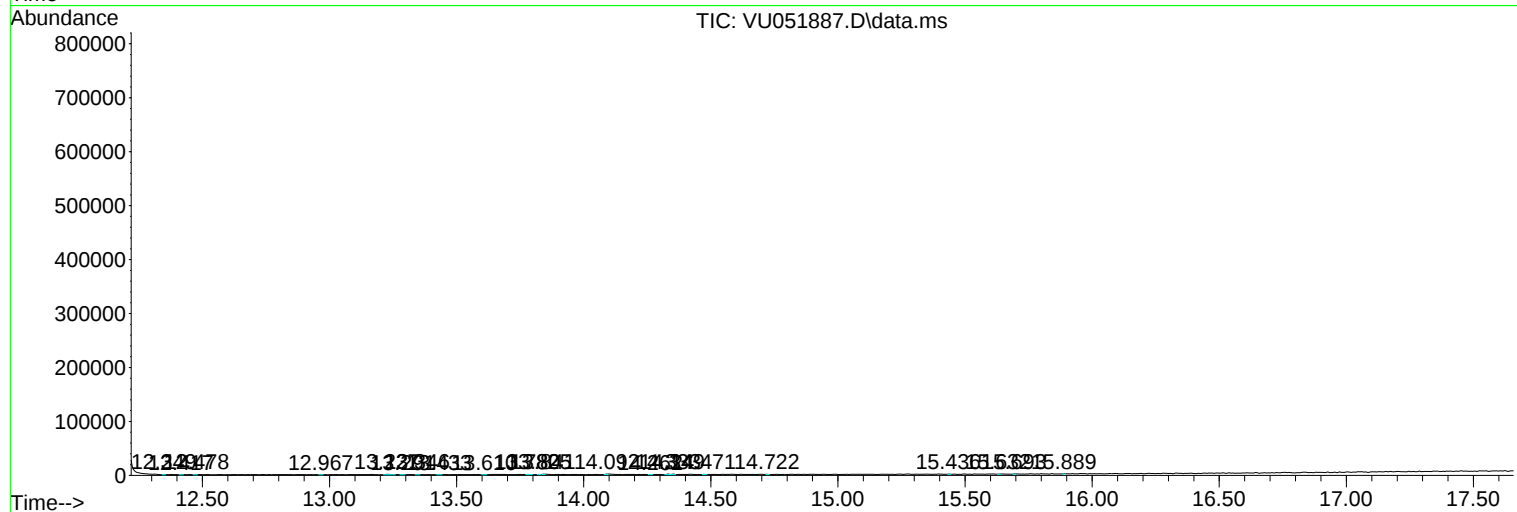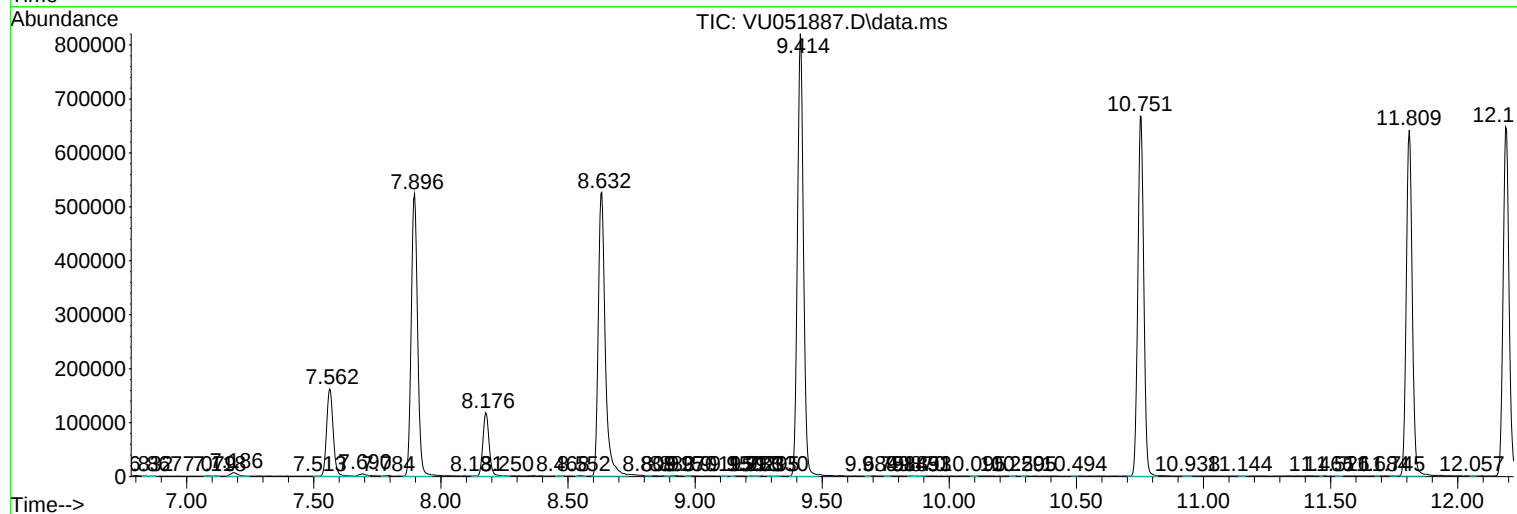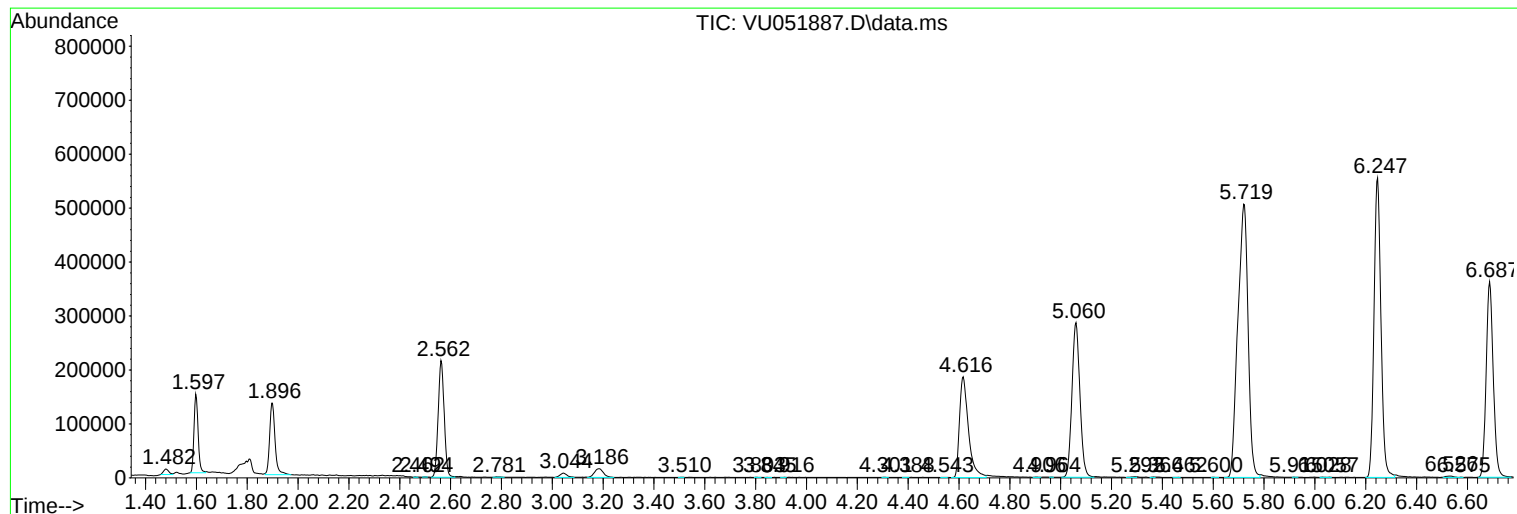

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111722\
Data File : VU051887.D
Acq On : 17 Nov 2022 11:29
Operator : JC/MD
Sample : VU1117WBL03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK020

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111722\
Data File : VU051887.D
Acq On : 17 Nov 2022 11:29
Operator : JC/MD
Sample : VU1117WBL03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK020

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc