

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111722\
 Data File : VU051888.D
 Acq On : 17 Nov 2022 11:53
 Operator : JC/MD
 Sample : VU1117WBL04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK021

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M

Title : VOC Analysis

Signal : TIC: VU051888.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rBV	132173	152430	11.19%	1.327%
2	1.903	167	175	196	rVB	121426	179251	13.16%	1.560%
3	2.501	359	361	365	rVB	929	595	0.04%	0.005%
4	2.565	365	381	396	rBV	194053	320585	23.53%	2.791%
5	2.700	420	423	428	rVB2	858	675	0.05%	0.006%
6	2.732	428	433	434	rBV3	365	301	0.02%	0.003%
7	2.748	434	438	439	rBV2	382	239	0.02%	0.002%
8	2.932	491	495	498	rBV3	345	271	0.02%	0.002%
9	3.044	520	530	544	rVV2	5517	10885	0.80%	0.095%
10	3.179	561	572	589	rVV	8632	18686	1.37%	0.163%
11	3.256	593	596	600	rBV2	272	232	0.02%	0.002%
12	3.298	606	609	611	rBV	417	324	0.02%	0.003%
13	3.385	633	636	644	rVB2	302	272	0.02%	0.002%
14	3.623	704	710	713	rBV2	391	384	0.03%	0.003%
15	4.208	888	892	896	rVB2	386	266	0.02%	0.002%
16	4.507	982	985	988	rVB2	404	254	0.02%	0.002%
17	4.616	1006	1019	1058	rBV	194080	481848	35.37%	4.195%
18	4.925	1109	1115	1118	rBV3	464	408	0.03%	0.004%
19	4.960	1123	1126	1132	rVB3	347	316	0.02%	0.003%
20	5.060	1139	1157	1179	rBV	274402	602270	44.21%	5.243%
21	5.272	1218	1223	1224	rVV2	534	483	0.04%	0.004%
22	5.288	1224	1228	1236	rVB4	1303	1616	0.12%	0.014%
23	5.372	1249	1254	1263	rVV2	740	908	0.07%	0.008%
24	5.407	1263	1265	1268	rVB	387	230	0.02%	0.002%
25	5.430	1268	1272	1277	rBV2	332	347	0.03%	0.003%
26	5.723	1340	1363	1396	rVV2	476828	1362327	100.00%	11.860%
27	6.005	1448	1451	1455	rVV2	371	310	0.02%	0.003%
28	6.060	1464	1468	1475	rVB2	436	542	0.04%	0.005%
29	6.118	1475	1486	1489	rBV3	715	1061	0.08%	0.009%
30	6.157	1494	1498	1503	rBV2	488	456	0.03%	0.004%
31	6.247	1512	1526	1551	rBV	520742	1000895	73.47%	8.713%
32	6.526	1605	1613	1622	rBV7	2709	4575	0.34%	0.040%
33	6.591	1629	1633	1634	rBV	479	274	0.02%	0.002%
34	6.623	1639	1643	1646	rVB	408	300	0.02%	0.003%
35	6.687	1646	1663	1687	rBV	352358	685944	50.35%	5.972%
36	6.790	1693	1695	1698	rBV5	336	249	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111722\
 Data File : VU051888.D
 Acq On : 17 Nov 2022 11:53
 Operator : JC/MD
 Sample : VU1117WBL04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK021

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

37	6.806	1698	1700	1703	rVV3	452	303	0.02%	0.003%
38	6.877	1718	1722	1727	rVB2	468	428	0.03%	0.004%
39	6.967	1747	1750	1757	rVB2	430	473	0.03%	0.004%
40	7.185	1809	1818	1828	rBV4	6783	11732	0.86%	0.102%
41	7.279	1841	1847	1848	rBV2	522	464	0.03%	0.004%
42	7.562	1923	1935	1960	rVV	155860	281120	20.64%	2.447%
43	7.652	1960	1963	1966	rVV2	514	379	0.03%	0.003%
44	7.687	1966	1974	1989	rVV3	4231	7773	0.57%	0.068%
45	7.790	2000	2006	2010	rBV2	664	643	0.05%	0.006%
46	7.896	2025	2039	2068	rBV	486292	845652	62.07%	7.362%
47	8.176	2113	2126	2144	rBV	111597	193059	14.17%	1.681%
48	8.272	2153	2156	2160	rBV3	326	256	0.02%	0.002%
49	8.327	2169	2173	2179	rVB4	634	638	0.05%	0.006%
50	8.475	2215	2219	2222	rBV	443	355	0.03%	0.003%
51	8.549	2238	2242	2248	rVV4	831	815	0.06%	0.007%
52	8.629	2253	2267	2298	rBV2	540363	1016993	74.65%	8.854%
53	8.854	2335	2337	2344	rVB5	675	643	0.05%	0.006%
54	8.909	2349	2354	2356	rVB3	549	494	0.04%	0.004%
55	9.218	2446	2450	2453	rBV2	260	247	0.02%	0.002%
56	9.369	2493	2497	2498	rBV2	358	253	0.02%	0.002%
57	9.414	2498	2511	2533	rBV	765232	1264917	92.85%	11.012%
58	9.632	2576	2579	2582	rVB2	395	242	0.02%	0.002%
59	9.764	2618	2620	2627	rVB2	324	255	0.02%	0.002%
60	9.800	2627	2631	2634	rBV2	369	361	0.03%	0.003%
61	9.861	2646	2650	2652	rBV	338	243	0.02%	0.002%
62	9.877	2653	2655	2663	rVB2	398	339	0.02%	0.003%
63	10.099	2715	2724	2726	rBV2	336	427	0.03%	0.004%
64	10.134	2731	2735	2739	rBV2	353	300	0.02%	0.003%
65	10.153	2739	2741	2747	rVB2	342	279	0.02%	0.002%
66	10.401	2815	2818	2822	rVB2	443	357	0.03%	0.003%
67	10.427	2822	2826	2829	rBV2	410	411	0.03%	0.004%
68	10.568	2866	2870	2873	rBV	336	255	0.02%	0.002%
69	10.603	2878	2881	2883	rBV2	474	302	0.02%	0.003%
70	10.754	2914	2928	2950	rBV	664601	1058099	77.67%	9.211%
71	10.899	2969	2973	2977	rVB3	556	418	0.03%	0.004%
72	11.060	3020	3023	3025	rBV2	440	243	0.02%	0.002%
73	11.153	3049	3052	3055	rVB	500	300	0.02%	0.003%
74	11.221	3068	3073	3076	rBV2	307	345	0.03%	0.003%
75	11.314	3099	3102	3106	rVB3	370	263	0.02%	0.002%
76	11.513	3158	3164	3173	rBV2	303	422	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111722\
 Data File : VU051888.D
 Acq On : 17 Nov 2022 11:53
 Operator : JC/MD
 Sample : VU1117WBL04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK021

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
 Title : VOC Analysis

77	11.571	3179	3182	3185	rBV	337	234	0.02%	0.002%
78	11.809	3243	3256	3283	rBV	599175	974265	71.51%	8.482%
79	12.192	3360	3375	3399	rBV	595967	980598	71.98%	8.537%
80	12.446	3450	3454	3457	rBV3	654	639	0.05%	0.006%
81	12.645	3512	3516	3520	rBV	662	571	0.04%	0.005%
82	12.700	3530	3533	3536	rBV3	484	357	0.03%	0.003%
83	12.851	3578	3580	3585	rVB2	560	400	0.03%	0.003%
84	12.912	3594	3599	3600	rBV	647	426	0.03%	0.004%
85	13.356	3735	3737	3741	rVB2	418	281	0.02%	0.002%
86	13.404	3750	3752	3756	rBV	369	264	0.02%	0.002%
87	13.481	3774	3776	3780	rVB	451	259	0.02%	0.002%
88	13.500	3780	3782	3785	rBV	401	276	0.02%	0.002%
89	13.584	3806	3808	3813	rBV2	406	317	0.02%	0.003%
90	13.623	3817	3820	3822	rBV2	384	259	0.02%	0.002%
91	13.748	3856	3859	3864	rBV2	709	585	0.04%	0.005%
92	14.246	4008	4014	4018	rBV3	793	948	0.07%	0.008%
93	14.336	4038	4042	4048	rVB3	1010	922	0.07%	0.008%
94	14.574	4114	4116	4119	rBV2	446	265	0.02%	0.002%
95	14.603	4123	4125	4127	rBV2	405	238	0.02%	0.002%
96	14.651	4137	4140	4143	rBV2	558	404	0.03%	0.004%
97	14.709	4153	4158	4161	rBV2	447	467	0.03%	0.004%
98	14.812	4187	4190	4194	rBV	513	363	0.03%	0.003%
99	14.918	4220	4223	4227	rBV	544	469	0.03%	0.004%
100	15.179	4301	4304	4306	rBV	604	461	0.03%	0.004%




Sum of corrected areas: 11486775

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111722\
Data File : VU051888.D
Acq On : 17 Nov 2022 11:53
Operator : JC/MD
Sample : VU1117WBL04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

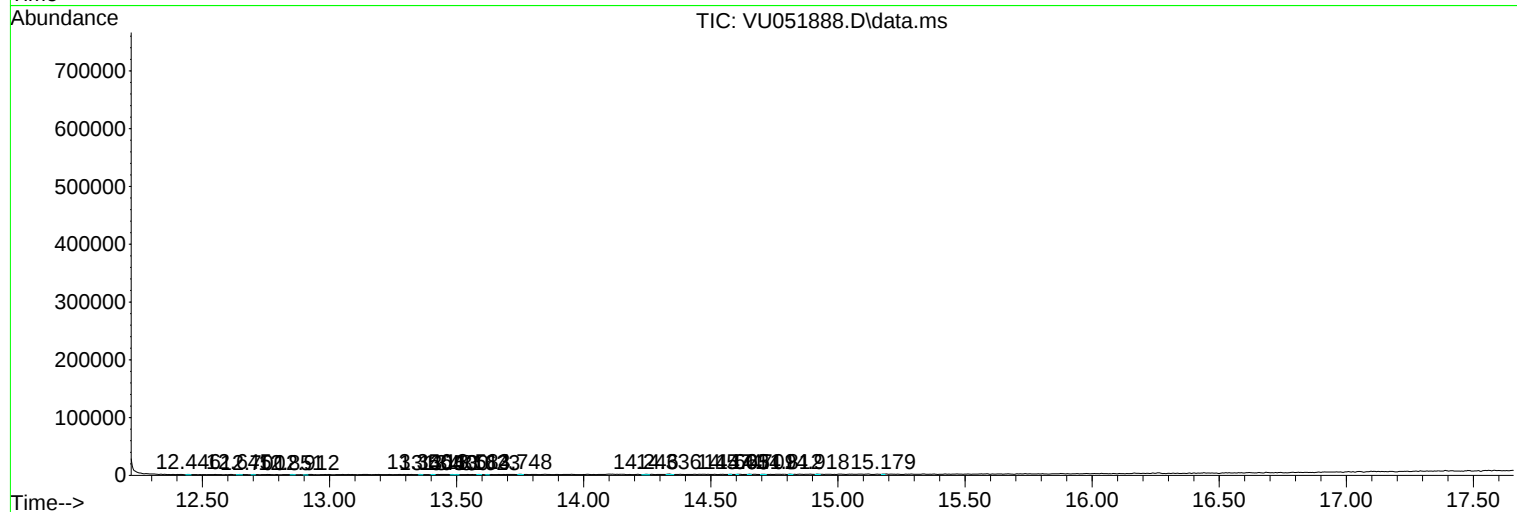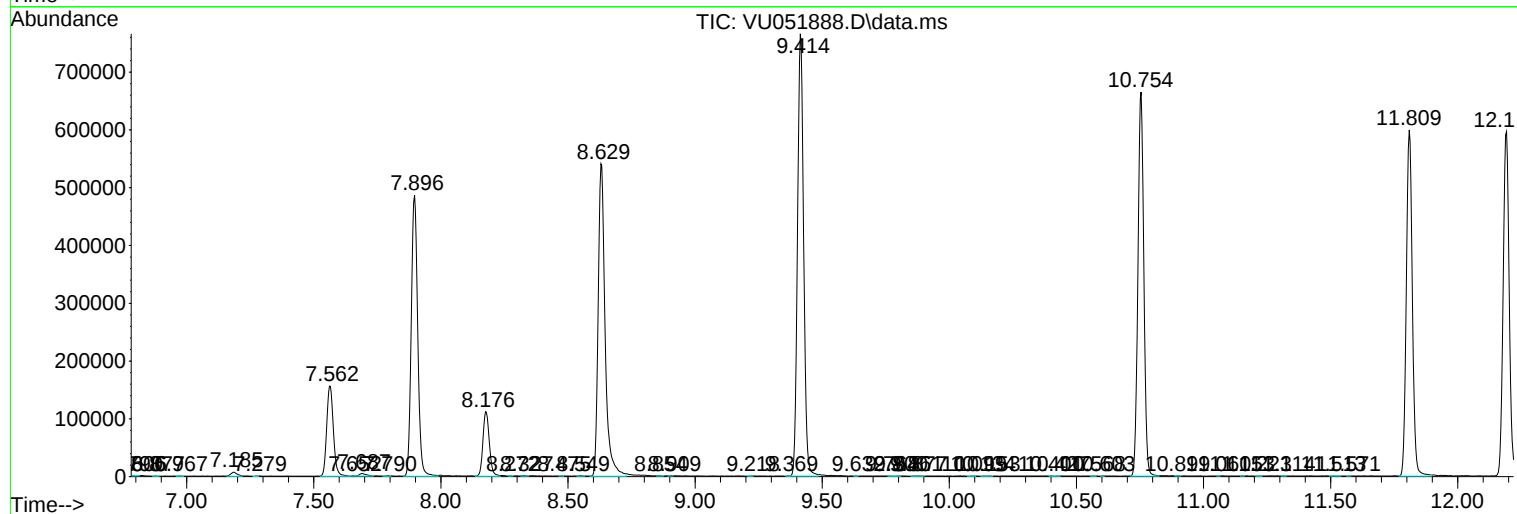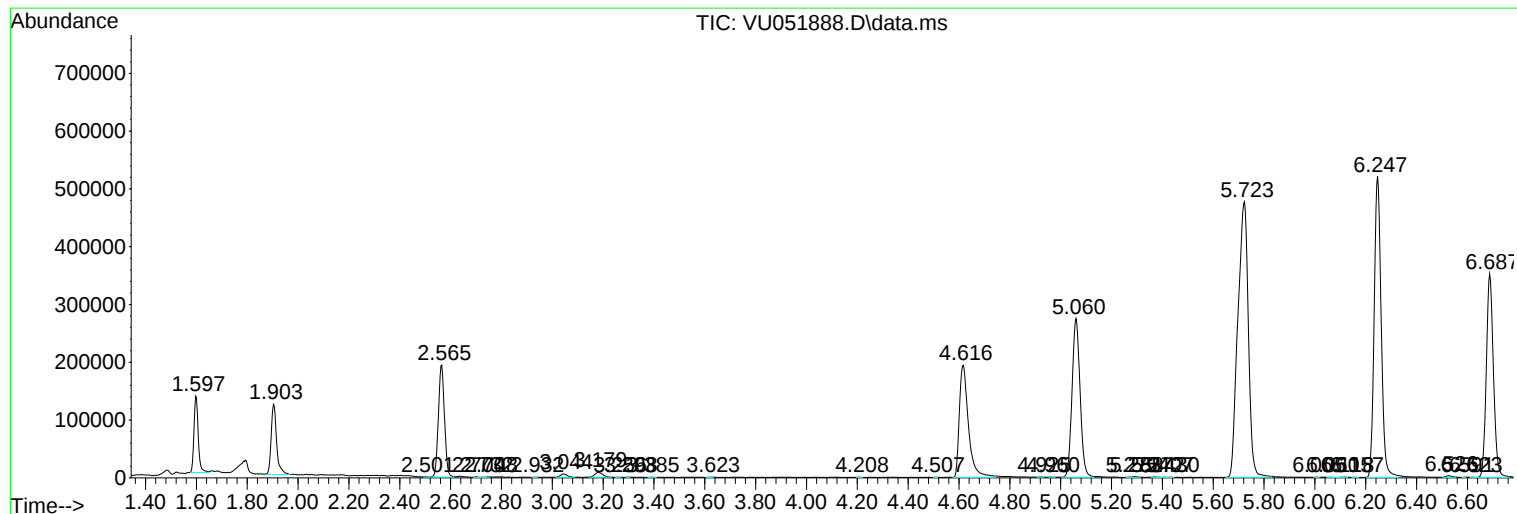

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111722\
Data File : VU051888.D
Acq On : 17 Nov 2022 11:53
Operator : JC/MD
Sample : VU1117WBL04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111722\
Data File : VU051888.D
Acq On : 17 Nov 2022 11:53
Operator : JC/MD
Sample : VU1117WBL04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------