


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111722\
Data File : VU051883.D
Acq On : 17 Nov 2022 09:26
Operator : JC/MD
Sample : BFB144
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB144

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Title : VOC Analysis
Last Update : Fri Nov 18 00:53:49 2022

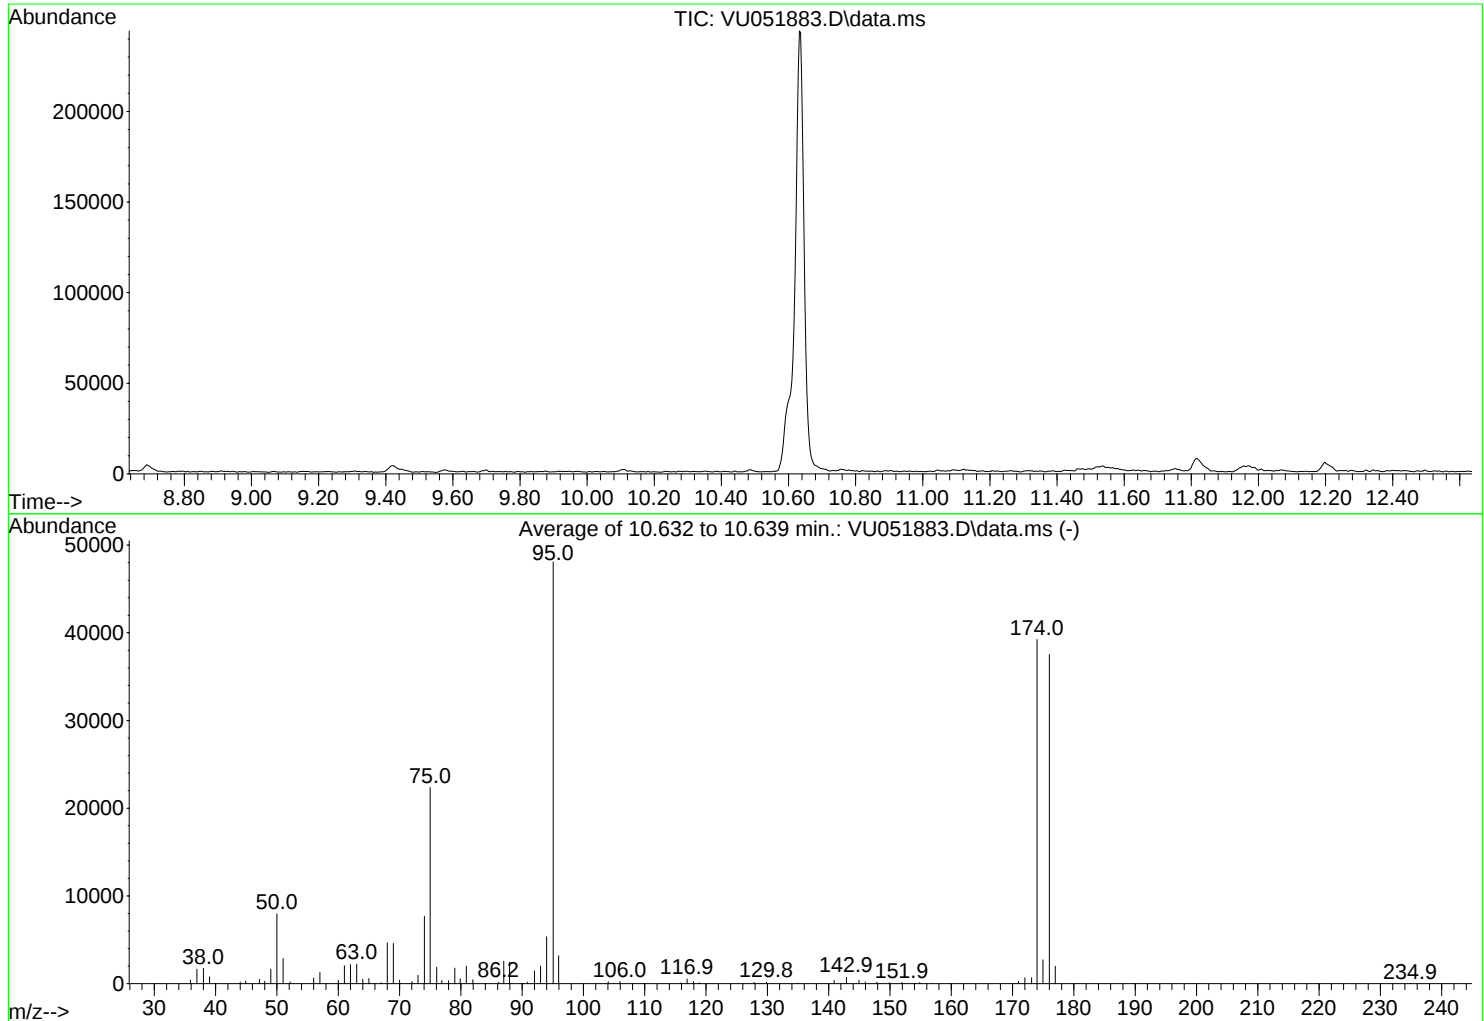

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.5	7948	PASS
75	95	30	80	46.5	22374	PASS
95	95	100	100	100.0	48093	PASS
96	95	5	9	6.6	3172	PASS
173	174	0.00	2	1.7	685	PASS
174	95	50	120	81.6	39235	PASS
175	174	5	9	6.9	2724	PASS
176	174	95	101	95.7	37531	PASS
177	176	5	9	5.3	1990	PASS

m/z	Abundance
40.00	364.0
44.00	864.0
44.90	187.0
59.00	160.0
73.10	955.0
74.00	183.0
75.00	207.0
95.90	129.0
103.00	259.0
105.00	162.0
115.00	180.0
118.90	208.0
124.90	536.0
126.10	127.0
133.00	1346.0
133.80	201.0
146.90	178.0
149.90	127.0
163.00	204.0
165.10	155.0
177.00	414.0
178.10	110.0
178.90	306.0
188.90	116.0
191.00	968.0
191.90	211.0
193.00	991.0
193.90	283.0
195.10	151.0
202.80	113.0
205.10	279.0
207.00	831.0
208.00	152.0
249.00	702.0
250.00	234.0
251.00	340.0
265.10	1223.0
266.00	556.0
267.10	402.0
281.10	12838.0
282.10	3844.0
283.10	2659.0
284.10	356.0
285.20	206.0

Instrument :
MSVOA_U
ClientSampleId :
BFB144

m/z	Abundance
35.90	429.0
37.00	1741.0
38.00	1772.0
39.00	782.0
40.00	357.0
44.00	1013.0
45.00	501.0
47.20	421.0
48.00	237.0
49.00	1816.0
50.00	7844.0
51.00	2884.0
52.10	159.0
56.00	612.0
57.00	1364.0
59.90	482.0
61.00	2047.0
62.00	2306.0
63.00	2279.0
64.00	533.0
65.00	545.0
67.00	106.0
68.00	4618.0
69.00	4652.0
69.90	374.0
72.00	263.0
73.00	1892.0
74.10	7937.0
75.00	23360.0
76.00	1984.0
76.90	428.0
77.90	342.0
79.00	1993.0
79.90	552.0
80.90	2030.0
82.00	493.0
86.10	195.0
87.00	2512.0
88.00	2515.0
90.90	159.0
92.00	1511.0
93.00	2049.0
94.00	5571.0
95.00	48776.0
96.00	3582.0
103.00	102.0
104.00	272.0
104.90	234.0
106.00	245.0
114.90	139.0
115.90	142.0
116.90	504.0
117.90	231.0
118.90	358.0
124.90	121.0
127.80	144.0
129.80	166.0
133.00	183.0
135.00	158.0
140.90	375.0
142.90	796.0
144.90	427.0
145.90	193.0
147.90	157.0
149.90	222.0
152.00	131.0
154.80	142.0
156.90	117.0
171.00	235.0
172.00	731.0
173.10	790.0
174.00	40520.0
174.90	2863.0
176.00	38472.0
176.90	2422.0
191.10	174.0
193.00	267.0
207.00	200.0
234.90	107.0
249.10	105.0
250.90	148.0
265.00	141.0
267.10	118.0
281.10	2228.0
282.00	764.0
283.10	364.0
284.10	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB144

m/z	Abundance
35.90	420.0
37.00	1672.0
38.00	1801.0
39.00	792.0
40.00	344.0
44.00	1047.0
44.90	488.0
47.10	494.0
48.00	294.0
49.00	1674.0
50.00	8186.0
51.00	2988.0
52.20	201.0
56.00	652.0
57.00	1308.0
60.00	391.0
61.00	2124.0
62.00	2284.0
63.00	2297.0
64.00	516.0
65.00	593.0
67.00	128.0
68.00	4801.0
69.00	4670.0
70.00	417.0
72.00	237.0
73.00	1987.0
74.10	8198.0
75.00	23344.0
76.00	1861.0
76.90	361.0
78.00	328.0
79.00	1821.0
79.90	594.0
80.90	2086.0
82.00	473.0
86.20	202.0
87.00	2689.0
87.90	2550.0
90.90	161.0
92.00	1507.0
93.00	1997.0
94.00	5547.0
95.00	49688.0
96.00	3394.0
104.10	199.0
104.90	207.0
105.90	234.0
114.90	100.0
115.90	119.0
116.90	541.0
117.90	227.0
119.00	270.0
124.90	125.0
127.80	152.0
129.90	185.0
132.90	124.0
140.90	364.0
141.90	103.0
142.90	751.0
145.00	421.0
146.00	184.0
147.80	182.0
149.90	223.0
151.90	128.0
154.80	143.0
170.90	265.0
172.00	698.0
173.10	719.0
174.00	40464.0
175.00	2790.0
176.00	38672.0
176.90	2476.0
191.10	148.0
193.00	126.0
207.00	156.0
264.90	109.0
281.10	1578.0
282.00	559.0
283.10	214.0

Instrument :
MSVOA_U
ClientSampleId :
BFB144

m/z	Abundance
35.90	314.0
36.90	1520.0
38.00	1612.0
39.00	773.0
40.00	327.0
44.00	1108.0
44.90	429.0
47.10	560.0
48.00	312.0
49.00	1455.0
50.00	7813.0
51.00	2748.0
52.20	199.0
56.00	650.0
57.00	1141.0
60.10	280.0
61.00	1961.0
62.00	1953.0
63.00	2023.0
64.00	426.0
65.00	595.0
67.00	106.0
68.00	4548.0
69.00	4406.0
70.10	390.0
72.10	227.0
73.00	1833.0
74.10	7409.0
75.00	21040.0
76.10	1758.0
76.90	255.0
78.10	316.0
79.00	1523.0
79.90	554.0
80.90	1902.0
81.90	427.0
86.10	122.0
87.00	2470.0
87.90	2195.0
90.80	155.0
92.00	1306.0
93.00	1959.0
94.00	4926.0
95.10	45816.0
96.00	2928.0
104.10	193.0
104.90	163.0
105.90	219.0
116.90	560.0
118.00	197.0
118.80	247.0
124.90	141.0
127.90	152.0
129.90	184.0
140.90	365.0
142.90	648.0
145.00	316.0
146.00	182.0
147.90	180.0
149.90	253.0
151.90	146.0
154.90	106.0
170.90	247.0
172.00	617.0
173.10	545.0
174.00	36720.0
175.00	2520.0
176.00	35448.0
177.00	2313.0
207.00	116.0
281.10	1105.0
282.00	408.0
283.00	130.0

Instrument :
MSVOA_U
ClientSampleId :
BFB144