

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111723\
 Data File : VU056433.D
 Acq On : 17 Nov 2023 11:34
 Operator : MD/SY
 Sample : 05389-03
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YCGB7

Quant Time: Nov 17 23:19:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 17 23:14:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	268118	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	258771	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	114299	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	61621	3.073	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	61.400%
7) Chloroethane-d5	1.907	69	55025	3.579	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	71.600%
11) 1,1-Dichloroethene-d2	2.560	65	29912	3.380	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.600%
20) 2-Butanone-d5	4.624	46	195665	48.930	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.860%
24) Chloroform-d	5.055	84	160823	4.146	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.000%
26) 1,2-Dichloroethane-d4	5.698	65	80965	4.517	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.400%
32) Benzene-d6	5.721	84	304559	3.950	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.000%
36) 1,2-Dichloropropane-d6	6.685	67	101153	4.353	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.000%
41) Toluene-d8	7.894	98	250296	3.676	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.600%
43) trans-1,3-Dichloroprop...	8.177	79	34892	3.915	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.400%
46) 2-Hexanone-d5	8.631	63	154031	43.982	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.960%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	72332	4.356	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.200%
66) 1,2-Dichlorobenzene-d4	12.190	152	91902	4.352	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	87.000%
Target Compounds						
					Qvalue	
13) Acetone	2.631	43	52847	15.517	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111723\
Data File : VU056433.D
Acq On : 17 Nov 2023 11:34
Operator : MD/SY
Sample : 05389-03
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YCGB7

Quant Time: Nov 17 23:19:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 17 23:14:39 2023
Response via : Initial Calibration

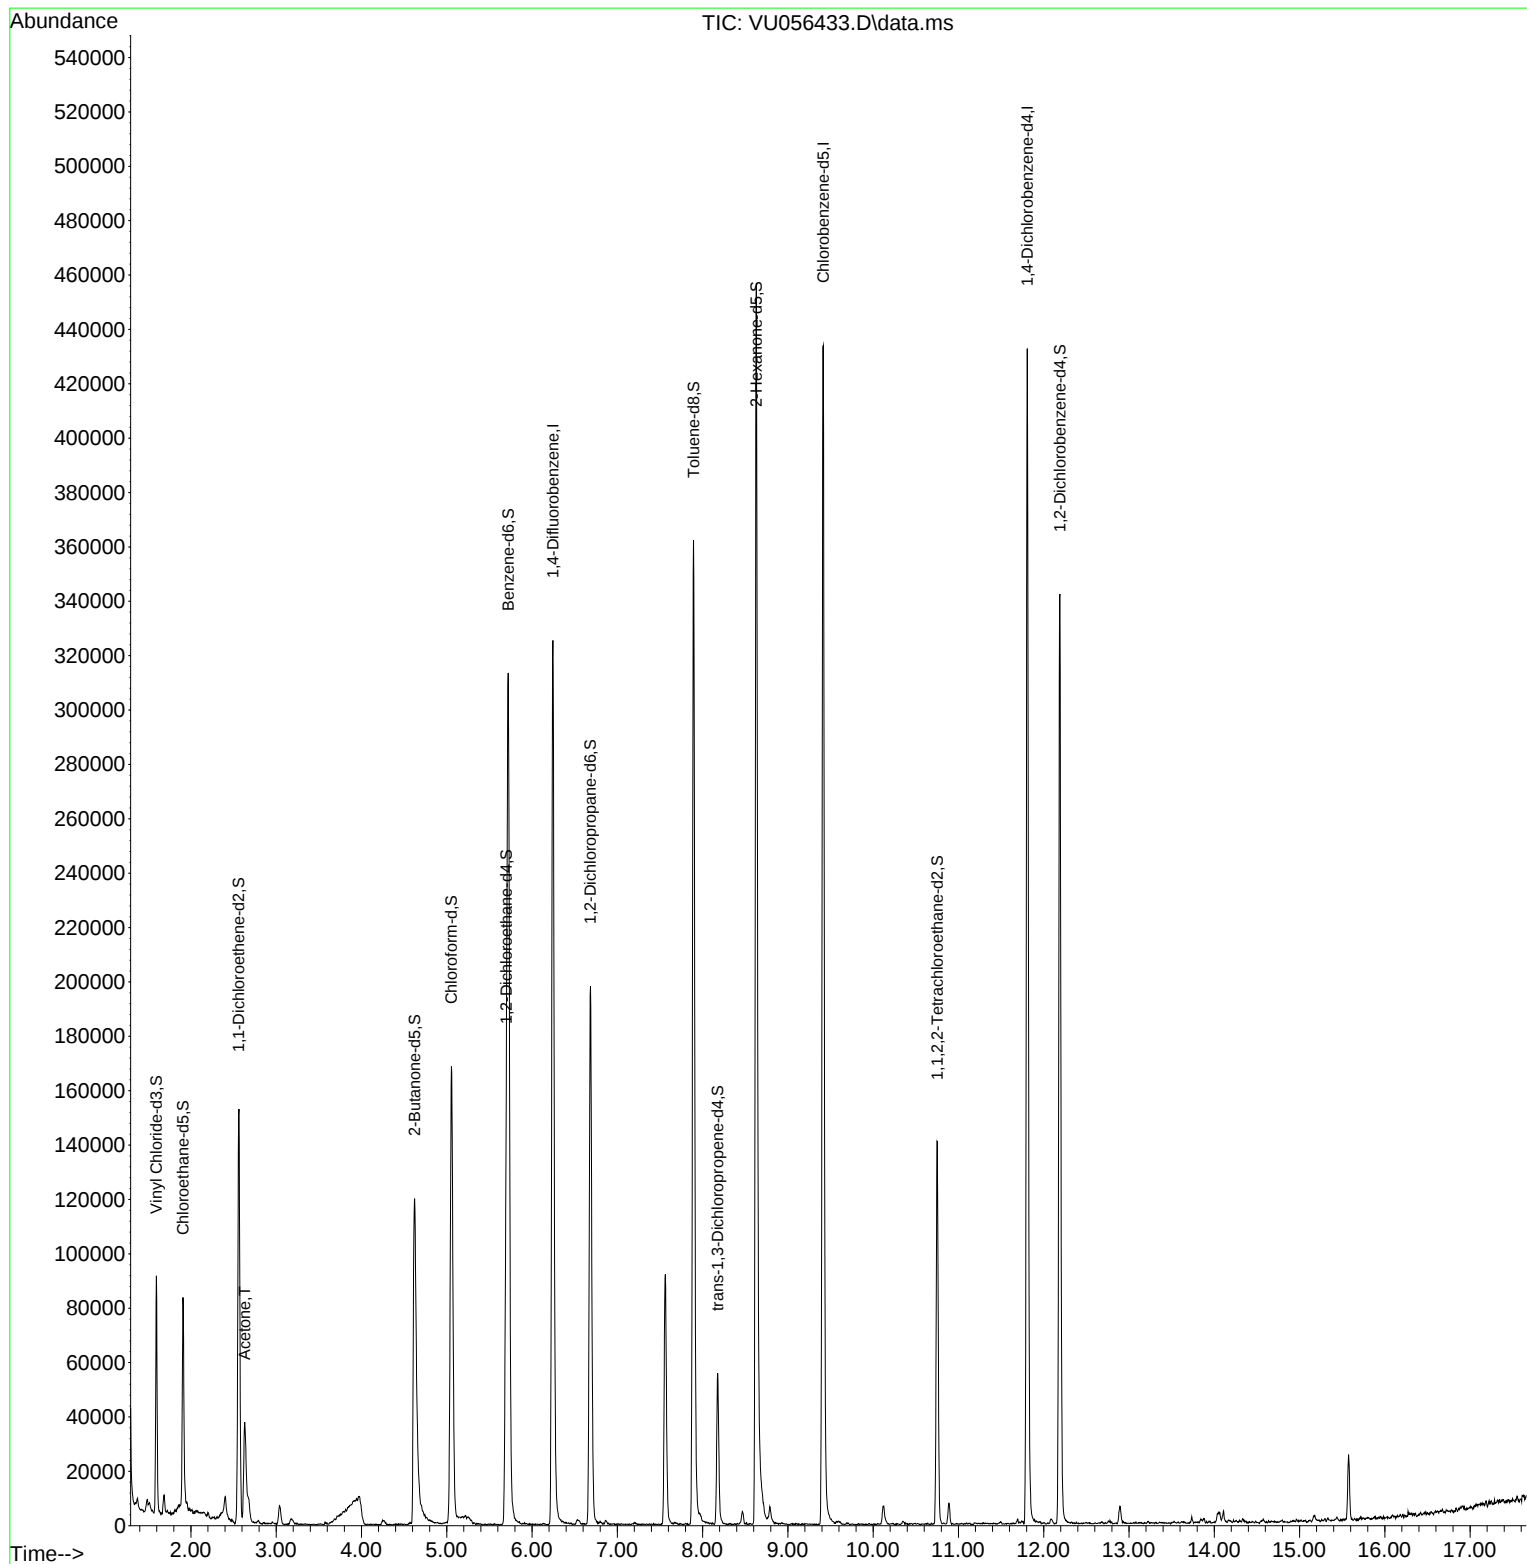

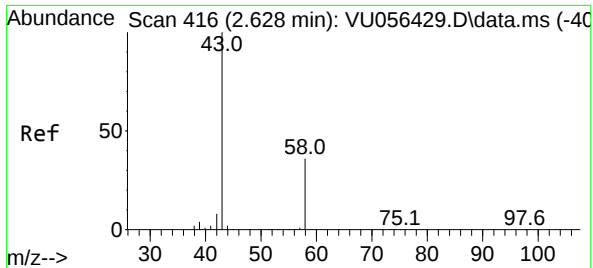

#13
 Acetone
 Concen: 15.517 ug/L
 RT: 2.631 min Scan# 41
 Delta R.T. 0.003 min
 Lab File: VU056433.D
 Acq: 17 Nov 2023 11:34

Instrument :
 MSVOA_U
 ClientSampleId :
 YCGB7

Tgt Ion: 43 Resp: 52847
 Ion Ratio Lower Upper
 43 100
 58 35.4 0.0 70.0

