
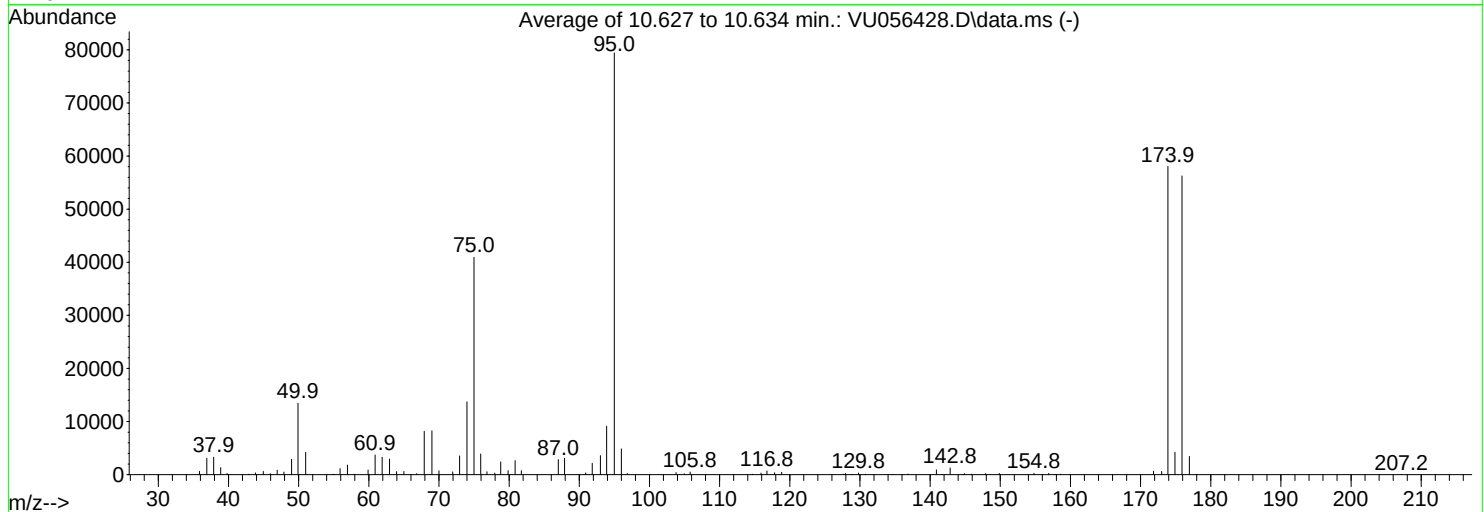


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111723\
Data File : VU056428.D
Acq On : 17 Nov 2023 08:04
Operator : MD/SY
Sample : BFB076
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB076

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Nov 18 00:12:04 2023

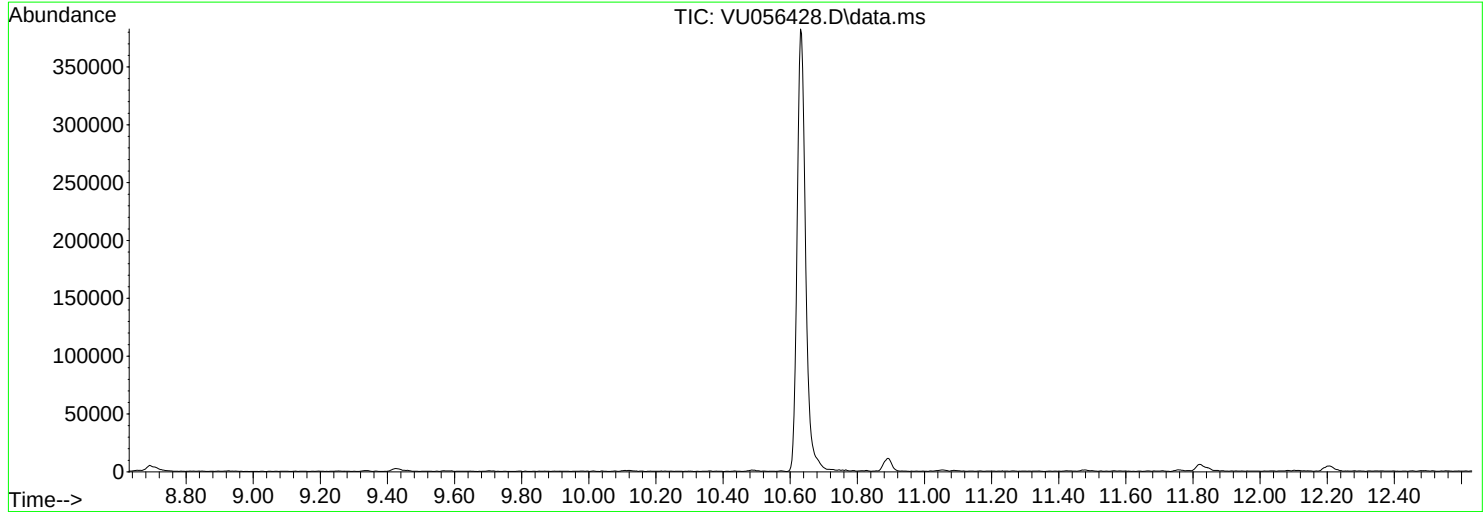

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	13454	PASS
75	95	30	80	51.5	40933	PASS
95	95	100	100	100.0	79432	PASS
96	95	5	9	6.1	4862	PASS
173	174	0.00	2	1.0	607	PASS
174	95	50	120	73.1	58037	PASS
175	174	5	9	7.3	4218	PASS
176	174	95	101	96.9	56248	PASS
177	176	5	9	6.1	3444	PASS

m/z	Abundance
43.90	333.0

Instrument :
MSVOA_U
ClientSampleId :
BFB076

m/z	Abundance
35.80	690.0
36.90	2834.0
37.90	3088.0
38.90	1303.0
39.80	170.0
43.80	676.0
45.00	535.0
46.00	184.0
47.00	896.0
47.90	531.0
49.00	2950.0
49.90	13074.0
51.00	4138.0
54.90	141.0
55.90	974.0
56.90	1600.0
57.90	128.0
59.90	815.0
60.90	3621.0
61.90	3381.0
62.90	2644.0
64.00	582.0
65.00	574.0
66.80	156.0
67.90	7875.0
69.00	8012.0
70.00	717.0
72.00	432.0
73.00	3475.0
74.00	13224.0
75.00	38552.0
76.00	3830.0
76.80	554.0
77.90	249.0
78.80	2494.0
79.80	724.0
80.80	2568.0
81.80	677.0
87.00	2826.0
87.90	2861.0
90.90	305.0
91.80	1973.0
93.00	3461.0
93.90	8729.0
95.00	75976.0
96.00	4415.0
96.80	188.0
103.80	369.0
104.90	139.0
105.80	493.0
114.70	128.0
115.90	316.0
116.70	581.0
117.80	214.0
118.90	427.0
127.70	264.0
128.90	117.0
129.80	296.0
134.70	120.0
136.80	107.0
140.90	866.0
142.90	1300.0
144.70	289.0
147.80	204.0
149.80	210.0
154.70	272.0
156.90	213.0
158.60	145.0
171.90	565.0
173.00	876.0
173.90	53912.0
174.90	4002.0
175.90	52200.0
177.00	3181.0

Instrument :
MSVOA_U
ClientSampleId :
BFB076

m/z	Abundance
35.90	622.0
36.90	3176.0
37.90	3422.0
38.90	1360.0
39.80	236.0
42.90	114.0
43.90	663.0
44.90	596.0
45.90	172.0
47.00	849.0
47.90	542.0
49.00	3003.0
49.90	13781.0
51.00	4414.0
52.00	104.0
54.90	134.0
55.90	1220.0
56.90	1843.0
57.90	121.0
59.90	937.0
60.90	3791.0
61.90	3320.0
63.00	2971.0
64.00	587.0
65.00	588.0
66.80	212.0
67.90	8520.0
69.00	8544.0
70.00	761.0
72.00	586.0
73.00	3564.0
74.00	14100.0
75.00	42152.0
76.00	3966.0
76.80	555.0
78.00	323.0
78.80	2422.0
79.90	773.0
80.90	2711.0
81.70	760.0
87.00	2906.0
87.90	3217.0
90.90	337.0
91.80	2200.0
93.00	3719.0
93.90	9310.0
95.00	81840.0
96.00	4954.0
96.80	215.0
103.80	418.0
105.00	205.0
105.80	518.0
114.60	115.0
115.90	312.0
116.70	703.0
117.80	368.0
118.80	479.0
127.90	296.0
128.90	108.0
129.80	319.0
130.80	129.0
134.70	109.0
136.80	105.0
140.90	882.0
141.80	116.0
142.90	1362.0
144.90	282.0
145.90	114.0
147.90	207.0
149.80	271.0
154.80	271.0
156.90	278.0
157.80	107.0
158.60	122.0
171.90	657.0
173.00	946.0
173.90	59704.0
174.90	4348.0
175.90	58192.0
176.90	3503.0

Instrument :
MSVOA_U
ClientSampleId :
BFB076

m/z	Abundance
35.90	634.0
36.90	3224.0
37.90	3329.0
38.90	1286.0
39.80	284.0
42.90	145.0
43.90	673.0
44.90	675.0
46.00	157.0
46.90	757.0
47.90	366.0
49.00	2763.0
49.90	13507.0
51.00	4128.0
52.00	102.0
55.10	135.0
55.90	1258.0
57.00	1983.0
59.90	904.0
60.90	3720.0
61.90	3170.0
63.00	3173.0
63.90	522.0
65.00	683.0
66.80	193.0
67.90	8108.0
69.00	8207.0
70.00	668.0
71.90	576.0
72.90	3538.0
74.00	13830.0
75.00	42096.0
75.90	3857.0
76.90	567.0
78.00	357.0
78.80	2301.0
79.90	810.0
80.90	2661.0
81.70	787.0
87.00	2813.0
87.90	3156.0
90.90	341.0
91.90	2271.0
93.00	3582.0
93.90	9379.0
95.00	80480.0
96.00	5218.0
96.90	219.0
103.80	375.0
105.00	197.0
105.80	406.0
115.90	272.0
116.80	772.0
117.90	462.0
118.80	493.0
128.00	345.0
129.80	278.0
130.80	169.0
136.90	130.0
140.90	948.0
141.70	103.0
142.80	1159.0
144.90	297.0
145.90	136.0
148.00	146.0
149.90	230.0
154.90	243.0
156.90	223.0
157.80	121.0
171.80	758.0
173.90	60496.0
174.90	4304.0
175.90	58352.0
176.90	3648.0
207.20	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB076