

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111725\
 Data File : VU063727.D
 Acq On : 17 Nov 2025 15:08
 Operator : MD/SY
 Sample : VU1117WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK126

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

Signal : TIC: VU063727.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.586	83	92	106	rBV	193845	216865	16.92%	2.173%
2	1.895	180	188	205	rVB	137200	176921	13.81%	1.773%
3	2.541	376	389	405	rBV	280564	470583	36.73%	4.716%
4	2.766	451	459	468	rVB2	4333	7320	0.57%	0.073%
5	3.017	528	537	548	rVB5	3691	7460	0.58%	0.075%
6	3.072	548	554	557	rBV2	342	368	0.03%	0.004%
7	3.158	570	581	591	rBV4	2590	5736	0.45%	0.057%
8	3.303	620	626	628	rBV3	522	442	0.03%	0.004%
9	3.326	628	633	647	rVB5	2742	5747	0.45%	0.058%
10	3.493	682	685	694	rBV2	244	252	0.02%	0.003%
11	3.541	696	700	703	rBV2	298	285	0.02%	0.003%
12	3.676	738	742	745	rVB3	539	414	0.03%	0.004%
13	3.789	772	777	778	rBV	377	285	0.02%	0.003%
14	3.798	778	780	786	rVB	417	311	0.02%	0.003%
15	3.953	822	828	831	rBV2	370	393	0.03%	0.004%
16	4.101	871	874	879	rBV	237	261	0.02%	0.003%
17	4.252	917	921	924	rBV	257	249	0.02%	0.002%
18	4.409	967	970	972	rBV2	441	247	0.02%	0.002%
19	4.474	982	990	992	rBV	355	497	0.04%	0.005%
20	4.596	1016	1028	1061	rBV	91268	262407	20.48%	2.630%
21	4.895	1119	1121	1127	rVB3	771	593	0.05%	0.006%
22	5.030	1146	1163	1189	rBV	215819	498447	38.90%	4.995%
23	5.168	1203	1206	1209	rBV3	468	309	0.02%	0.003%
24	5.261	1233	1235	1241	rVB3	478	427	0.03%	0.004%
25	5.287	1241	1243	1246	rVB2	633	345	0.03%	0.003%
26	5.322	1252	1254	1257	rBV2	349	239	0.02%	0.002%
27	5.364	1262	1267	1269	rBV3	641	602	0.05%	0.006%
28	5.486	1302	1305	1313	rBV4	553	617	0.05%	0.006%
29	5.599	1335	1340	1342	rBV	440	316	0.02%	0.003%
30	5.692	1348	1369	1408	rBV2	433990	1281346	100.00%	12.841%
31	5.975	1453	1457	1459	rBV3	346	264	0.02%	0.003%
32	6.017	1466	1470	1472	rBV	545	424	0.03%	0.004%
33	6.219	1520	1533	1576	rBV	353229	751016	58.61%	7.526%
34	6.448	1601	1604	1607	rVB2	571	394	0.03%	0.004%
35	6.515	1613	1625	1643	rBV7	7872	17595	1.37%	0.176%
36	6.660	1657	1670	1708	rBV	264620	563164	43.95%	5.644%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111725\
 Data File : VU063727.D
 Acq On : 17 Nov 2025 15:08
 Operator : MD/SY
 Sample : VU1117WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK126

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

37	6.888	1736	1741	1745	rBV2	553	557	0.04%	0.006%
38	7.155	1821	1824	1827	rBV2	423	271	0.02%	0.003%
39	7.370	1885	1891	1894	rBV2	518	543	0.04%	0.005%
40	7.393	1895	1898	1902	rVV2	285	274	0.02%	0.003%
41	7.416	1902	1905	1910	rVB	348	315	0.02%	0.003%
42	7.448	1910	1915	1916	rBV2	272	238	0.02%	0.002%
43	7.538	1932	1943	1975	rBV	127645	250267	19.53%	2.508%
44	7.740	2003	2006	2009	rVB	489	280	0.02%	0.003%
45	7.772	2009	2016	2018	rBV6	1842	1904	0.15%	0.019%
46	7.872	2034	2047	2082	rBV	553131	1065626	83.16%	10.679%
47	8.155	2125	2135	2157	rVV	85246	156593	12.22%	1.569%
48	8.374	2200	2203	2205	rBV3	671	433	0.03%	0.004%
49	8.473	2230	2234	2238	rVB4	385	339	0.03%	0.003%
50	8.531	2242	2252	2262	rVB5	3209	4769	0.37%	0.048%
51	8.612	2265	2277	2321	rBV2	219391	581247	45.36%	5.825%
52	9.087	2419	2425	2429	rBV3	551	607	0.05%	0.006%
53	9.149	2434	2444	2448	rBV3	670	1054	0.08%	0.011%
54	9.393	2504	2520	2561	rVV	521499	963838	75.22%	9.659%
55	9.547	2564	2568	2580	rVV3	3936	6239	0.49%	0.063%
56	9.679	2602	2609	2617	rVB5	3080	4842	0.38%	0.049%
57	9.763	2632	2635	2639	rVB3	371	270	0.02%	0.003%
58	9.869	2664	2668	2670	rBV2	439	356	0.03%	0.004%
59	10.097	2723	2739	2754	rBV10	4119	11425	0.89%	0.114%
60	10.274	2790	2794	2797	rBV2	398	339	0.03%	0.003%
61	10.338	2809	2814	2818	rVV2	223	250	0.02%	0.003%
62	10.425	2838	2841	2844	rVV2	324	255	0.02%	0.003%
63	10.460	2844	2852	2864	rVB3	3141	4890	0.38%	0.049%
64	10.615	2898	2900	2913	rVB5	728	1316	0.10%	0.013%
65	10.730	2923	2936	2953	rBV	385312	628204	49.03%	6.296%
66	10.878	2977	2982	2987	rVB3	870	698	0.05%	0.007%
67	11.068	3029	3041	3053	rBV4	3677	5685	0.44%	0.057%
68	11.357	3128	3131	3134	rBV2	366	244	0.02%	0.002%
69	11.386	3137	3140	3144	rVB2	392	280	0.02%	0.003%
70	11.451	3150	3160	3172	rBV2	5172	8008	0.62%	0.080%
71	11.505	3172	3177	3181	rVB2	546	607	0.05%	0.006%
72	11.637	3215	3218	3222	rVB	405	260	0.02%	0.003%
73	11.724	3237	3245	3253	rBV3	9144	13472	1.05%	0.135%
74	11.788	3253	3265	3290	rVV	553276	941964	73.51%	9.440%
75	11.956	3314	3317	3320	rBV2	424	285	0.02%	0.003%
76	12.039	3339	3343	3346	rBV	525	352	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111725\
 Data File : VU063727.D
 Acq On : 17 Nov 2025 15:08
 Operator : MD/SY
 Sample : VU1117WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK126

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

77	12.084	3354	3357	3359	rBV	462	276	0.02%	0.003%
78	12.097	3359	3361	3365	rBV2	527	397	0.03%	0.004%
79	12.168	3371	3383	3407	rBV	529292	914511	71.37%	9.165%
80	12.412	3455	3459	3460	rBV3	439	294	0.02%	0.003%
81	12.483	3476	3481	3485	rBV3	344	340	0.03%	0.003%
82	12.557	3501	3504	3507	rVB2	454	294	0.02%	0.003%
83	12.628	3521	3526	3528	rBV2	356	308	0.02%	0.003%
84	12.650	3529	3533	3539	rVB2	480	546	0.04%	0.005%
85	12.830	3586	3589	3592	rVB2	518	300	0.02%	0.003%
86	12.894	3606	3609	3614	rVB	388	327	0.03%	0.003%
87	12.949	3623	3626	3628	rBV2	452	246	0.02%	0.002%
88	12.968	3629	3632	3635	rBV3	845	731	0.06%	0.007%
89	13.200	3696	3704	3715	rVB4	7628	12653	0.99%	0.127%
90	13.338	3743	3747	3750	rBV2	508	450	0.04%	0.005%
91	13.480	3783	3791	3794	rBV2	414	612	0.05%	0.006%
92	13.499	3795	3797	3803	rVV2	715	606	0.05%	0.006%
93	13.528	3803	3806	3810	rVB2	433	347	0.03%	0.003%
94	13.766	3877	3880	3882	rBV2	454	317	0.02%	0.003%
95	13.820	3887	3897	3908	rBV4	16862	28758	2.24%	0.288%
96	14.065	3964	3973	3992	rBV	28243	52393	4.09%	0.525%
97	14.306	4034	4048	4063	rBV3	17479	29737	2.32%	0.298%
98	14.480	4100	4102	4105	rVB2	673	309	0.02%	0.003%
99	14.872	4220	4224	4228	rBV4	925	634	0.05%	0.006%
100	15.303	4353	4358	4360	rBV3	724	693	0.05%	0.007%




Sum of corrected areas: 9978616

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111725\
Data File : VU063727.D
Acq On : 17 Nov 2025 15:08
Operator : MD/SY
Sample : VU1117WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK126

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

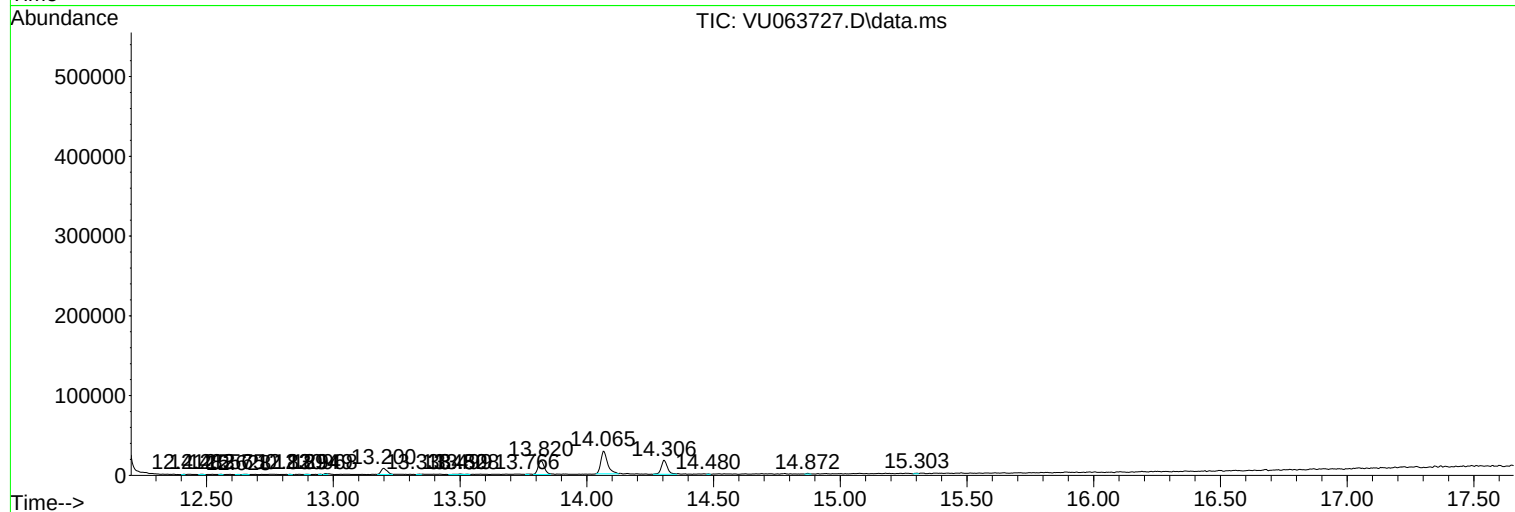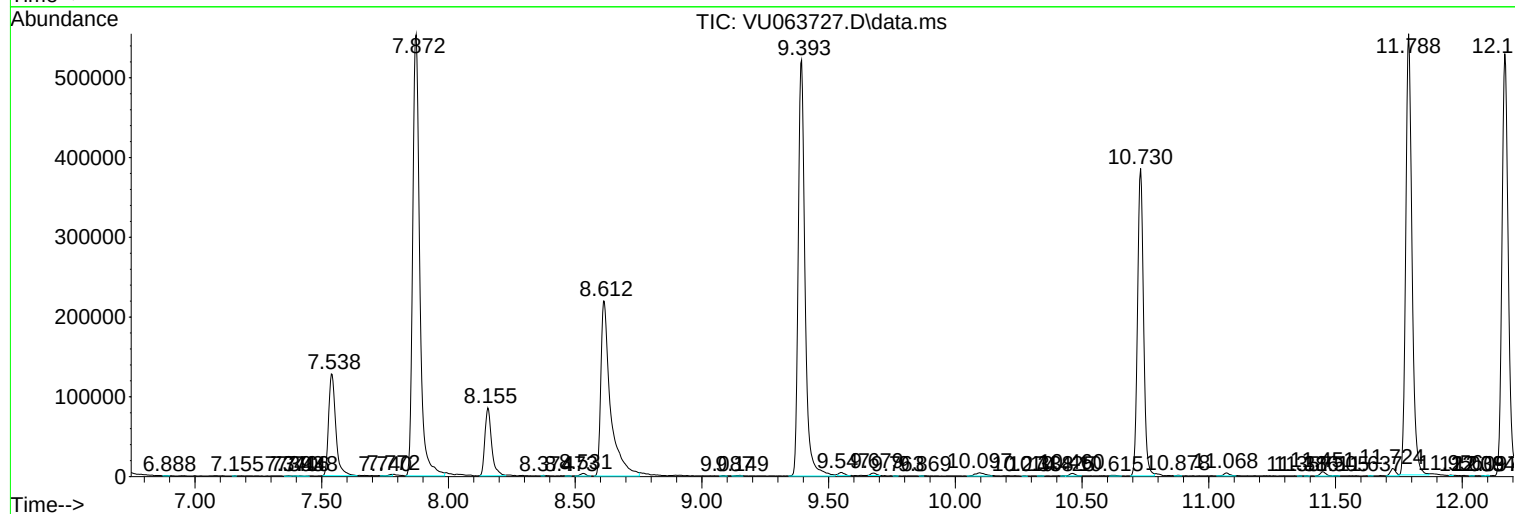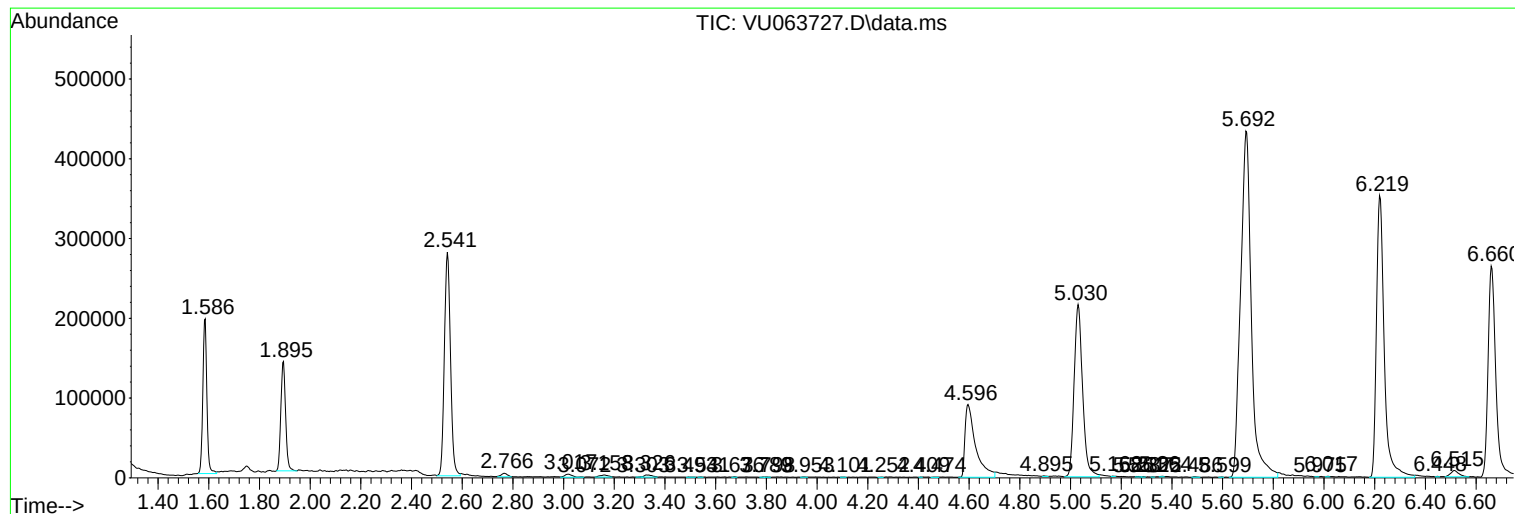

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111725\
Data File : VU063727.D
Acq On : 17 Nov 2025 15:08
Operator : MD/SY
Sample : VU1117WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK126

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111725\
Data File : VU063727.D
Acq On : 17 Nov 2025 15:08
Operator : MD/SY
Sample : VU1117WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK126

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc