


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU111819\
Data File : VU035734.D
Acq On : 18 Nov 2019 09:29
Operator : JC/SP
Sample : BFB01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB01

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR110419WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Nov 20 00:37:27 2019

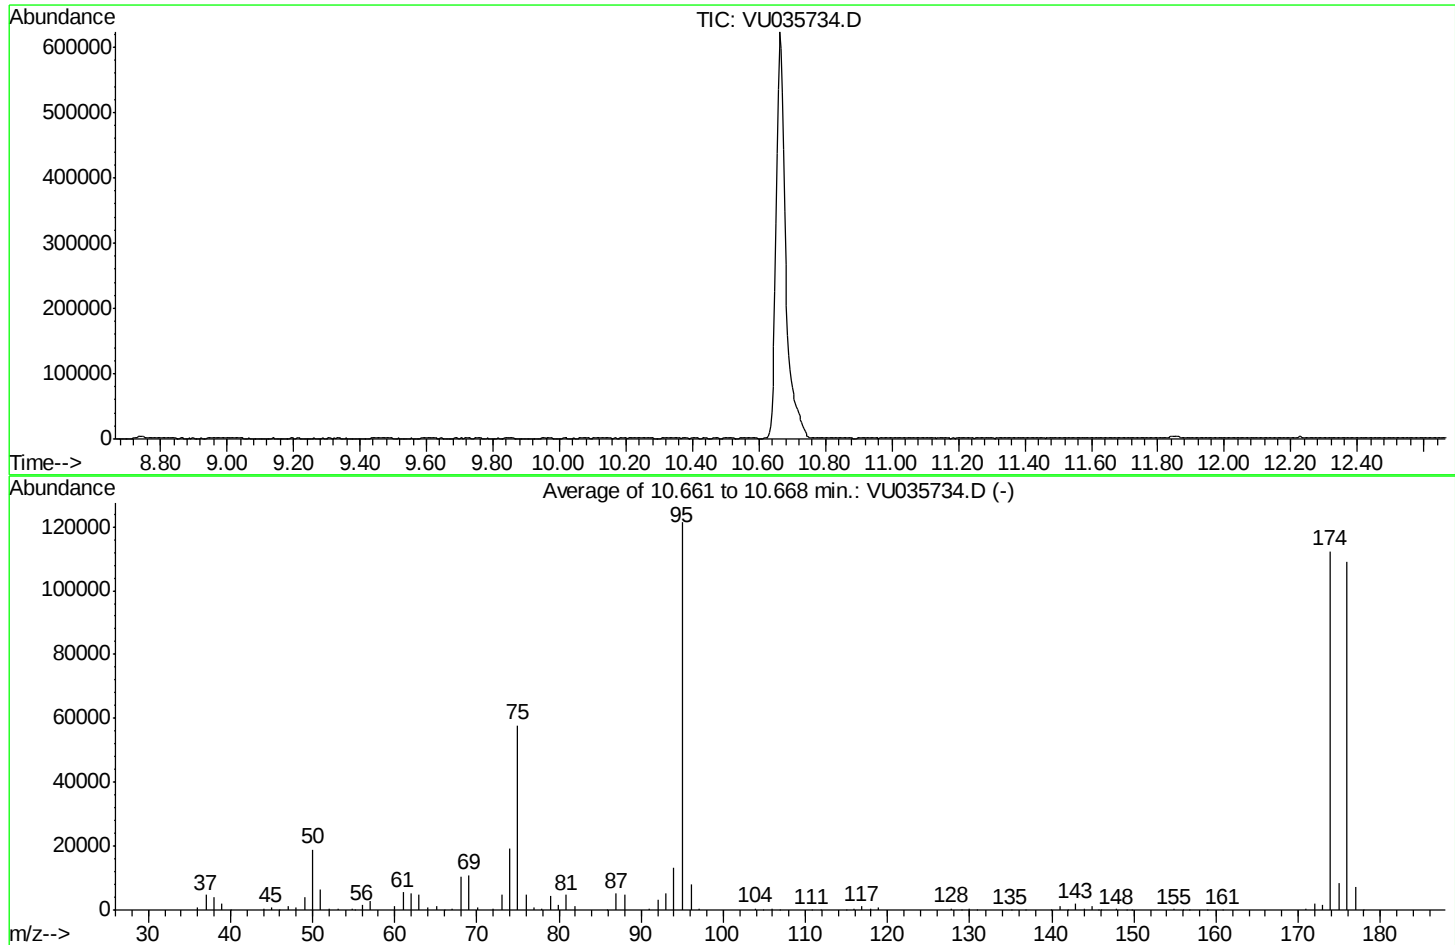

AutoFind: Scans 2899, 2900, 2901; Background Corrected with Scan 2885

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	18976	PASS
75	95	30	80	47.6	57794	PASS
95	95	100	100	100.0	121386	PASS
96	95	5	9	6.6	7965	PASS
173	174	0.00	2	1.6	1782	PASS
174	95	50	120	92.6	112370	PASS
175	174	5	9	7.5	8400	PASS
176	174	95	101	97.1	109144	PASS
177	176	5	9	6.5	7062	PASS

m/z	Abundance
36.00	801.0
37.00	4476.0
38.00	3952.0
39.00	2095.0
40.10	285.0
44.00	1451.0
45.00	736.0
46.00	140.0
47.10	1284.0
47.90	599.0
49.10	4127.0
50.10	19424.0
51.00	6385.0
51.90	210.0
53.00	308.0
54.90	242.0
56.00	1394.0
57.10	2601.0
60.00	1161.0
61.00	5700.0
62.00	5298.0
63.00	4963.0
64.00	843.0
65.10	1263.0
66.00	194.0
67.00	349.0
68.00	10601.0
69.00	10996.0
70.10	787.0
72.00	623.0
73.00	4556.0
74.10	19040.0
75.00	58160.0
76.10	4981.0
77.00	992.0
77.90	539.0
78.90	4283.0
79.90	1473.0
80.90	4753.0
82.00	1231.0
85.80	195.0
86.90	5273.0
88.00	5140.0
91.00	432.0
92.00	3388.0
93.00	5201.0
94.00	13426.0
95.00	120176.0
96.10	8021.0
97.00	314.0
104.00	514.0
104.80	150.0
105.90	473.0
106.90	104.0
114.90	181.0
115.90	496.0
116.90	1181.0
117.90	539.0
118.90	890.0
127.80	456.0
128.90	143.0
129.90	552.0
130.80	240.0
135.00	139.0
136.90	154.0
141.00	1096.0
141.90	152.0
142.90	1743.0
144.00	264.0
144.90	977.0
145.70	142.0
146.00	141.0
147.90	285.0
149.10	160.0
154.90	391.0
156.00	120.0
156.80	181.0
158.90	130.0
160.80	114.0
170.90	323.0
172.00	1788.0
173.00	1698.0
173.90	109984.0
175.00	8264.0
175.90	105736.0
177.00	7055.0
177.90	223.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
36.00	786.0
37.00	4819.0
38.00	3899.0
39.00	2067.0
40.10	296.0
44.00	1461.0
45.00	792.0
46.00	160.0
47.00	1401.0
48.00	612.0
49.10	3998.0
50.10	19488.0
51.00	6487.0
52.00	245.0
53.00	269.0
54.90	253.0
56.00	1602.0
57.00	2704.0
60.00	1219.0
61.00	5760.0
62.00	5508.0
63.00	5173.0
64.10	749.0
65.10	1163.0
66.00	166.0
67.00	328.0
68.00	10815.0
69.00	11252.0
70.10	798.0
71.90	630.0
73.00	4754.0
74.10	20040.0
75.00	59376.0
76.10	5070.0
77.00	973.0
77.90	569.0
78.90	4463.0
79.90	1620.0
80.90	4915.0
82.00	1259.0
85.80	145.0
86.90	5284.0
88.00	4679.0
90.90	393.0
92.00	3295.0
93.00	5282.0
94.00	13491.0
95.00	124464.0
96.10	8165.0
97.00	351.0
103.90	544.0
104.80	143.0
105.90	465.0
110.80	104.0
111.90	103.0
115.00	190.0
115.90	548.0
116.90	1240.0
117.90	533.0
118.90	874.0
127.80	490.0
129.00	148.0
129.90	433.0
130.80	189.0
135.00	193.0
136.90	145.0
140.90	1154.0
141.80	138.0
142.90	1957.0
144.00	250.0
144.90	1055.0
145.90	211.0
147.90	297.0
149.00	154.0
149.70	120.0
154.90	339.0
156.80	196.0
158.90	137.0
170.90	335.0
172.00	1902.0
173.00	1849.0
173.90	115464.0
175.00	8693.0
175.90	112008.0
177.00	7273.0
177.90	195.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
36.00	683.0
37.00	4727.0
38.00	3693.0
39.00	1829.0
40.10	281.0
44.00	1457.0
45.00	823.0
46.00	134.0
47.00	1416.0
48.10	660.0
49.00	3767.0
50.00	18016.0
51.00	5983.0
51.90	277.0
53.10	194.0
54.80	252.0
55.10	247.0
56.00	1568.0
57.00	2754.0
60.00	1125.0
61.00	5253.0
62.00	5181.0
63.00	4879.0
64.10	791.0
65.00	998.0
66.00	147.0
67.00	254.0
68.00	10269.0
69.10	10523.0
70.10	730.0
71.90	575.0
73.00	4565.0
74.00	19032.0
75.00	55848.0
76.00	4672.0
77.00	829.0
78.00	555.0
78.90	4266.0
79.90	1510.0
80.90	4661.0
81.90	1150.0
85.90	137.0
87.00	5033.0
88.00	4161.0
91.00	348.0
92.00	3073.0
93.00	4892.0
94.00	12934.0
95.00	119520.0
96.10	7710.0
97.00	307.0
103.90	521.0
104.90	137.0
105.90	458.0
110.80	135.0
111.90	110.0
115.00	138.0
115.90	559.0
116.90	1176.0
117.90	488.0
118.90	819.0
127.80	528.0
129.00	138.0
130.00	387.0
130.90	137.0
135.00	240.0
136.80	130.0
139.90	125.0
140.90	1161.0
141.80	132.0
142.90	1929.0
144.00	207.0
144.90	1031.0
145.90	258.0
147.90	288.0
149.00	123.0
149.70	133.0
154.90	241.0
156.80	190.0
158.90	112.0
170.90	336.0
171.90	2078.0
173.00	1800.0
173.90	111664.0
175.00	8244.0
175.90	109688.0
176.90	6860.0
177.90	176.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
40.00	171.0
44.00	924.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01