
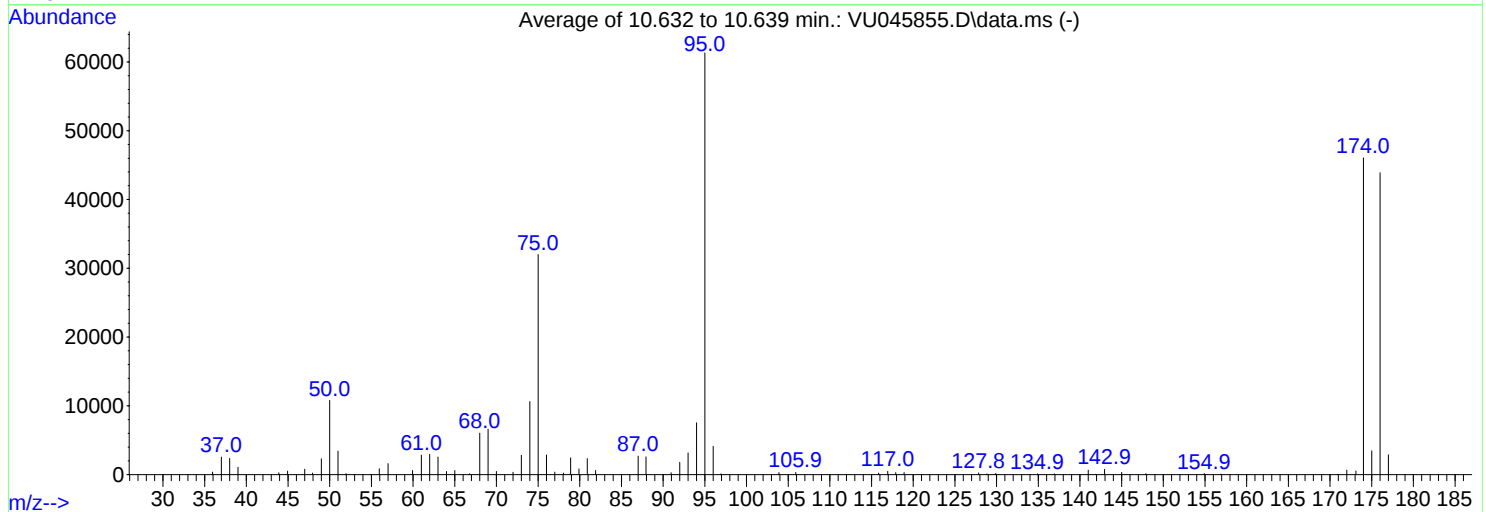


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111821\
 Data File : VU045855.D
 Acq On : 18 Nov 2021 09:05
 Operator : SY/MD
 Sample : BFB028
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB028

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Nov 22 03:50:15 2021

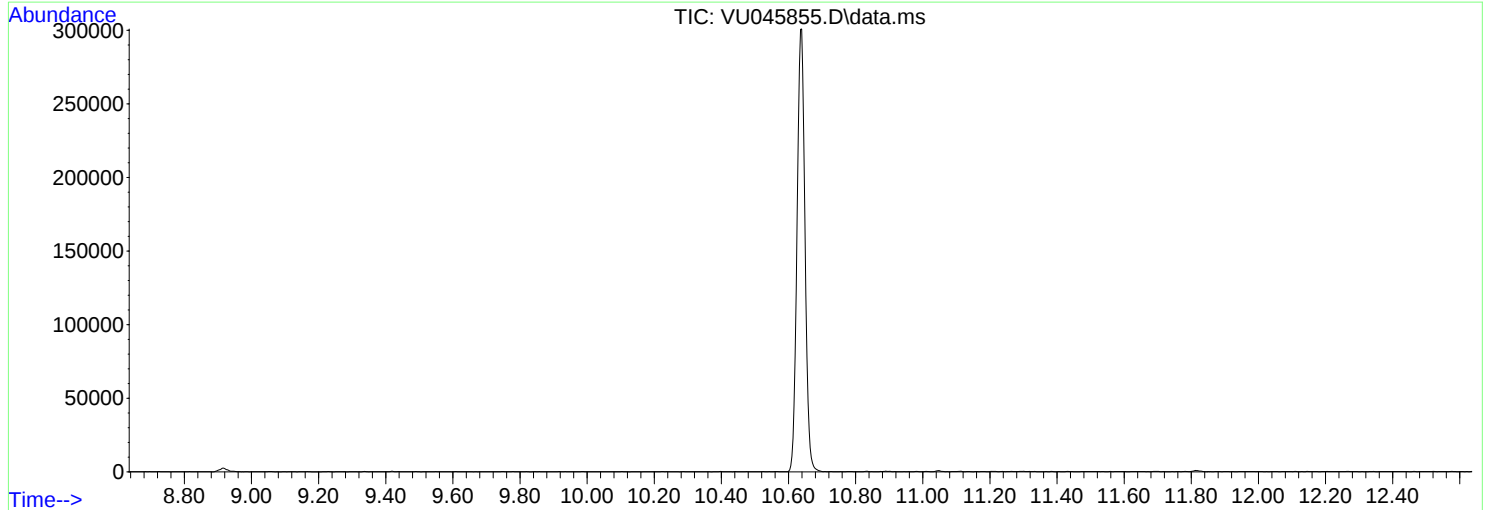

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	10790	PASS
75	95	30	80	52.2	32016	PASS
95	95	100	100	100.0	61323	PASS
96	95	5	9	6.7	4114	PASS
173	174	0.00	2	1.2	538	PASS
174	95	50	120	75.1	46064	PASS
175	174	5	9	7.5	3459	PASS
176	174	95	101	95.3	43904	PASS
177	176	5	9	6.6	2886	PASS

m/z	Abundance
35.90	416.0
37.00	2690.0
38.00	2323.0
39.00	1128.0
43.90	427.0
44.90	544.0
47.00	805.0
47.90	231.0
49.00	2264.0
50.00	10867.0
51.00	3416.0
51.90	150.0
54.90	104.0
56.00	831.0
57.00	1723.0
59.90	635.0
61.00	2938.0
62.00	2993.0
63.00	2627.0
64.00	400.0
65.00	541.0
66.80	126.0
68.00	6081.0
69.00	6733.0
70.00	471.0
72.00	339.0
73.00	3000.0
74.00	10800.0
75.00	32736.0
76.00	2845.0
77.00	361.0
78.10	191.0
78.90	2599.0
79.90	796.0
80.90	2360.0
81.90	664.0
87.00	2847.0
87.90	2632.0
90.90	319.0
92.00	1734.0
93.00	3080.0
94.00	7724.0
95.00	62784.0
96.00	3922.0
96.90	100.0
103.90	313.0
105.00	101.0
105.90	363.0
115.90	269.0
117.00	532.0
117.90	304.0
118.90	304.0
127.90	279.0
128.80	104.0
129.90	179.0
134.90	125.0
137.00	115.0
141.00	617.0
141.90	116.0
142.90	774.0
145.00	318.0
147.90	154.0
154.90	148.0
156.90	138.0
170.90	109.0
172.00	673.0
173.10	536.0
174.00	48128.0
175.00	3380.0
176.00	46408.0
177.00	3087.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

m/z	Abundance
43.90	137.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

m/z	Abundance
36.00	342.0
37.00	2354.0
38.00	2290.0
39.00	1020.0
43.90	409.0
45.00	472.0
47.00	740.0
48.00	248.0
49.00	2279.0
50.00	10398.0
51.00	3310.0
52.00	133.0
52.90	102.0
55.90	886.0
57.00	1444.0
60.00	571.0
61.00	2660.0
62.00	2855.0
63.00	2437.0
64.00	500.0
65.00	656.0
66.80	138.0
68.00	5856.0
69.00	6264.0
70.00	453.0
72.00	361.0
73.00	2551.0
74.00	10128.0
75.00	30416.0
76.00	2761.0
77.00	367.0
78.00	262.0
78.90	2202.0
79.90	819.0
80.90	2255.0
81.90	547.0
87.00	2472.0
88.00	2384.0
91.00	237.0
92.00	1798.0
93.00	3086.0
94.00	7065.0
95.00	58056.0
96.00	4113.0
97.00	134.0
103.90	268.0
105.90	297.0
115.80	213.0
116.90	432.0
117.90	268.0
118.90	331.0
127.80	248.0
128.90	107.0
129.90	176.0
134.90	104.0
136.90	113.0
141.00	641.0
143.00	745.0
145.00	294.0
147.90	124.0
154.90	161.0
172.00	601.0
173.10	532.0
174.00	42512.0
175.00	3411.0
176.00	40432.0
177.00	2633.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

m/z	Abundance
35.90	380.0
37.00	2644.0
38.00	2412.0
39.00	1098.0
43.90	406.0
45.00	545.0
47.00	797.0
48.00	229.0
49.00	2372.0
50.00	11106.0
51.00	3525.0
51.90	145.0
56.00	848.0
57.00	1634.0
59.90	622.0
61.00	2898.0
62.00	3019.0
63.00	2617.0
64.00	497.0
65.00	623.0
66.80	143.0
68.00	6152.0
69.00	6810.0
70.00	483.0
72.00	349.0
73.00	2883.0
74.00	10984.0
75.00	32896.0
76.00	2962.0
77.00	403.0
78.10	234.0
78.90	2508.0
79.90	875.0
80.90	2392.0
81.90	641.0
87.00	2771.0
88.00	2707.0
91.00	287.0
92.00	1818.0
93.00	3324.0
94.00	7829.0
95.00	63128.0
96.00	4306.0
97.00	123.0
103.90	297.0
105.90	346.0
115.90	254.0
117.00	474.0
117.90	307.0
118.90	309.0
127.90	266.0
128.90	107.0
129.90	178.0
134.90	132.0
136.90	120.0
141.00	687.0
143.00	787.0
145.00	338.0
147.90	164.0
154.90	167.0
156.90	139.0
172.00	694.0
173.10	547.0
174.00	47552.0
175.00	3587.0
176.00	44872.0
177.00	2938.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028