


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111822\
Data File : VU051896.D
Acq On : 18 Nov 2022 09:30
Operator : JC/MD
Sample : BFB145
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB145

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111522WMA.M
Title : VOC Analysis
Last Update : Fri Nov 18 00:53:49 2022

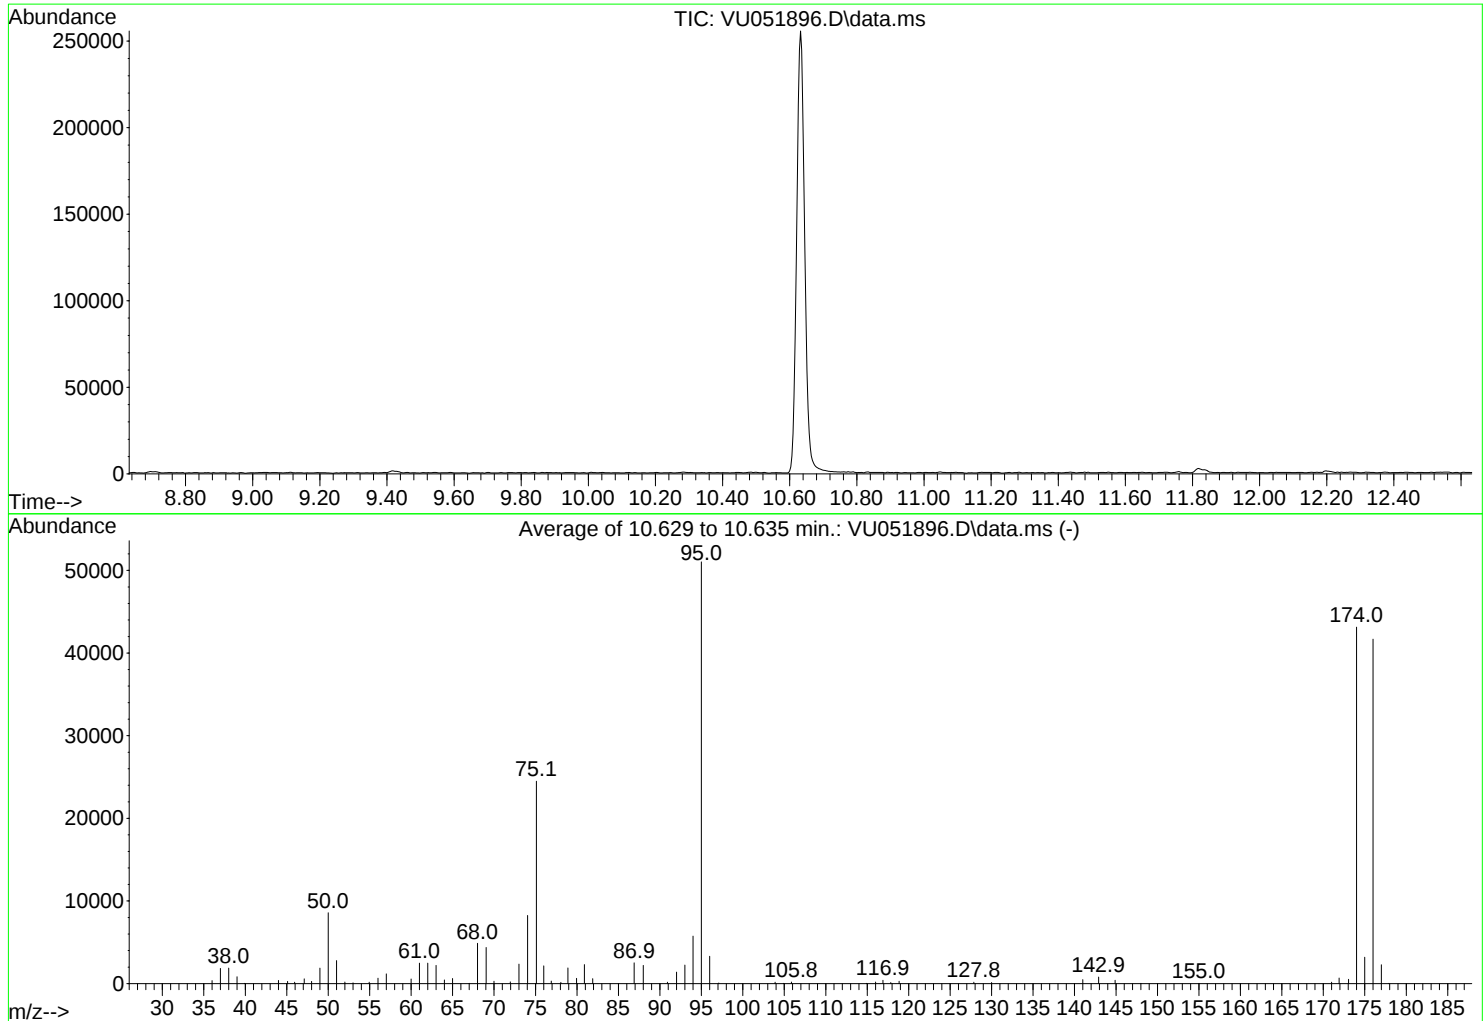

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.8	8571	PASS
75	95	30	80	48.0	24485	PASS
95	95	100	100	100.0	51035	PASS
96	95	5	9	6.5	3314	PASS
173	174	0.00	2	1.2	523	PASS
174	95	50	120	84.5	43125	PASS
175	174	5	9	7.4	3191	PASS
176	174	95	101	96.7	41688	PASS
177	176	5	9	5.5	2292	PASS

m/z	Abundance
39.80	163.0
44.00	369.0

Instrument :
MSVOA_U
ClientSampleId :
BFB145

m/z	Abundance
36.00	318.0
37.00	1850.0
38.00	1907.0
39.00	779.0
40.00	158.0
44.00	721.0
45.10	264.0
46.00	201.0
47.10	544.0
48.00	327.0
49.00	1787.0
50.00	8475.0
51.00	2969.0
52.00	147.0
53.00	182.0
55.00	165.0
56.00	661.0
57.00	1204.0
60.00	586.0
61.00	2452.0
62.00	2362.0
63.00	2078.0
64.00	424.0
65.00	553.0
68.00	4729.0
69.10	4359.0
70.00	260.0
71.90	186.0
73.00	2422.0
74.10	8370.0
75.10	24576.0
76.00	2187.0
76.90	355.0
78.00	153.0
78.90	1805.0
79.90	575.0
80.90	2283.0
81.90	617.0
86.90	2427.0
88.00	2143.0
90.90	143.0
92.00	1427.0
93.00	2124.0
94.00	5618.0
95.00	50056.0
96.00	3458.0
97.10	105.0
103.90	199.0
104.90	100.0
105.90	212.0
114.90	104.0
116.00	181.0
116.90	414.0
117.90	125.0
118.80	261.0
127.90	178.0
130.00	175.0
141.00	475.0
142.90	765.0
144.90	363.0
171.00	139.0
171.90	680.0
173.10	471.0
174.00	42048.0
175.00	3142.0
176.00	40792.0
177.00	2389.0

Instrument :
MSVOA_U
ClientSampleId :
BFB145

m/z	Abundance
36.00	398.0
37.00	1911.0
38.00	1924.0
39.00	850.0
40.00	192.0
44.00	754.0
45.10	284.0
46.00	191.0
47.10	601.0
48.00	287.0
49.00	1899.0
50.00	8832.0
51.00	2884.0
52.00	196.0
53.00	136.0
54.90	162.0
56.00	654.0
57.00	1203.0
60.00	614.0
61.00	2539.0
62.00	2568.0
63.00	2306.0
64.00	490.0
65.00	608.0
68.00	4999.0
69.00	4461.0
70.00	301.0
71.90	226.0
73.00	2457.0
74.00	8531.0
75.10	25184.0
76.00	2163.0
76.90	306.0
78.10	152.0
78.90	1954.0
79.90	674.0
80.90	2374.0
81.90	618.0
86.90	2570.0
88.00	2269.0
90.90	190.0
92.00	1438.0
93.00	2307.0
94.00	5953.0
95.00	52656.0
96.00	3408.0
97.10	106.0
103.90	186.0
105.80	197.0
116.00	214.0
116.90	419.0
117.90	127.0
118.90	286.0
127.80	156.0
130.00	142.0
141.00	514.0
142.90	837.0
144.90	426.0
171.00	196.0
171.90	678.0
173.10	514.0
174.00	44536.0
175.00	3278.0
176.00	42952.0
177.00	2380.0

Instrument :
MSVOA_U
ClientSampleId :
BFB145

m/z	Abundance
36.00	404.0
37.00	1745.0
38.00	1783.0
39.00	870.0
40.00	260.0
44.00	799.0
45.10	272.0
45.90	157.0
47.10	612.0
48.00	221.0
49.00	1935.0
50.00	8406.0
51.00	2491.0
52.00	244.0
54.90	178.0
56.00	641.0
57.00	1133.0
60.00	497.0
61.00	2422.0
62.00	2499.0
63.00	2244.0
64.00	451.0
65.00	678.0
67.00	118.0
68.00	4907.0
69.00	4288.0
70.00	329.0
72.00	251.0
73.00	2218.0
74.00	7838.0
75.10	23696.0
76.00	2102.0
76.90	279.0
78.10	174.0
78.90	1912.0
80.00	680.0
80.90	2285.0
81.90	563.0
86.90	2571.0
88.00	2192.0
90.90	182.0
92.00	1346.0
93.00	2306.0
94.00	5679.0
95.00	50392.0
96.00	3075.0
103.90	162.0
105.80	201.0
116.00	180.0
116.90	392.0
117.80	136.0
118.90	317.0
127.80	170.0
130.00	109.0
141.00	471.0
142.90	796.0
144.90	407.0
148.00	115.0
155.00	122.0
171.00	206.0
171.90	655.0
173.00	585.0
174.00	42792.0
175.00	3153.0
176.00	41320.0
177.00	2108.0
177.90	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB145