

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111823\
 Data File : VU056504.D
 Acq On : 19 Nov 2023 01:43
 Operator : MD/SY
 Sample : 05476-12
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AE0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056504.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	105	rVB	87386	98335	10.28%	1.303%
2	1.727	128	136	144	rVB	27462	33592	3.51%	0.445%
3	1.907	184	192	208	rVB	81634	113661	11.88%	1.506%
4	2.563	383	396	409	rBV	150055	248477	25.97%	3.293%
5	3.177	572	587	607	rBV2	9443	24318	2.54%	0.322%
6	3.782	763	775	785	rBV7	5199	10975	1.15%	0.145%
7	4.618	1024	1035	1068	rBV	138506	367372	38.39%	4.869%
8	5.055	1156	1171	1192	rBV2	176465	395687	41.35%	5.244%
9	5.717	1357	1377	1405	rBV2	318250	850125	88.84%	11.268%
10	6.242	1527	1540	1566	rBV	337335	662080	69.19%	8.775%
11	6.685	1665	1678	1707	rVB	205606	409561	42.80%	5.428%
12	7.560	1938	1950	1967	rBV	96261	173040	18.08%	2.293%
13	7.894	2041	2054	2083	rBV	358393	649973	67.92%	8.615%
14	8.177	2131	2142	2158	rBV	59390	101175	10.57%	1.341%
15	8.630	2271	2283	2323	rBV2	487402	956936	100.00%	12.683%
16	9.412	2513	2526	2551	rBV	476309	838059	87.58%	11.108%
17	10.749	2930	2942	2967	rBV	161655	266456	27.84%	3.532%
18	11.807	3256	3271	3289	rBV	444520	729419	76.22%	9.668%
19	12.187	3376	3389	3409	rBV	364898	615658	64.34%	8.160%




Sum of corrected areas: 7544899

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111823\
Data File : VU056504.D
Acq On : 19 Nov 2023 01:43
Operator : MD/SY
Sample : 05476-12
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

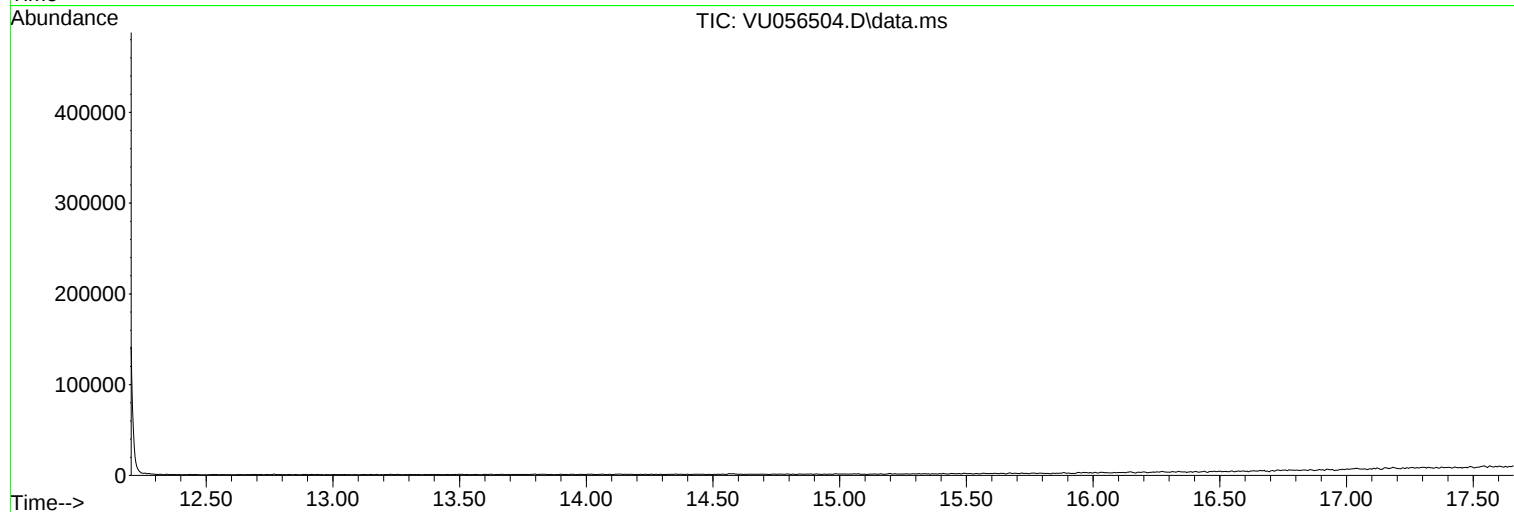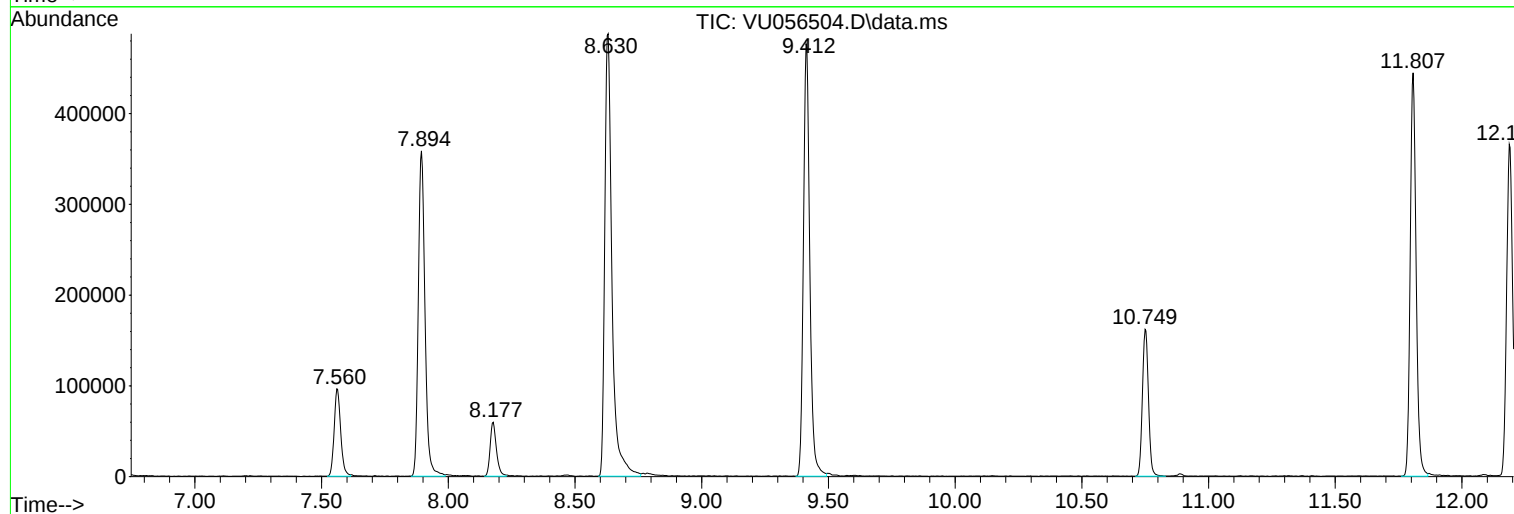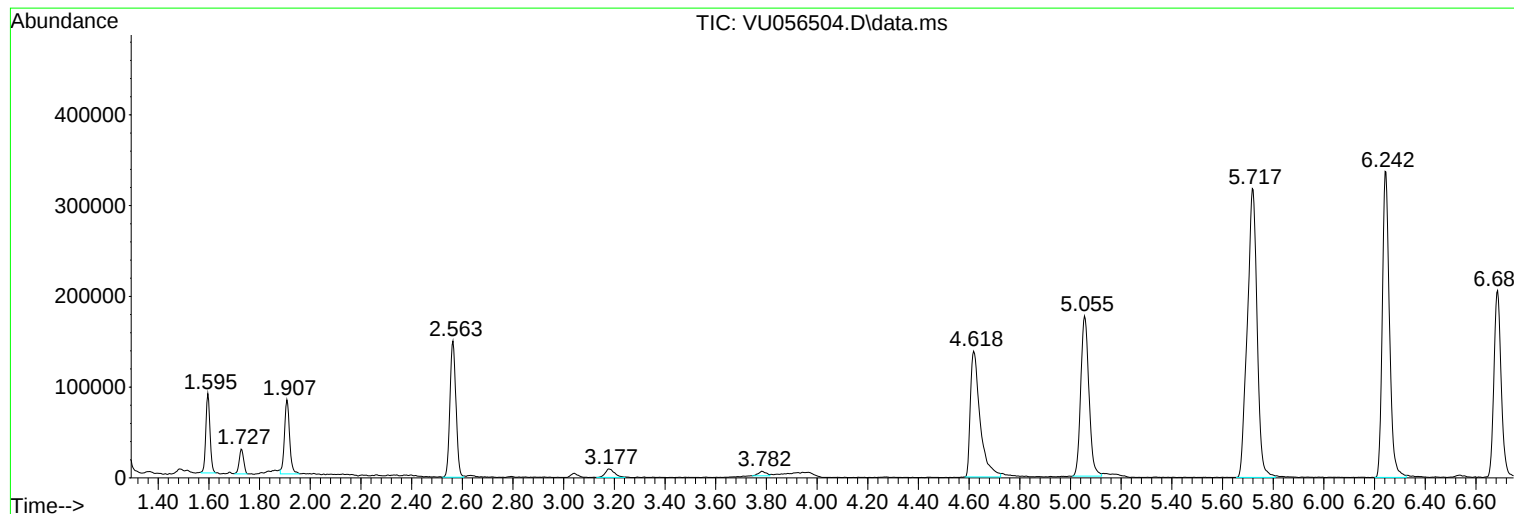

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111823\
Data File : VU056504.D
Acq On : 19 Nov 2023 01:43
Operator : MD/SY
Sample : 05476-12
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COAE0










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.560	1.31 ug/L	173040	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Thiatricyclo[3.1.1.0(2,4)]heptane	112	C6H8S	1000221-37-0	32
2			Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	23
3			2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	9
4			.alpha.,.alpha.-Dichloromethyl m...	114	C2H4Cl2O	004885-02-3	9
5			2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	9

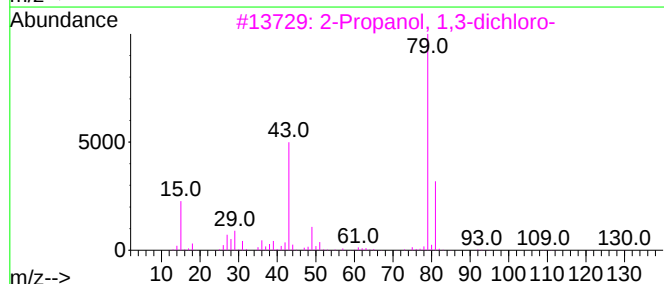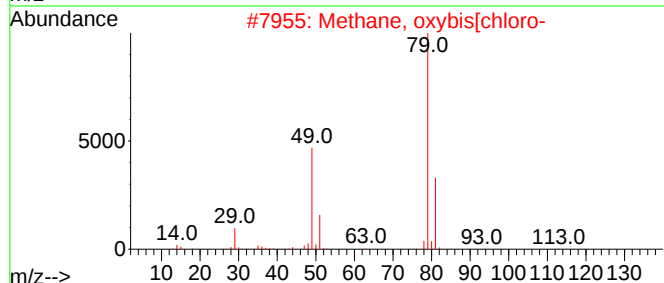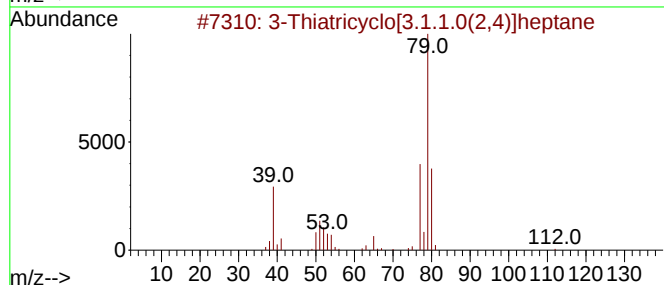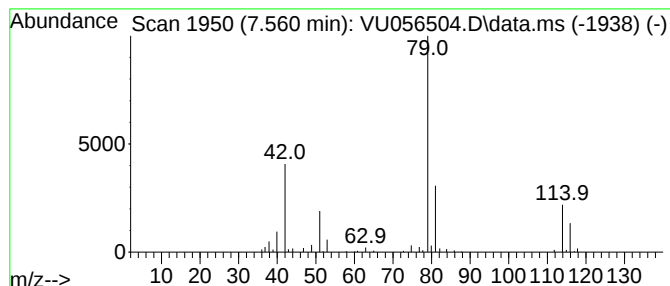

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111823\
Data File : VU056504.D
Acq On : 19 Nov 2023 01:43
Operator : MD/SY
Sample : 05476-12
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.560	1.3	ug/L	173040	1	6.245	662080	5.0