

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111825\
 Data File : VU063734.D
 Acq On : 18 Nov 2025 11:17
 Operator : MD/SY
 Sample : VU1118WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK128

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

Signal : TIC: VU063734.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.586	85	92	104	rBV	176909	193101	15.48%	2.046%
2	1.894	181	188	205	rVB	130191	167871	13.46%	1.778%
3	2.541	378	389	409	rBV	269860	451117	36.16%	4.779%
4	2.849	478	485	490	rBV2	493	758	0.06%	0.008%
5	3.158	573	581	584	rBV5	1682	2719	0.22%	0.029%
6	3.290	619	622	626	rBV	290	235	0.02%	0.002%
7	3.328	628	634	642	rVV5	1332	2291	0.18%	0.024%
8	3.476	677	680	681	rBV2	205	135	0.01%	0.001%
9	3.573	707	710	713	rBV	313	243	0.02%	0.003%
10	3.618	720	724	727	rBV	537	383	0.03%	0.004%
11	3.669	738	740	742	rVV	333	175	0.01%	0.002%
12	3.721	746	756	759	rBV	376	523	0.04%	0.006%
13	3.775	772	773	776	rVB	205	100	0.01%	0.001%
14	3.843	791	794	797	rVB	242	169	0.01%	0.002%
15	3.904	810	813	817	rVB2	394	281	0.02%	0.003%
16	3.936	819	823	826	rBV2	323	269	0.02%	0.003%
17	4.000	841	843	847	rVB	245	138	0.01%	0.001%
18	4.148	885	889	891	rBV	358	230	0.02%	0.002%
19	4.251	917	921	923	rBV2	270	168	0.01%	0.002%
20	4.335	943	947	950	rBV2	187	167	0.01%	0.002%
21	4.406	966	969	972	rBV2	167	95	0.01%	0.001%
22	4.512	999	1002	1006	rBV2	266	214	0.02%	0.002%
23	4.595	1019	1028	1061	rBV	85078	246680	19.77%	2.613%
24	5.029	1148	1163	1189	rBV	213862	488249	39.14%	5.172%
25	5.489	1301	1306	1307	rVB3	229	133	0.01%	0.001%
26	5.563	1323	1329	1330	rBV	422	295	0.02%	0.003%
27	5.608	1340	1343	1348	rVB2	244	215	0.02%	0.002%
28	5.695	1348	1370	1405	rBV2	422709	1247591	100.00%	13.217%
29	6.033	1472	1475	1481	rVB3	590	501	0.04%	0.005%
30	6.061	1481	1484	1486	rBV	207	115	0.01%	0.001%
31	6.107	1496	1498	1506	rVB2	442	382	0.03%	0.004%
32	6.219	1521	1533	1563	rBV	339673	714259	57.25%	7.567%
33	6.508	1613	1623	1644	rVB7	6417	15655	1.25%	0.166%
34	6.660	1657	1670	1695	rBV	258838	543786	43.59%	5.761%
35	6.978	1766	1769	1774	rBV2	222	269	0.02%	0.003%
36	7.196	1832	1837	1843	rBV2	307	313	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111825\
 Data File : VU063734.D
 Acq On : 18 Nov 2025 11:17
 Operator : MD/SY
 Sample : VU1118WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK128

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

37	7.229	1843	1847	1848	rBV2	165	104	0.01%	0.001%
38	7.283	1861	1864	1867	rBV	284	179	0.01%	0.002%
39	7.322	1872	1876	1878	rBV	288	228	0.02%	0.002%
40	7.373	1890	1892	1894	rVB2	219	101	0.01%	0.001%
41	7.393	1894	1898	1899	rBV2	216	147	0.01%	0.002%
42	7.537	1930	1943	1967	rBV	127528	243367	19.51%	2.578%
43	7.778	2013	2018	2022	rBV5	917	1016	0.08%	0.011%
44	7.872	2034	2047	2081	rBV	540969	1017406	81.55%	10.778%
45	8.155	2124	2135	2158	rBV	81184	151495	12.14%	1.605%
46	8.312	2180	2184	2185	rBB	61	99	0.01%	0.001%
47	8.357	2195	2198	2199	rBV	180	109	0.01%	0.001%
48	8.396	2207	2210	2212	rBV	144	111	0.01%	0.001%
49	8.483	2234	2237	2239	rVB	238	93	0.01%	0.001%
50	8.499	2239	2242	2245	rVB2	208	139	0.01%	0.001%
51	8.528	2245	2251	2266	rBV6	1754	2757	0.22%	0.029%
52	8.614	2266	2278	2318	rBV3	202135	545404	43.72%	5.778%
53	9.000	2396	2398	2401	rBV2	229	115	0.01%	0.001%
54	9.106	2427	2431	2433	rBV	330	256	0.02%	0.003%
55	9.145	2440	2443	2449	rVB2	654	644	0.05%	0.007%
56	9.193	2455	2458	2464	rBV2	283	298	0.02%	0.003%
57	9.225	2466	2468	2473	rVB2	350	216	0.02%	0.002%
58	9.303	2489	2492	2495	rBV2	342	284	0.02%	0.003%
59	9.393	2507	2520	2552	rBV	504600	929043	74.47%	9.842%
60	9.679	2601	2609	2616	rBV3	1589	2482	0.20%	0.026%
61	9.730	2622	2625	2627	rVB	308	147	0.01%	0.002%
62	9.839	2657	2659	2662	rBV	239	100	0.01%	0.001%
63	9.917	2680	2683	2688	rVB2	244	155	0.01%	0.002%
64	9.942	2688	2691	2693	rVB	196	106	0.01%	0.001%
65	9.968	2693	2699	2702	rBV2	253	276	0.02%	0.003%
66	10.103	2726	2741	2753	rBV9	2105	5842	0.47%	0.062%
67	10.200	2768	2771	2774	rBV	258	157	0.01%	0.002%
68	10.232	2778	2781	2783	rBV2	295	211	0.02%	0.002%
69	10.277	2790	2795	2800	rBV3	393	369	0.03%	0.004%
70	10.315	2800	2807	2810	rBV2	257	359	0.03%	0.004%
71	10.425	2838	2841	2843	rBV2	239	147	0.01%	0.002%
72	10.460	2845	2852	2860	rVV3	1825	2725	0.22%	0.029%
73	10.589	2889	2892	2894	rBV	227	167	0.01%	0.002%
74	10.621	2897	2902	2911	rVB5	1237	1857	0.15%	0.020%
75	10.679	2916	2920	2922	rBV2	326	231	0.02%	0.002%
76	10.730	2922	2936	2955	rBV	356956	603527	48.38%	6.394%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111825\
 Data File : VU063734.D
 Acq On : 18 Nov 2025 11:17
 Operator : MD/SY
 Sample : VU1118WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK128

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

77	10.872	2976	2980	2981	rBV3	299	201	0.02%	0.002%
78	10.929	2995	2998	3005	rBV2	301	313	0.03%	0.003%
79	11.068	3036	3041	3045	rBV2	1690	1789	0.14%	0.019%
80	11.267	3101	3103	3106	rVV	215	132	0.01%	0.001%
81	11.312	3115	3117	3120	rBV2	255	131	0.01%	0.001%
82	11.331	3120	3123	3125	rBV2	268	196	0.02%	0.002%
83	11.421	3146	3151	3152	rBV2	261	223	0.02%	0.002%
84	11.450	3152	3160	3178	rVB2	2771	4784	0.38%	0.051%
85	11.592	3199	3204	3208	rBV2	327	362	0.03%	0.004%
86	11.691	3231	3235	3238	rBV2	267	237	0.02%	0.003%
87	11.727	3238	3246	3253	rBV2	4510	6734	0.54%	0.071%
88	11.788	3253	3265	3289	rVV	514879	897736	71.96%	9.510%
89	11.991	3326	3328	3331	rBV3	432	291	0.02%	0.003%
90	12.042	3341	3344	3347	rBV	367	297	0.02%	0.003%
91	12.113	3363	3366	3370	rVB	503	361	0.03%	0.004%
92	12.167	3370	3383	3406	rBV	506684	871876	69.88%	9.237%
93	12.380	3447	3449	3451	rVB2	344	177	0.01%	0.002%
94	12.402	3451	3456	3459	rBV	531	586	0.05%	0.006%
95	12.437	3463	3467	3472	rBV2	579	649	0.05%	0.007%
96	12.579	3509	3511	3512	rBV	398	181	0.01%	0.002%
97	13.203	3699	3705	3712	rVB4	3217	4618	0.37%	0.049%
98	13.820	3889	3897	3909	rBV6	9094	14211	1.14%	0.151%
99	14.068	3966	3974	3994	rVB	13659	25970	2.08%	0.275%
100	14.306	4039	4048	4063	rBV4	8501	15080	1.21%	0.160%




Sum of corrected areas: 9439429

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111825\
Data File : VU063734.D
Acq On : 18 Nov 2025 11:17
Operator : MD/SY
Sample : VU1118WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK128

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

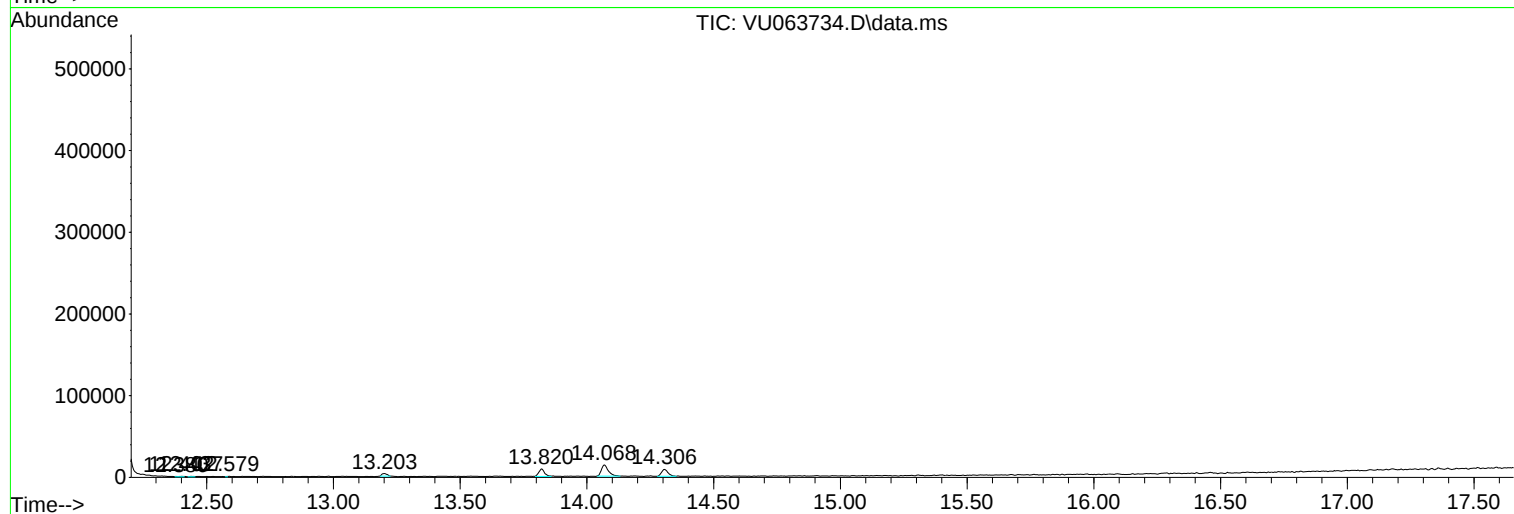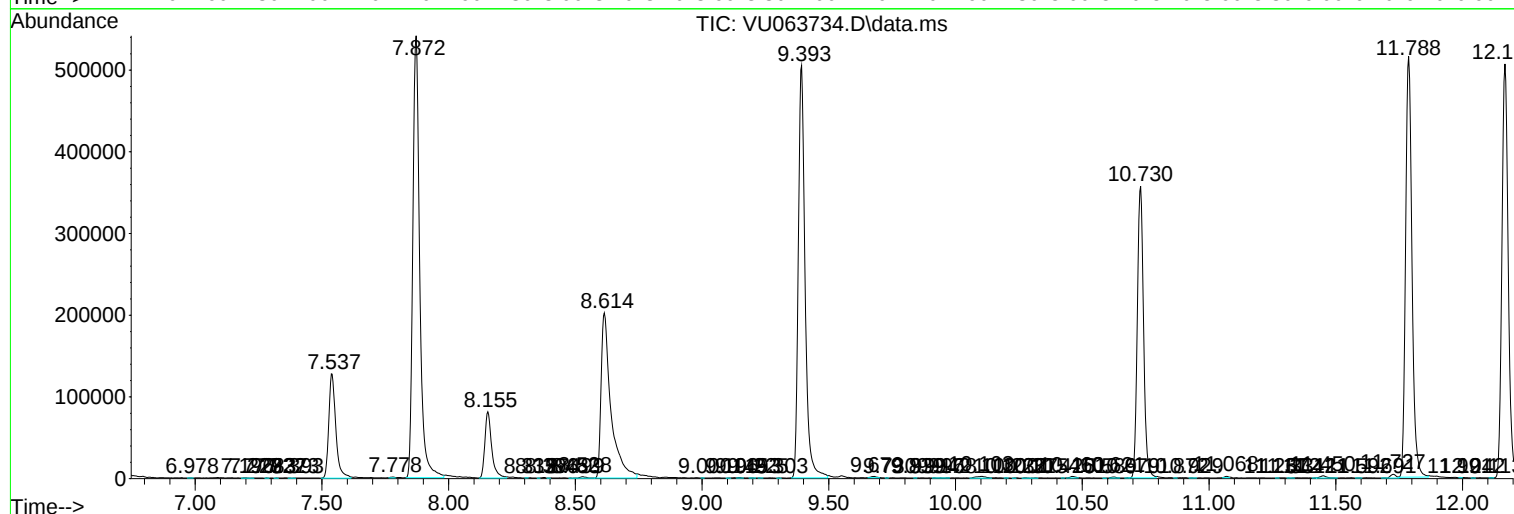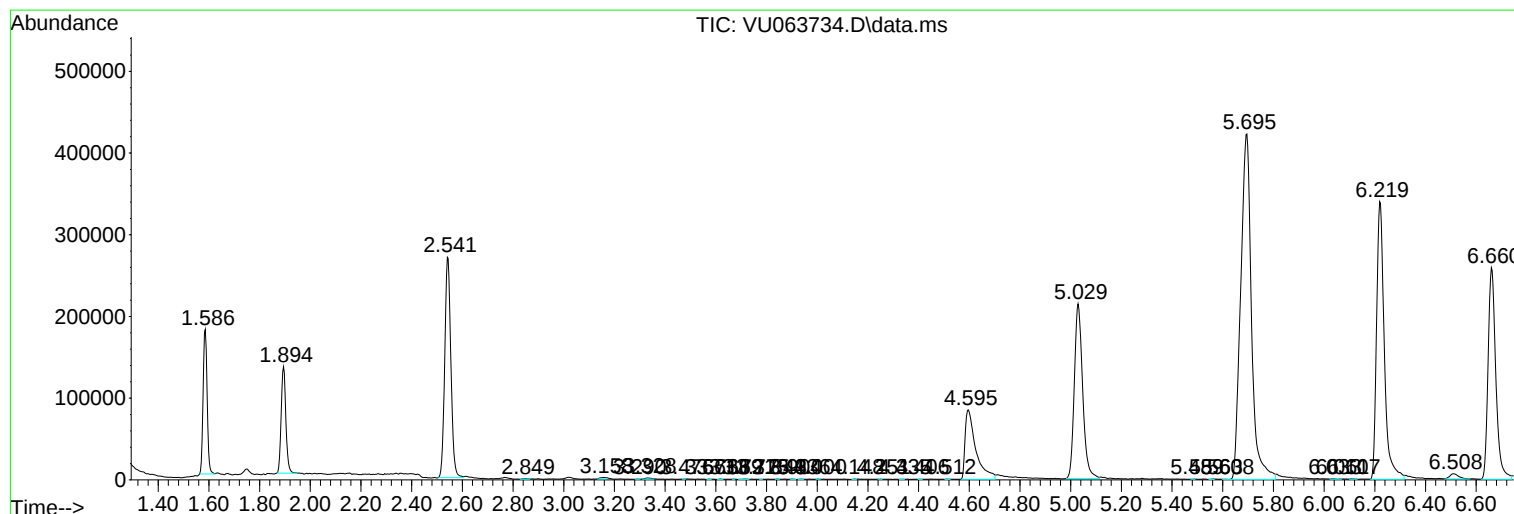

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111825\
Data File : VU063734.D
Acq On : 18 Nov 2025 11:17
Operator : MD/SY
Sample : VU1118WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK128

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111825\
Data File : VU063734.D
Acq On : 18 Nov 2025 11:17
Operator : MD/SY
Sample : VU1118WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK128

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------