
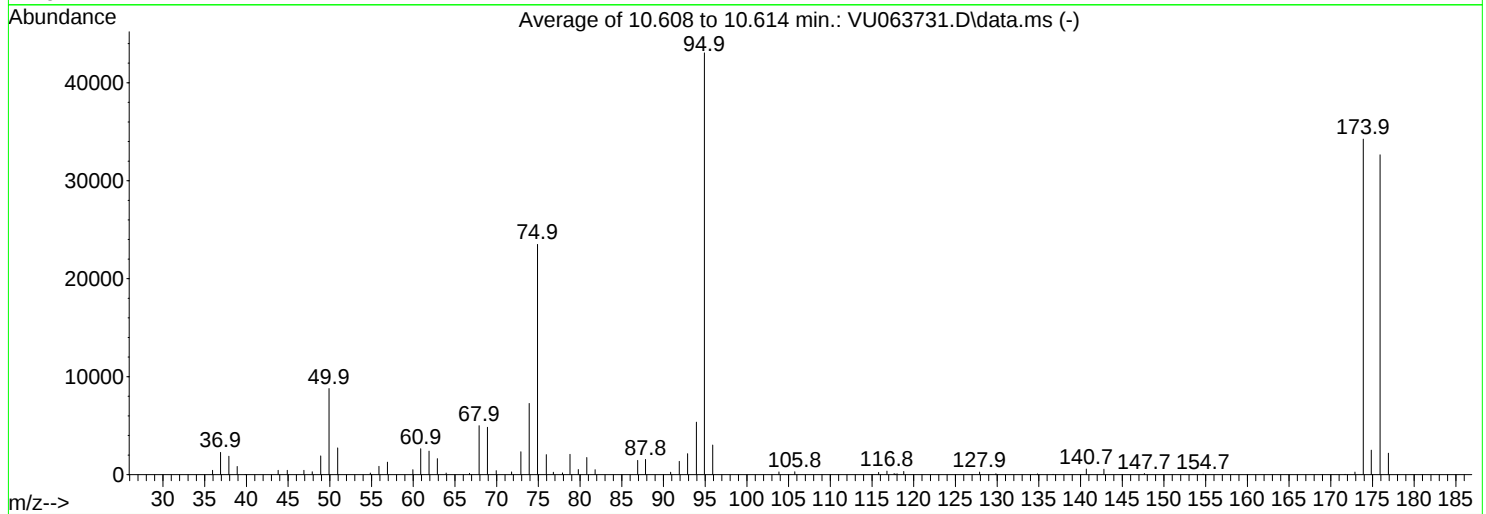


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111825\
Data File : VU063731.D
Acq On : 18 Nov 2025 08:48
Operator : MD/SY
Sample : BFB091
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB091

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Title : VOC Analysis
Last Update : Wed Nov 19 04:47:02 2025

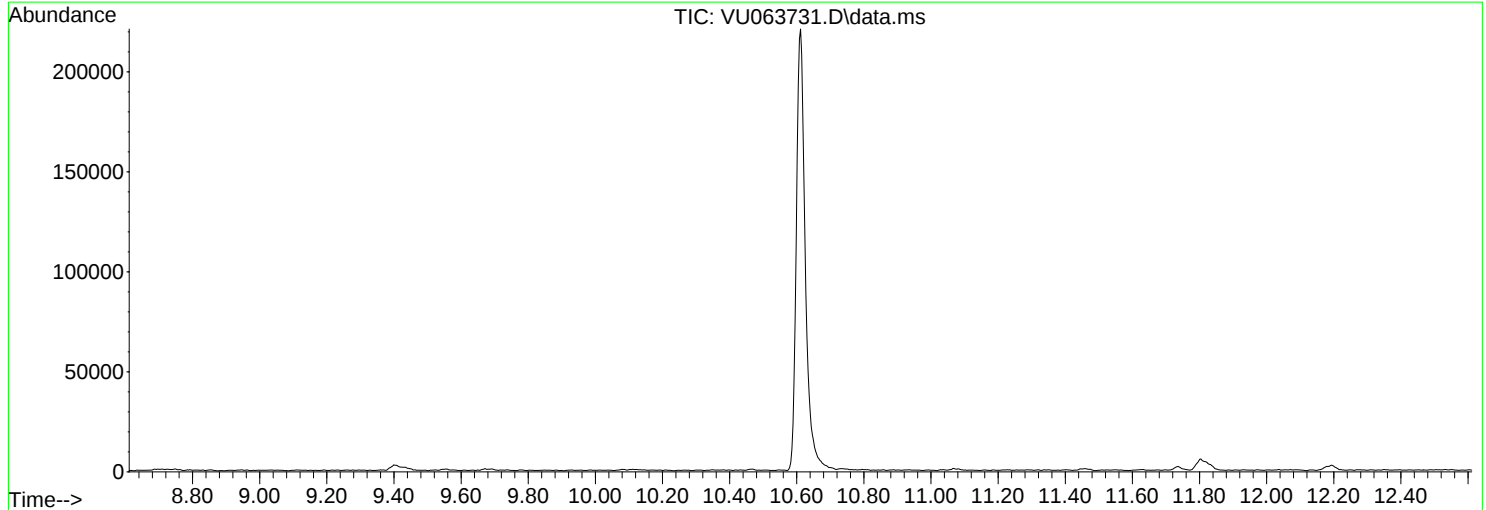

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2886

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.4	8780	PASS
75	95	30	80	54.6	23504	PASS
95	95	100	100	100.0	43053	PASS
96	95	5	9	7.0	3023	PASS
173	174	0.00	2	0.8	263	PASS
174	95	50	120	79.6	34253	PASS
175	174	5	9	7.3	2502	PASS
176	174	95	101	95.3	32651	PASS
177	176	5	9	6.7	2184	PASS

Scan 2886 (10.569 min): VU063731.D\data.ms
BFB091

m/z	Abundance
39.80	180.0
43.80	553.0

Instrument :
MSVOA_U
ClientSampleId :
BFB091

m/z	Abundance
35.90	397.0
36.90	2309.0
37.90	1788.0
38.90	900.0
39.80	248.0
43.90	1017.0
44.90	450.0
47.00	466.0
47.90	306.0
48.90	2103.0
49.90	9283.0
50.90	2699.0
54.90	147.0
55.90	906.0
56.90	1291.0
59.90	480.0
60.90	2647.0
61.90	2524.0
62.90	1583.0
63.90	184.0
66.80	142.0
67.90	5118.0
68.90	4732.0
69.90	364.0
71.80	239.0
72.90	2508.0
73.90	7196.0
74.90	23856.0
76.00	1970.0
76.80	230.0
78.00	194.0
78.80	2081.0
79.80	502.0
80.80	1836.0
81.80	565.0
86.90	1434.0
87.80	1547.0
90.80	217.0
91.90	1298.0
92.90	2169.0
94.00	5548.0
94.90	43096.0
95.90	3187.0
103.80	277.0
105.70	277.0
115.80	179.0
116.90	339.0
117.60	171.0
118.00	139.0
118.80	299.0
127.90	257.0
129.90	183.0
136.70	109.0
140.70	546.0
142.80	552.0
147.70	103.0
154.70	147.0
172.90	297.0
173.90	33880.0
174.80	2441.0
175.90	32136.0
176.90	2238.0

Instrument :
MSVOA_U
ClientSampleId :
BFB091

m/z	Abundance
35.90	446.0
36.90	2321.0
37.90	1926.0
38.90	841.0
39.90	200.0
43.90	993.0
44.90	458.0
46.90	431.0
47.90	305.0
48.90	1933.0
49.90	8990.0
51.00	2832.0
54.90	178.0
55.90	827.0
56.90	1279.0
60.00	550.0
60.90	2688.0
61.90	2470.0
62.90	1682.0
63.90	159.0
66.80	116.0
67.90	5163.0
68.90	4903.0
69.90	415.0
71.80	282.0
72.90	2385.0
73.90	7376.0
74.90	24176.0
75.90	2056.0
76.80	235.0
77.90	176.0
78.80	2152.0
79.80	543.0
80.80	1768.0
81.80	516.0
86.90	1493.0
87.80	1595.0
90.90	246.0
91.90	1401.0
92.90	2203.0
94.00	5537.0
94.90	44232.0
95.90	3116.0
103.90	283.0
105.80	302.0
115.80	246.0
116.80	379.0
117.70	154.0
118.00	151.0
118.80	354.0
127.90	265.0
129.80	134.0
134.80	116.0
140.70	586.0
142.80	554.0
147.70	107.0
171.70	108.0
172.90	255.0
173.90	35344.0
174.90	2583.0
175.90	33624.0
176.90	2244.0

Instrument :
MSVOA_U
ClientSampleId :
BFB091

m/z	Abundance
36.00	472.0
36.90	2206.0
37.90	1934.0
38.90	757.0
40.00	168.0
43.80	993.0
44.90	394.0
46.80	423.0
47.90	278.0
48.90	1718.0
49.90	8068.0
50.90	2655.0
54.80	159.0
55.90	796.0
56.90	1239.0
59.90	505.0
60.90	2594.0
61.90	2200.0
62.90	1645.0
64.00	157.0
66.70	122.0
67.90	4726.0
68.90	4893.0
70.00	431.0
71.80	292.0
72.90	2124.0
73.90	7218.0
74.90	22480.0
75.90	2075.0
76.80	258.0
77.80	184.0
78.80	1976.0
79.80	524.0
80.80	1637.0
81.80	450.0
86.90	1420.0
87.90	1501.0
90.90	277.0
91.90	1360.0
92.90	2050.0
93.90	4999.0
94.90	41832.0
95.90	2765.0
103.90	252.0
105.80	308.0
115.80	247.0
116.70	365.0
117.80	170.0
118.80	349.0
127.90	250.0
134.90	133.0
140.70	587.0
142.80	553.0
147.60	121.0
172.90	238.0
173.90	33536.0
174.90	2481.0
175.90	32192.0
176.90	2071.0

Instrument :
MSVOA_U
ClientSampleId :
BFB091