


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU111918\
Data File : VU028241.D
Acq On : 19 Nov 2018 09:03
Operator : MD/SY
Sample : BFB56
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB56

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111718WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Nov 20 07:07:24 2018

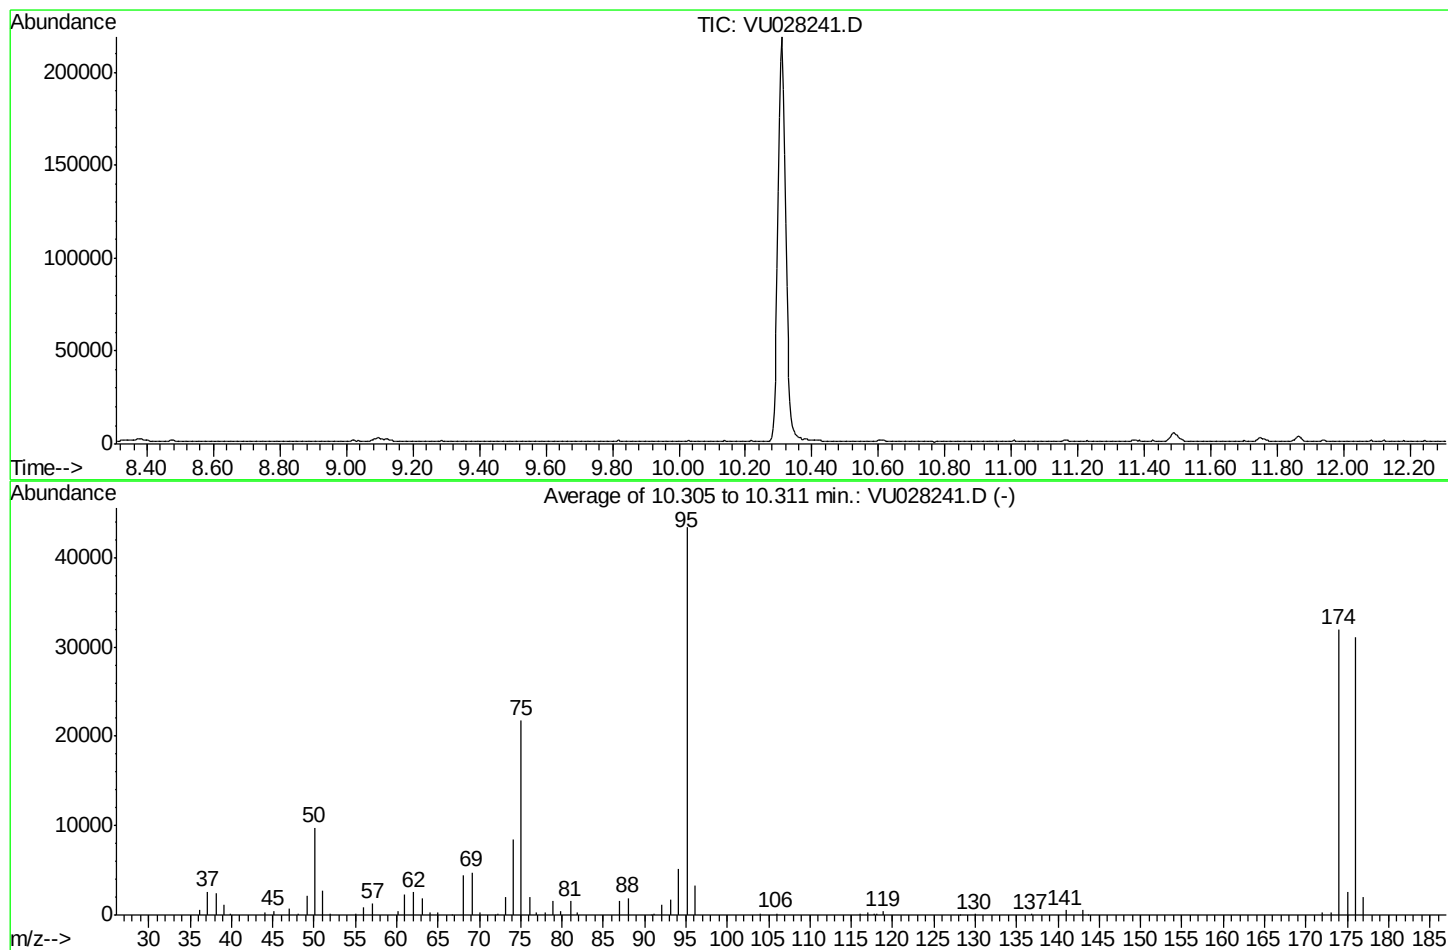

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	9785	PASS
75	95	30	80	50.2	21773	PASS
95	95	100	100	100.0	43397	PASS
96	95	5	9	7.5	3236	PASS
173	174	0.00	2	0.8	251	PASS
174	95	50	120	73.6	31941	PASS
175	174	5	9	8.3	2644	PASS
176	174	95	101	97.2	31034	PASS
177	176	5	9	6.6	2035	PASS

m/z	Abundance
40.00	244.0
44.10	1070.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56

m/z	Abundance
36.10	492.0
37.10	2465.0
38.10	2354.0
39.10	1087.0
39.90	360.0
44.00	1379.0
45.10	484.0
47.00	787.0
48.10	198.0
49.10	2168.0
50.10	9374.0
51.10	2921.0
52.00	150.0
55.00	176.0
56.10	838.0
57.10	1265.0
60.10	449.0
61.00	2207.0
62.10	2538.0
63.10	1834.0
64.00	238.0
64.90	323.0
68.10	4345.0
69.10	4823.0
70.10	369.0
72.20	281.0
73.10	2248.0
74.10	8377.0
75.10	21144.0
76.10	2013.0
77.00	344.0
77.90	266.0
78.90	1560.0
79.90	481.0
81.00	1487.0
81.90	368.0
87.00	1656.0
88.00	1785.0
91.10	182.0
92.10	1190.0
93.10	1754.0
94.10	4926.0
95.10	43784.0
96.10	3020.0
104.00	180.0
106.00	220.0
116.00	220.0
116.90	311.0
117.80	137.0
118.90	343.0
128.10	107.0
130.00	119.0
141.00	604.0
143.00	565.0
172.00	379.0
174.00	33240.0
175.00	2754.0
176.00	31856.0
177.00	2061.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56

m/z	Abundance
36.10	525.0
37.10	2797.0
38.10	2578.0
39.10	1167.0
40.00	409.0
44.00	1299.0
45.10	495.0
47.00	821.0
48.20	199.0
49.10	2346.0
50.10	10072.0
51.10	2838.0
52.00	117.0
55.00	190.0
56.00	888.0
57.10	1309.0
60.10	518.0
61.00	2407.0
62.10	2617.0
63.10	1892.0
64.00	236.0
65.10	261.0
66.70	109.0
68.10	4550.0
69.10	4935.0
70.10	328.0
72.20	243.0
73.10	2115.0
74.10	8718.0
75.10	22208.0
76.10	2135.0
77.00	334.0
77.90	311.0
79.00	1577.0
79.90	429.0
81.00	1614.0
81.90	337.0
87.00	1584.0
88.00	1958.0
91.10	180.0
92.10	1188.0
93.10	1821.0
94.10	5408.0
95.10	44800.0
96.10	3361.0
104.00	168.0
106.00	200.0
116.00	232.0
117.00	334.0
117.80	124.0
118.20	126.0
118.90	394.0
129.90	108.0
136.70	146.0
141.00	594.0
143.00	560.0
143.70	120.0
172.00	340.0
174.00	32760.0
175.00	2716.0
176.00	31856.0
177.00	2034.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56

m/z	Abundance
36.10	501.0
37.10	2704.0
38.10	2582.0
39.10	1098.0
40.00	450.0
44.00	1211.0
45.10	520.0
47.10	642.0
48.10	194.0
49.10	2076.0
50.10	9911.0
51.10	2421.0
52.00	105.0
55.00	134.0
56.00	798.0
57.10	1207.0
60.10	505.0
61.00	2377.0
62.10	2533.0
63.10	1709.0
64.00	278.0
65.10	241.0
68.10	4611.0
69.10	4592.0
70.10	287.0
72.00	152.0
73.10	1861.0
74.10	8194.0
75.10	21968.0
76.10	1962.0
76.90	291.0
77.90	241.0
79.00	1494.0
79.90	325.0
81.00	1552.0
81.90	276.0
87.00	1641.0
88.00	1879.0
90.80	112.0
91.10	117.0
92.10	1151.0
93.10	1755.0
94.10	5017.0
95.10	41608.0
96.10	3329.0
104.00	151.0
106.00	152.0
116.00	202.0
117.00	299.0
118.10	143.0
118.90	388.0
129.90	106.0
136.80	146.0
141.00	509.0
143.00	464.0
143.70	101.0
172.00	246.0
173.10	755.0
174.00	29824.0
175.00	2463.0
176.00	29392.0
177.00	2010.0

Instrument :
MSVOA_U
ClientSampleId :
BFB56