

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U111919\
 Data File : VU035773.D
 Acq On : 19 Nov 2019 16:30
 Operator : JC/SP
 Sample : K5910-14DLRE 5X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GAQJ7DLRE

Quant Time: Nov 20 02:46:27 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR110419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Nov 20 00:37:27 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	190426	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	226419	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.85	152	76877	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.62	65	78451	4.00	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.00%
7) Chloroethane-d5	1.93	69	78693	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.20%
11) 1,1-Dichloroethene-d2	2.60	63	106764	3.24	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.80%
20) 2-Butanone-d5	4.70	46	236242	54.59	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.18%
24) Chloroform-d	5.11	84	162230	5.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.80%
26) 1,2-Dichloroethane-d4	5.75	65	87260	5.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.40%
32) Benzene-d6	5.77	84	312058	4.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.60%
36) 1,2-Dichloropropane-d6	6.74	67	108196	4.70	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.00%
41) Toluene-d8	7.93	98	255073	3.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.60%
43) trans-1,3-Dichloropropene-	8.22	79	37735	4.10	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.00%
46) 2-Hexanone-d5	8.70	63	163687	45.38	ug/L	0.02
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.76%
57) 1,1,2,2-Tetrachloroethane-	10.79	84	94919	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.20%
64) 1,2-Dichlorobenzene-d4	12.22	152	79039	5.19	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.80%

Target Compounds


					Ovalue
13) Acetone	2.67	43	7480	2.397 ug/L	91
22) cis-1,2-Dichloroethene	4.72	96	9660	0.507 ug/L	100
34) Trichloroethene	6.58	95	187300	9.185 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU111919\
Data File : VU035773.D
Acq On : 19 Nov 2019 16:30
Operator : JC/SP
Sample : K5910-14DLRE 5X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GAQJ7DLRE

Quant Time: Nov 20 02:46:27 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR110419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 20 00:37:27 2019
Response via : Initial Calibration

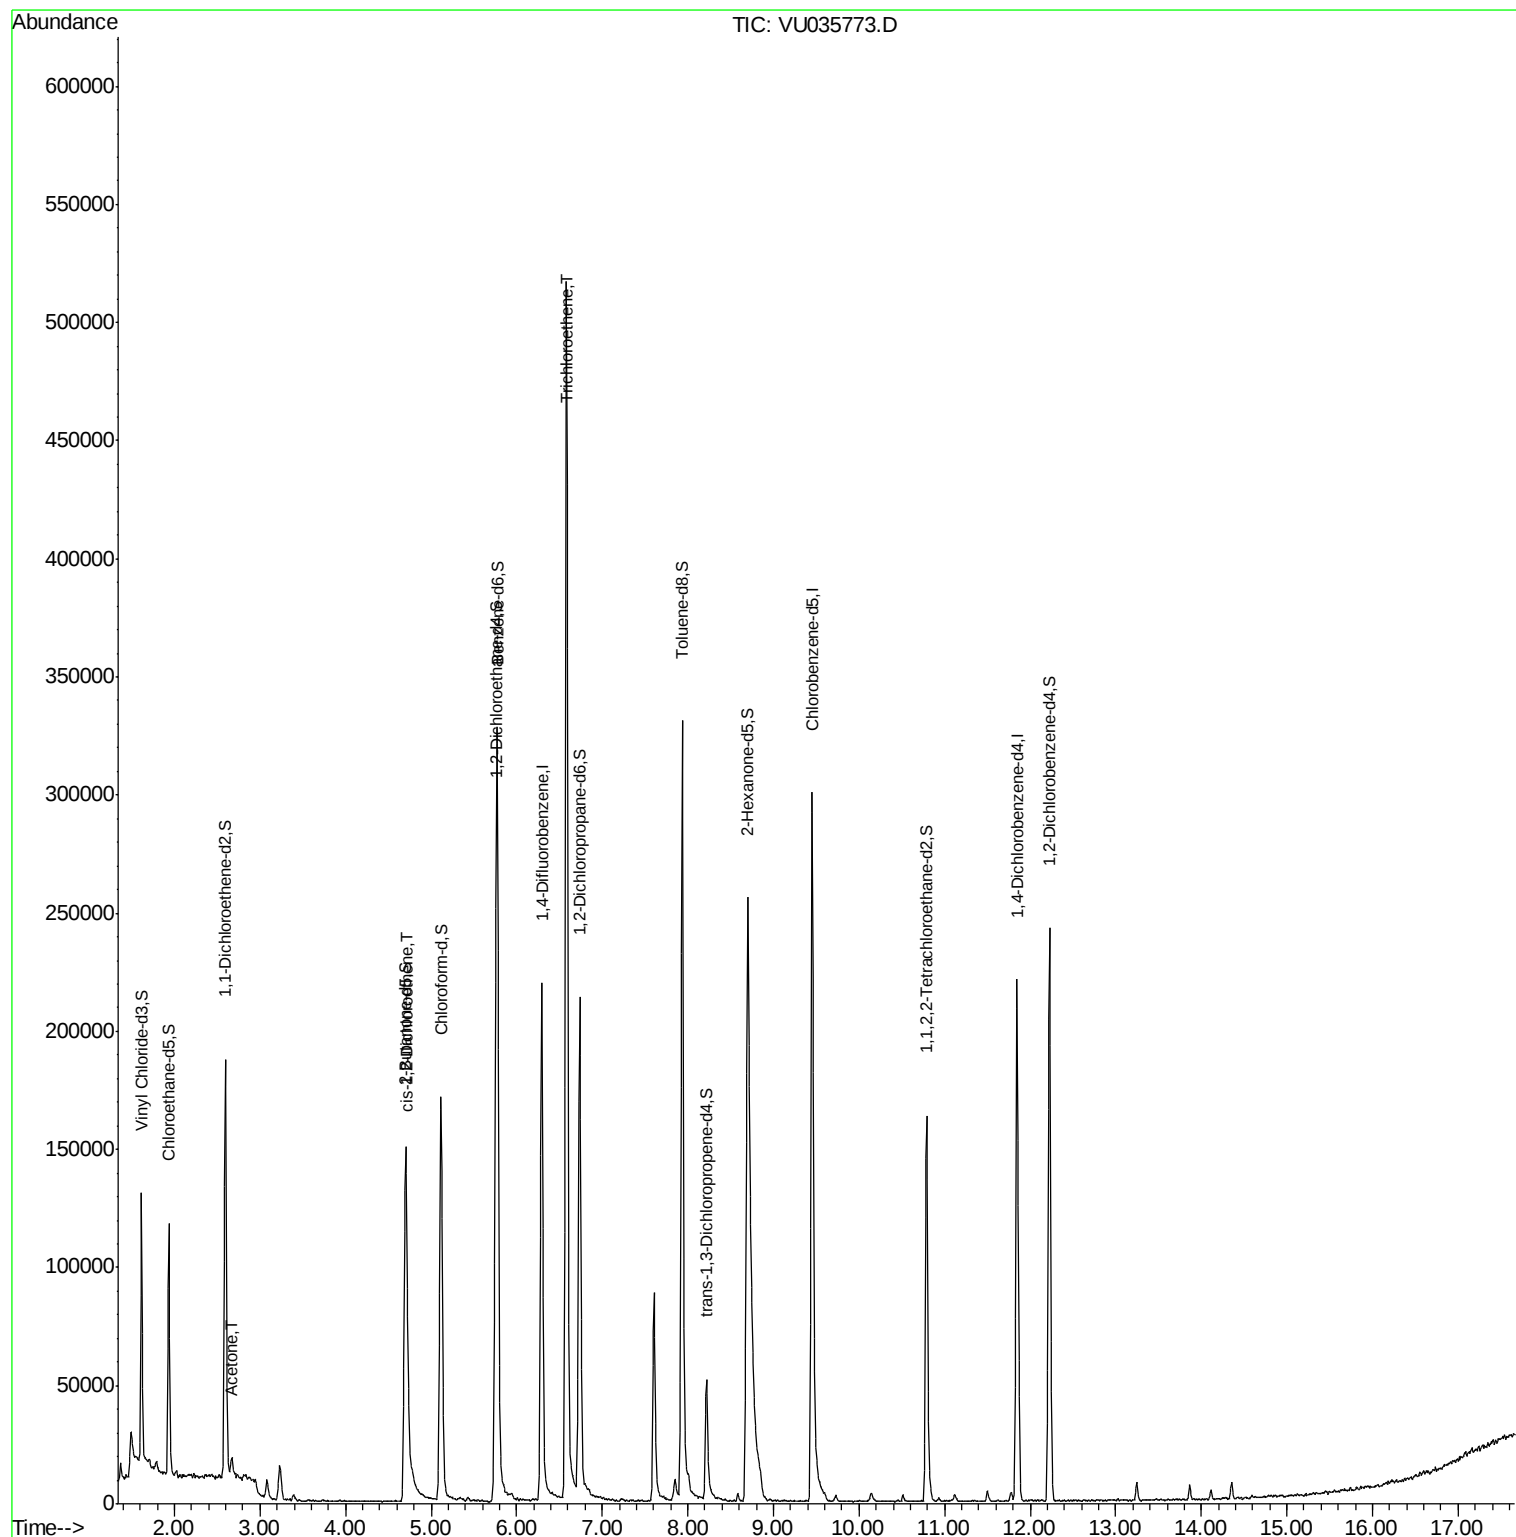

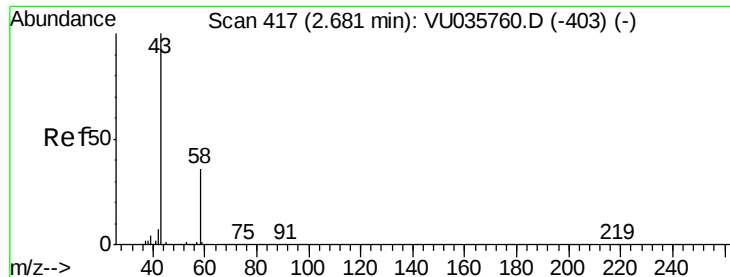

#13

Acetone

Concen: 2.397 ug/L

RT: 2.67 min Scan# 413

Delta R.T. -0.01 min

Lab File: VU035773.D

Acq: 19 Nov 2019 16:30

Instrument :

MSVOA_U

ClientSampleId :


GAQJ7DLRE

Tot Ion: 43 Resp: 7480

Ion Ratio Lower Upper




43 100

58 40.3 0.0 69.8

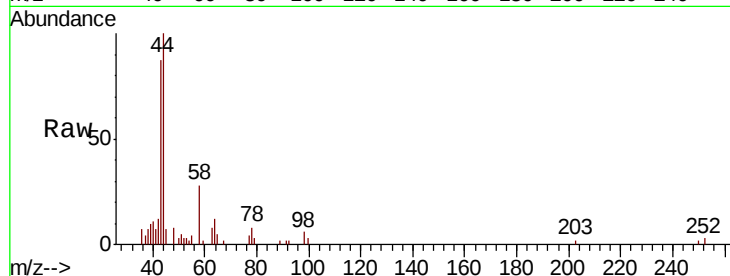

Abundance Ion 43.05 (42.75 to 43.75): VU035773.D (-324) (-)

Ion 58.05 (57.75 to 58.75): VU035773.D (-324) (-)

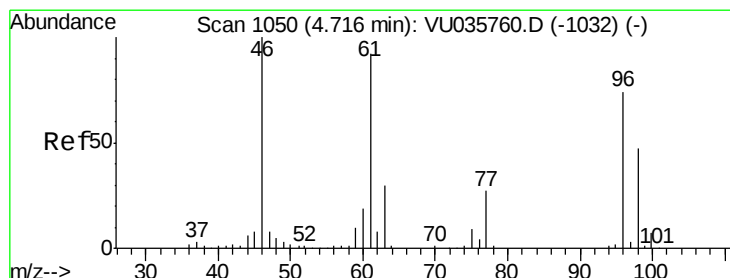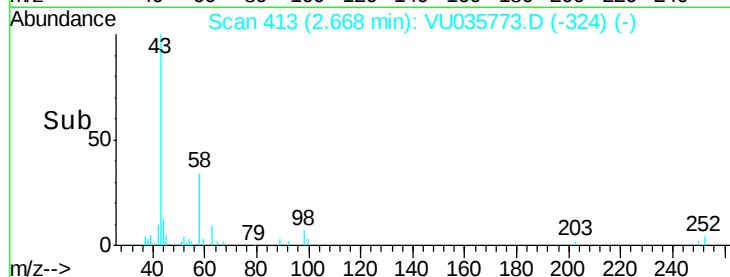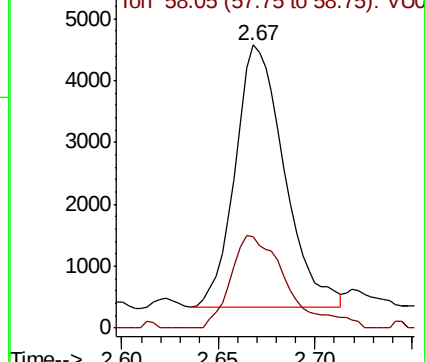

#22

cis-1,2-Dichloroethene

Concen: 0.507 ug/L

RT: 4.72 min Scan# 1051

Delta R.T. 0.00 min

Lab File: VU035773.D

Acq: 19 Nov 2019 16:30


Tgt Ion: 96 Resp: 9660

Ion Ratio Lower Upper

96 100

61 123.8 87.0 161.6



68 0.0 0.0 0.0

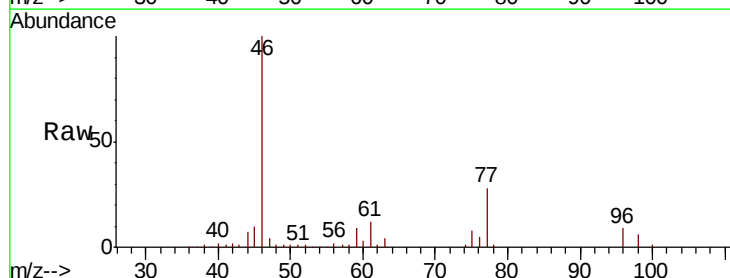


Abundance Ion 96.00 (95.70 to 96.70): VU035773.D (-957) (-)

Ion 61.05 (60.75 to 61.75): VU035773.D (-957) (-)

Ion 68.15 (67.85 to 68.85): VU035773.D (-957) (-)

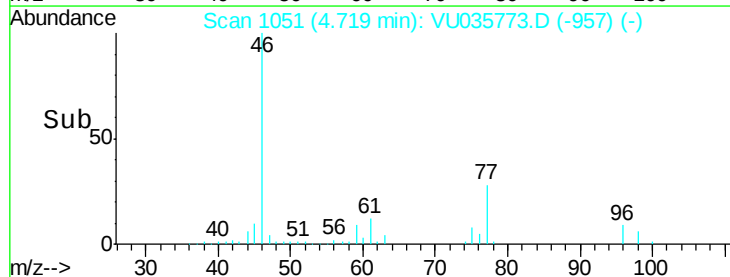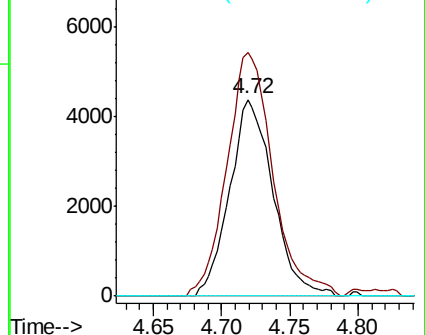

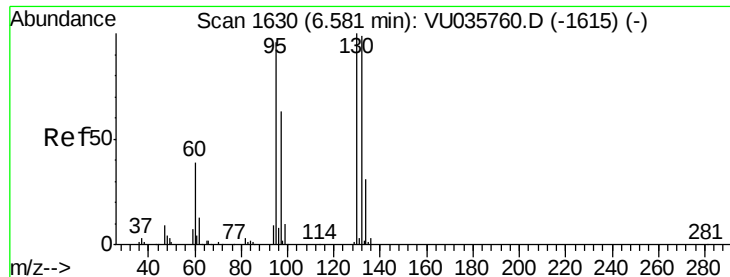

#34

Trichloroethene

Concen: 9.185 ug/L

RT: 6.58 min Scan# 1631

Delta R.T. 0.00 min

Lab File: VU035773.D


Acq: 19 Nov 2019 16:30

Instrument :

MSVOA_U

ClientSampleId :

GAQJ7DLRE

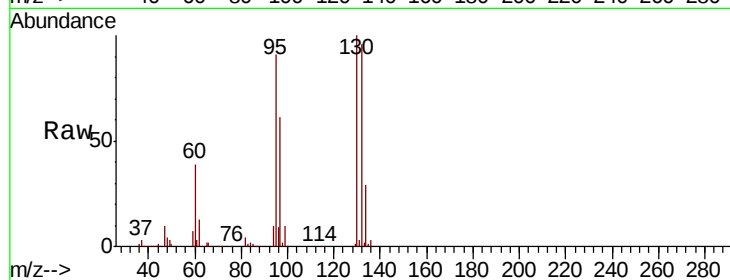

Tot Ion: 95 Resp: 187300

Ion Ratio Lower Upper

95 100

97 67.0 44.5 82.7

132 105.8 69.9 129.7

130 110.3 74.1 137.7

Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

