


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU111919\
 Data File : VU035759.D
 Acq On : 19 Nov 2019 08:41
 Operator : JC/MD
 Sample : BFB02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB02

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR110419WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Nov 22 08:26:38 2019

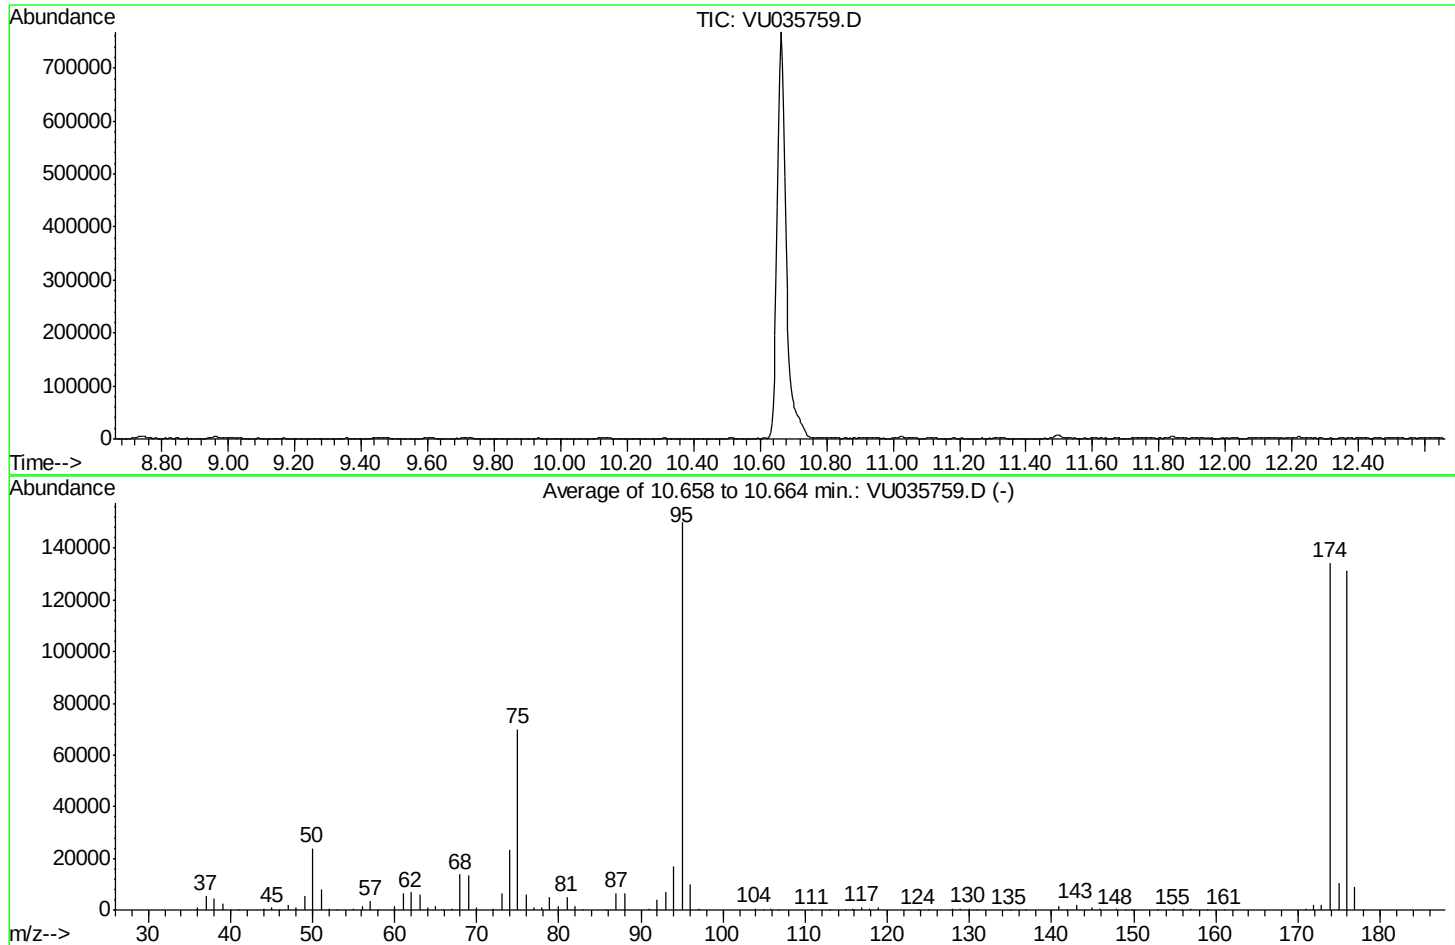

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	23922	PASS
75	95	30	80	46.6	69882	PASS
95	95	100	100	100.0	150037	PASS
96	95	5	9	6.5	9736	PASS
173	174	0.00	2	1.4	1931	PASS
174	95	50	120	89.5	134322	PASS
175	174	5	9	7.9	10564	PASS
176	174	95	101	97.6	131125	PASS
177	176	5	9	6.7	8742	PASS

m/z	Abundance
36.00	1064.0
37.00	5291.0
38.00	4582.0
39.10	2332.0
40.00	405.0
44.00	1357.0
45.10	866.0
45.90	195.0
47.10	1578.0
47.90	710.0
49.00	4958.0
50.00	22232.0
51.10	7694.0
52.00	361.0
52.90	181.0
55.00	485.0
56.10	1641.0
57.10	3499.0
58.00	127.0
60.00	1419.0
61.10	5778.0
62.00	6438.0
63.00	5527.0
64.00	1213.0
65.00	1041.0
65.90	125.0
66.90	334.0
68.00	12930.0
69.00	12723.0
70.00	1079.0
72.00	784.0
73.00	6069.0
74.00	21976.0
75.00	65968.0
76.00	5877.0
76.90	813.0
77.90	791.0
78.90	4735.0
79.90	1563.0
80.90	4782.0
81.90	1165.0
82.90	137.0
85.80	104.0
87.00	6154.0
88.00	6092.0
91.00	405.0
92.00	3708.0
93.00	6526.0
94.00	15917.0
95.00	142592.0
96.00	9277.0
97.20	230.0
103.90	523.0
104.90	262.0
105.80	559.0
110.90	116.0
112.90	122.0
114.80	237.0
115.80	442.0
116.90	1093.0
117.90	540.0
118.90	974.0
124.90	103.0
127.90	458.0
128.90	270.0
129.90	438.0
130.90	181.0
134.90	256.0
136.80	209.0
140.90	1194.0
141.80	127.0
143.00	1959.0
144.10	133.0
145.00	1036.0
145.80	290.0
147.90	277.0
149.80	106.0
154.80	392.0
156.90	306.0
158.90	269.0
161.10	136.0
171.00	478.0
171.90	2034.0
172.90	1851.0
174.00	122456.0
175.00	9905.0
175.90	119648.0
176.90	8059.0
178.00	154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

m/z	Abundance
36.00	1102.0
37.00	5873.0
38.00	4610.0
39.10	2647.0
40.00	430.0
44.00	1500.0
45.00	955.0
45.90	240.0
47.10	1768.0
48.00	883.0
49.00	5425.0
50.00	24640.0
51.00	8154.0
52.00	364.0
52.90	203.0
55.00	473.0
56.10	1751.0
57.00	3507.0
57.90	177.0
60.00	1429.0
61.00	6394.0
62.00	6892.0
63.00	5994.0
64.00	1267.0
65.00	1368.0
65.90	170.0
66.90	334.0
68.00	14104.0
69.00	13828.0
70.00	1091.0
72.00	785.0
73.00	6422.0
74.10	23696.0
75.00	71744.0
76.00	6182.0
77.00	1040.0
77.90	870.0
78.90	5136.0
80.00	1644.0
81.00	5231.0
81.90	1390.0
82.90	132.0
85.70	100.0
87.00	6806.0
88.00	6454.0
91.00	445.0
92.00	4159.0
93.00	7020.0
94.00	17512.0
95.00	154304.0
96.00	9999.0
97.10	315.0
103.90	596.0
104.90	241.0
105.80	533.0
110.90	130.0
113.00	135.0
114.80	241.0
115.70	475.0
116.90	1223.0
117.90	545.0
118.90	995.0
123.80	104.0
127.90	496.0
128.90	319.0
129.90	552.0
130.90	185.0
134.90	266.0
136.80	229.0
140.90	1449.0
141.80	138.0
143.00	2243.0
144.10	115.0
144.90	1100.0
145.80	281.0
147.80	289.0
148.90	129.0
149.80	110.0
154.80	424.0
155.90	101.0
156.90	383.0
158.90	278.0
161.10	152.0
171.00	453.0
171.90	2165.0
172.90	2029.0
174.00	137664.0
174.90	10857.0
175.90	135360.0
176.90	9072.0
178.00	171.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

m/z	Abundance
36.00	1013.0
37.00	5976.0
38.00	4405.0
39.10	2468.0
40.00	429.0
40.90	100.0
44.00	1568.0
45.00	1069.0
45.90	237.0
47.10	1963.0
48.00	938.0
49.00	5418.0
50.00	24896.0
51.00	7800.0
52.00	337.0
53.00	240.0
55.00	420.0
56.10	1647.0
57.00	3458.0
57.90	174.0
60.00	1282.0
61.00	6685.0
62.00	6892.0
63.10	5977.0
64.00	1271.0
65.00	1561.0
65.90	147.0
67.00	368.0
68.00	13903.0
69.10	13618.0
70.00	967.0
72.00	704.0
73.00	6185.0
74.00	23544.0
75.00	71936.0
76.00	5964.0
77.00	1224.0
77.90	868.0
78.90	5283.0
80.00	1631.0
81.00	5176.0
81.90	1531.0
82.90	116.0
85.70	124.0
87.00	6732.0
88.00	6208.0
90.90	469.0
92.00	4290.0
93.00	6761.0
94.00	17480.0
95.00	153216.0
96.00	9932.0
97.00	405.0
103.90	658.0
104.90	195.0
105.80	462.0
106.70	131.0
110.80	116.0
113.00	110.0
114.80	238.0
115.80	432.0
116.00	431.0
116.90	1279.0
117.80	517.0
118.90	976.0
123.80	114.0
127.90	479.0
128.90	318.0
129.90	622.0
130.80	177.0
135.00	247.0
136.90	244.0
140.90	1397.0
141.90	128.0
143.00	2361.0
144.00	128.0
144.90	1172.0
145.80	221.0
147.80	290.0
149.00	153.0
150.10	136.0
152.80	119.0
154.90	360.0
155.80	138.0
156.90	366.0
158.90	206.0
161.00	156.0
171.00	399.0
171.90	2173.0
172.90	1915.0
173.90	142848.0
174.90	10932.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

175.90138368.0

176.909097.0

177.90218.0

Instrument :
MSVOA_U

ClientSampleId :
BFB02

Scan 2884 (10.613 min): VU035759.D
BFB02

m/z	Abundance
40.00	395.0
44.00	987.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02