
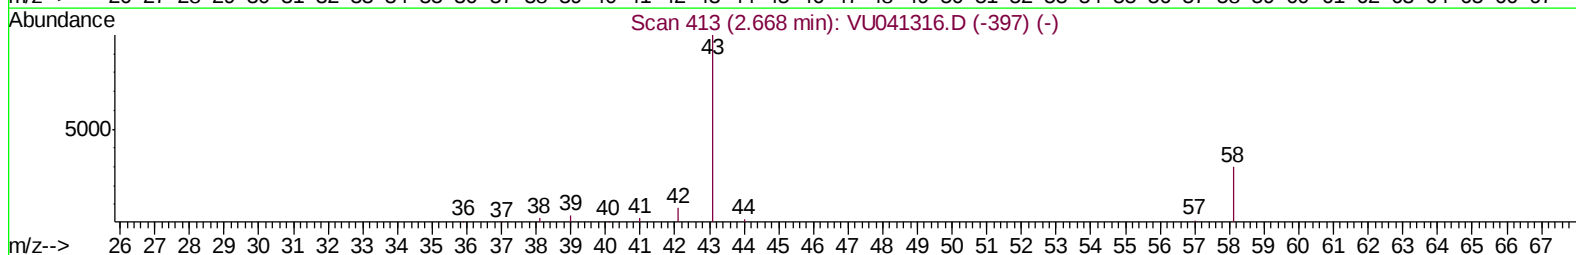
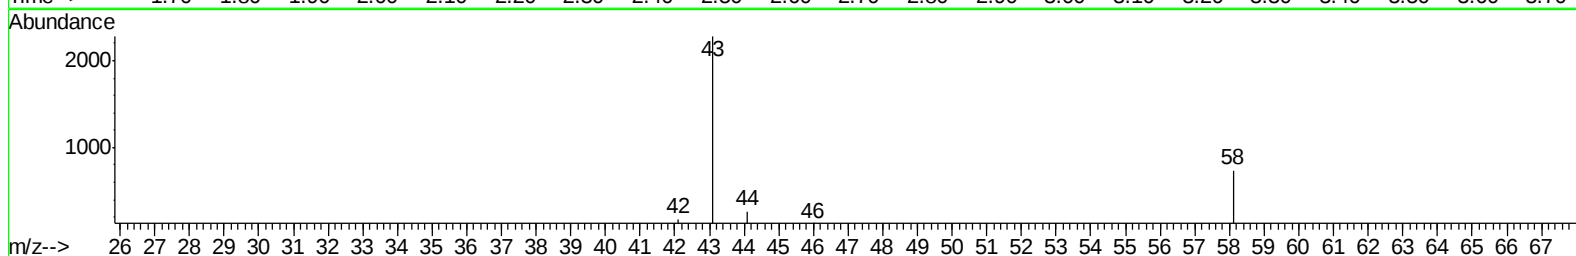


Data File : VU041323.D
Acq On : 18 Nov 2020 19:49
Operator : SY/MD
Sample : L4790-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 19 00:52:32 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Nov 19 00:50:13 2020
Response via : Initial Calibration

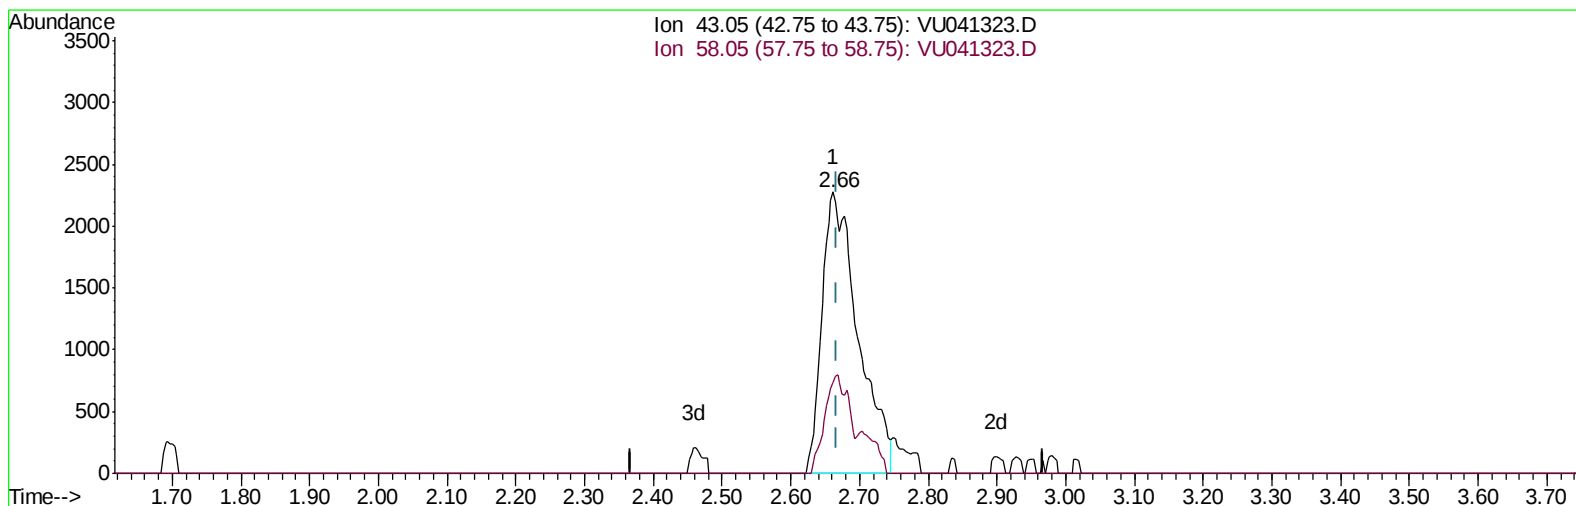

TIC: VU041323.D

(13) Acetone (T)

2.662min (-0.006) 6.68ug/L m

response 8266

Ion	Exp%	Act%
43.05	100	100
58.05	12.70	23.45
0.00	0.00	0.00
0.00	0.00	0.00