

Data File : VU041334.D  
Acq On : 19 Nov 2020 00:10  
Operator : SY/MD  
Sample : L4790-18  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
H4419

Quant Time: Nov 19 00:54:54 2020  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMUTR111620WMA.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Thu Nov 19 00:50:13 2020  
Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|----------------------------|-------|------|----------|------|-------|----------|
| 1) 1,4-Difluorobenzene     | 6.26  | 114  | 63348    | 5.00 | ug/L  | 0.00     |
| 28) Chlorobenzene-d5       | 9.42  | 117  | 65869    | 5.00 | ug/L  | 0.00     |
| 60) 1,4-Dichlorobenzene-d4 | 11.81 | 152  | 27005    | 5.00 | ug/L  | 0.00     |

#### System Monitoring Compounds

|                                |        |       |          |          |      |         |
|--------------------------------|--------|-------|----------|----------|------|---------|
| 4) Vinyl Chloride-d3           | 1.60   | 65    | 20314    | 4.36     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 40 - 130 | Recovery | =    | 87.20%  |
| 7) Chloroethane-d5             | 1.92   | 69    | 18000    | 4.52     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 65 - 130 | Recovery | =    | 90.40%  |
| 11) 1,1-Dichloroethene-d2      | 2.58   | 63    | 31753    | 3.30     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 60 - 125 | Recovery | =    | 66.00%  |
| 20) 2-Butanone-d5              | 4.65   | 46    | 91069    | 47.40    | ug/L | 0.00    |
| Spiked Amount                  | 50.000 | Range | 40 - 130 | Recovery | =    | 94.80%  |
| 24) Chloroform-d               | 5.08   | 84    | 49525    | 4.91     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 125 | Recovery | =    | 98.20%  |
| 26) 1,2-Dichloroethane-d4      | 5.72   | 65    | 31410    | 4.78     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 130 | Recovery | =    | 95.60%  |
| 32) Benzene-d6                 | 5.74   | 84    | 85502    | 4.82     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 125 | Recovery | =    | 96.40%  |
| 36) 1,2-Dichloropropane-d6     | 6.70   | 67    | 29242    | 4.78     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 60 - 140 | Recovery | =    | 95.60%  |
| 41) Toluene-d8                 | 7.91   | 98    | 69292    | 4.14     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 130 | Recovery | =    | 82.80%  |
| 43) trans-1,3-Dichloropropene- | 8.19   | 79    | 11642    | 4.42     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 55 - 130 | Recovery | =    | 88.40%  |
| 46) 2-Hexanone-d5              | 8.64   | 63    | 62422    | 44.37    | ug/L | 0.00    |
| Spiked Amount                  | 50.000 | Range | 45 - 130 | Recovery | =    | 88.74%  |
| 57) 1,1,2,2-Tetrachloroethane- | 10.75  | 84    | 27179    | 4.58     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 65 - 120 | Recovery | =    | 91.60%  |
| 64) 1,2-Dichlorobenzene-d4     | 12.19  | 152   | 26904    | 5.11     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 80 - 120 | Recovery | =    | 102.20% |

#### Target Compounds

|                               |       |    |        |               | Qvalue |
|-------------------------------|-------|----|--------|---------------|--------|
| 3) Chloromethane              | 1.53  | 50 | 528    | 0.094 ug/L    | 98     |
| 5) Vinyl chloride             | 1.61  | 62 | 69419  | 12.623 ug/L # | 72     |
| 8) Chloroethane               | 2.04  | 64 | 864    | 0.237 ug/L #  | 51     |
| 13) Acetone                   | 2.66  | 43 | 1943   | 1.524 ug/L    | 91     |
| 14) Carbon disulfide          | 2.81  | 76 | 1795   | 0.148 ug/L #  | 74     |
| 17) Methyl tert-butyl Ether   | 3.38  | 73 | 120034 | 10.633 ug/L   | 100    |
| 18) trans-1,2-Dichloroethene  | 3.37  | 96 | 21716  | 5.407 ug/L    | 96     |
| 19) 1,1-Dichloroethane        | 3.89  | 63 | 7065   | 0.787 ug/L    | 97     |
| 22) cis-1,2-Dichloroethene    | 4.68  | 96 | 6338   | 1.397 ug/L    | 87     |
| 33) Benzene                   | 5.79  | 78 | 6668   | 0.374 ug/L    | 100    |
| 34) Trichloroethene           | 6.55  | 95 | 1328   | 0.275 ug/L #  | 77     |
| 35) Methylcyclohexane         | 6.70  | 83 | 6946   | 1.084 ug/L #  | 13     |
| 37) 1,2-Dichloropropane       | 6.70  | 63 | 3454   | 0.662 ug/L #  | 86     |
| 39) cis-1,3-Dichloropropene   | 7.57  | 75 | 865    | 0.119 ug/L #  | 81     |
| 42) Toluene                   | 7.98  | 91 | 4501   | 0.236 ug/L    | 85     |
| 44) trans-1,3-Dichloropropene | 8.19  | 75 | 433    | 0.063 ug/L #  | 43     |
| 59) 1,2,3-Trichloropropane    | 11.81 | 75 | 3387   | 0.823 ug/L    | 91     |

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_U\DATA\VU111920\  
Quantitation Report (Not Reviewed)

Data File : VU041334.D  
Acq On : 19 Nov 2020 00:10  
Operator : SY/MD  
Sample : L4790-18  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
H4419

Quant Time: Nov 19 00:54:54 2020  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMUTR111620WMA.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Thu Nov 19 00:50:13 2020  
Response via : Initial Calibration


| Internal Standards | R.T.  | QIon | Response | Conc  | Units  | Dev(Min) |
|--------------------|-------|------|----------|-------|--------|----------|
| 69) Naphthalene    | 14.08 | 128  | 683      | 0.088 | ug/L # | 81       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU041334.D  
Acq On : 19 Nov 2020 00:10  
Operator : SY/MD  
Sample : L4790-18  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
H4419

Quant Time: Nov 19 00:54:54 2020  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMUTR111620WMA.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Thu Nov 19 00:50:13 2020  
Response via : Initial Calibration

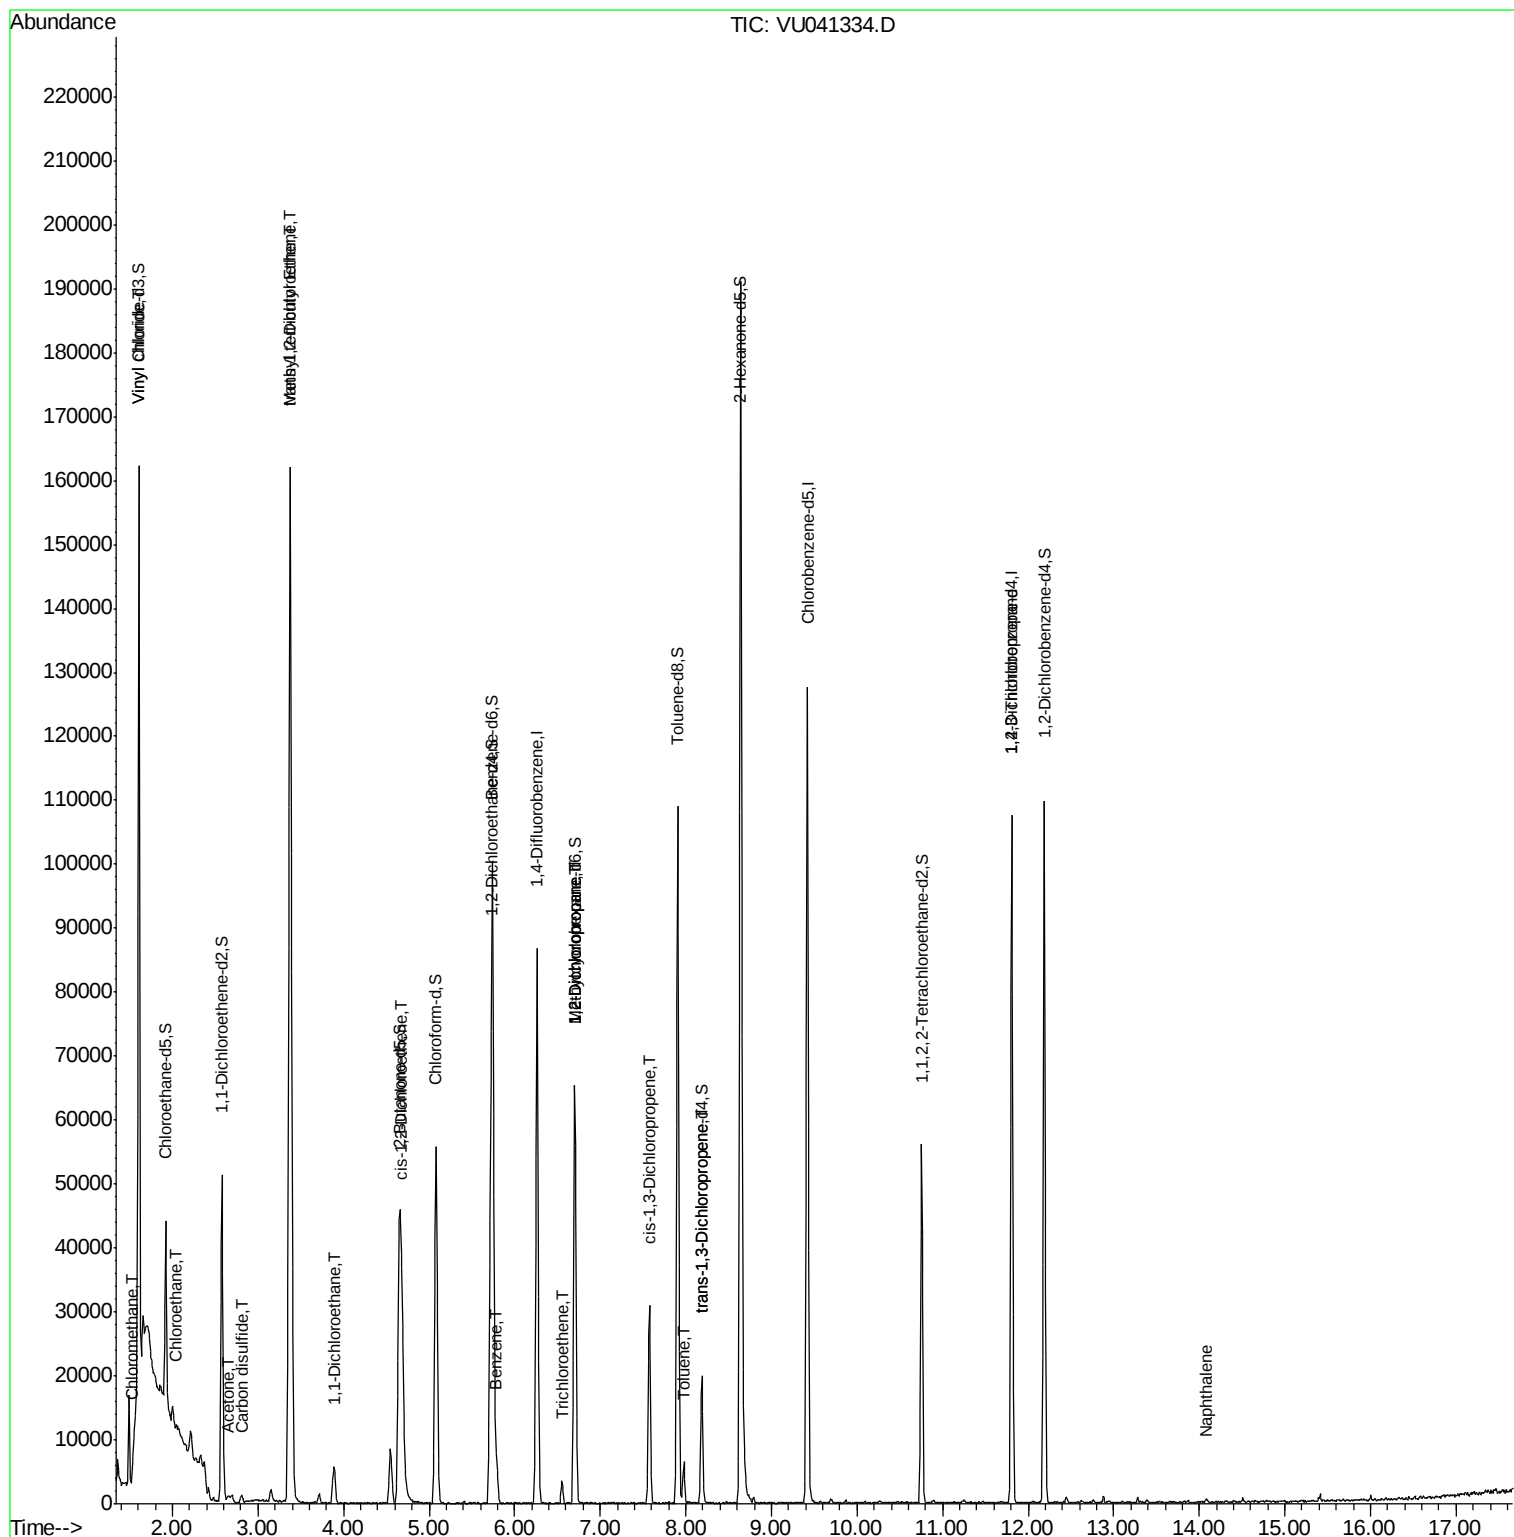

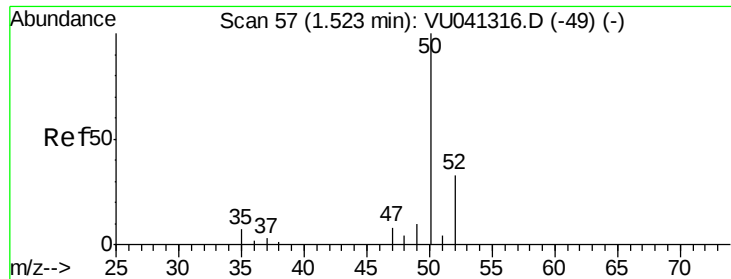

#3

Chloromethane

Concen: 0.094 ug/L

RT: 1.53 min Scan# 58

Delta R.T. 0.00 min

Lab File: VU041334.D

Acq: 19 Nov 2020 00:10


Instrument :  
MSVOA\_U  
ClientSampled :  
H4419

Tgt Ion: 50 Resp: 528




Ion Ratio Lower Upper

50 100

52 31.0 22.4 41.6

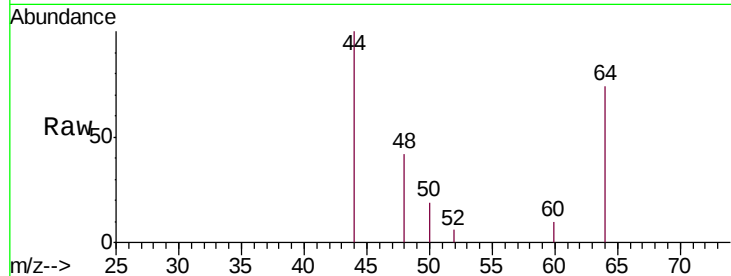

Abundance Ion 50.05 (49.75 to 50.75): VU041334.D (-1) (-)

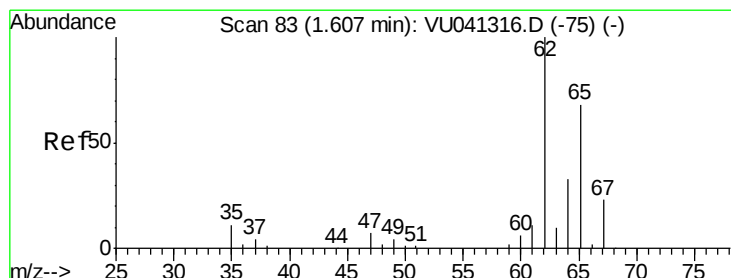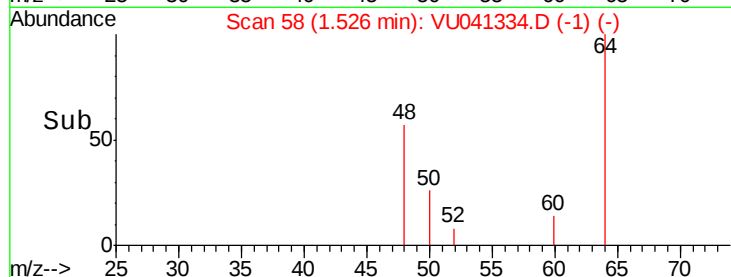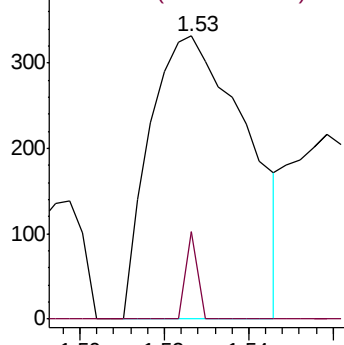

#5

Vinyl chloride

Concen: 12.623 ug/L

RT: 1.61 min Scan# 84

Delta R.T. 0.00 min

Lab File: VU041334.D


Acq: 19 Nov 2020 00:10

Tgt Ion: 62 Resp: 69419



Ion Ratio Lower Upper


62 100

64 48.1 22.7 42.3#

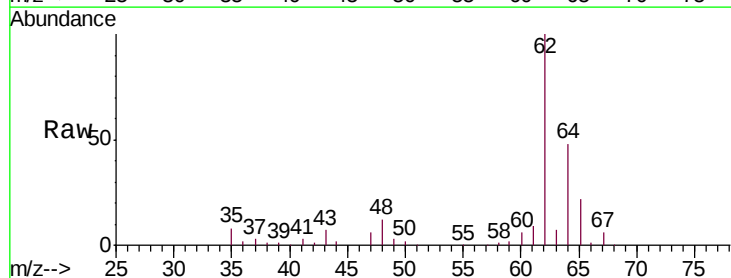

Abundance Ion 62.00 (61.70 to 62.70): VU041334.D (-1) (-)



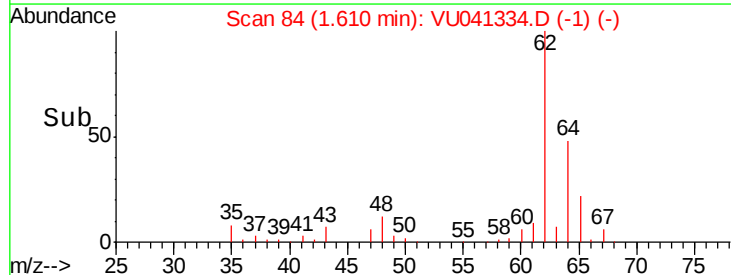
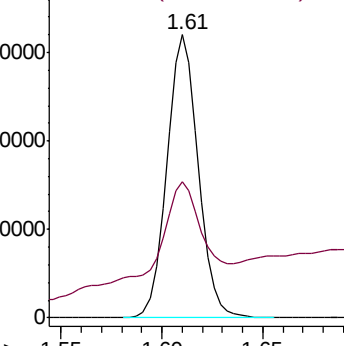


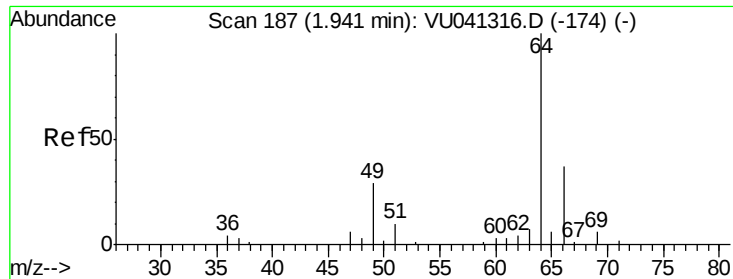

#8  
Chloroethane  
Concen: 0.237 ug/L  
RT: 2.04 min Scan# 219  
Delta R.T. 0.10 min  
Lab File: VU041334.D  
Acq: 19 Nov 2020 00:10




Instrument :  
MSVOA\_U  
ClientSampleId :  
H4419


Tgt Ion: 64 Resp: 864  
Ion Ratio Lower Upper  
64 100  
66 4.6 22.3 41.5#

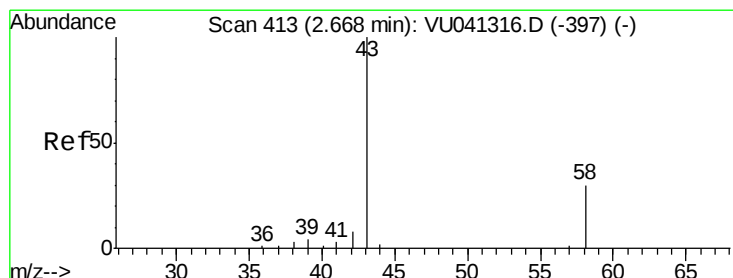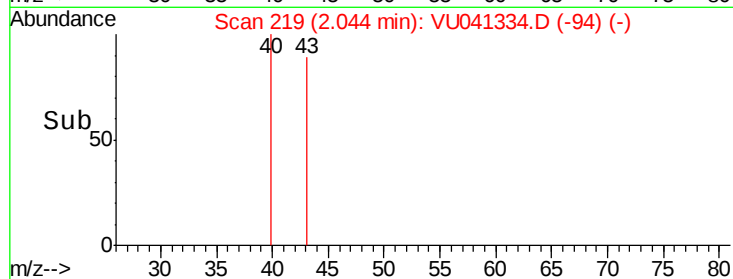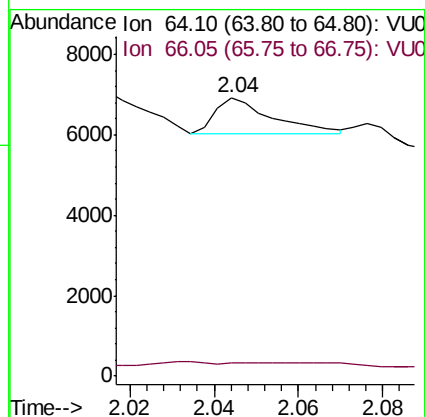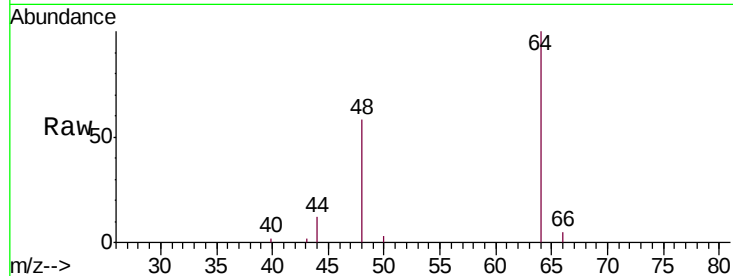

#13  
Acetone  
Concen: 1.524 ug/L  
RT: 2.66 min Scan# 411  
Delta R.T. -0.01 min  
Lab File: VU041334.D  
Acq: 19 Nov 2020 00:10

Tgt Ion: 43 Resp: 1943  
Ion Ratio Lower Upper  
43 100  
58 9.2 0.0 25.4

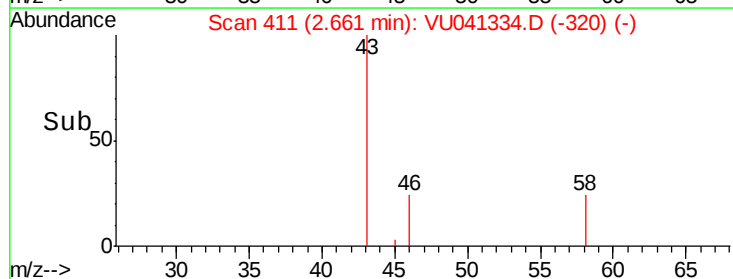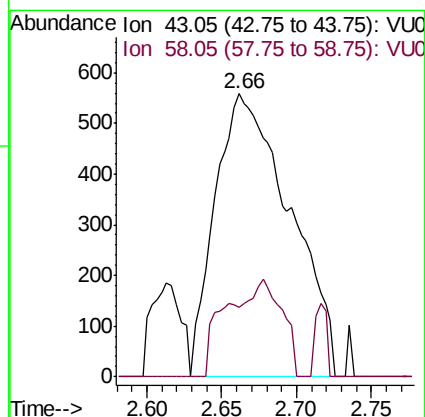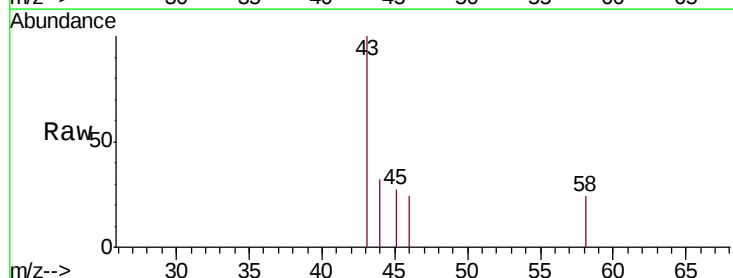

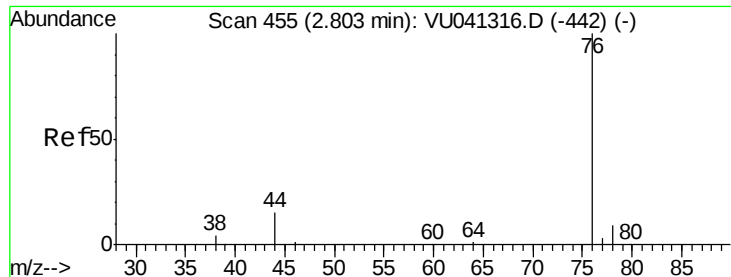

#14

Carbon disulfide

Concen: 0.148 ug/L

RT: 2.81 min Scan# 456

Delta R.T. 0.00 min

Lab File: VU041334.D

Acq: 19 Nov 2020 00:10

Instrument :

MSVOA\_U

ClientSampleId :


H4419

Tgt Ion: 76 Resp: 1795

Ion Ratio Lower Upper

76 100

78 0.0 7.5 11.3#

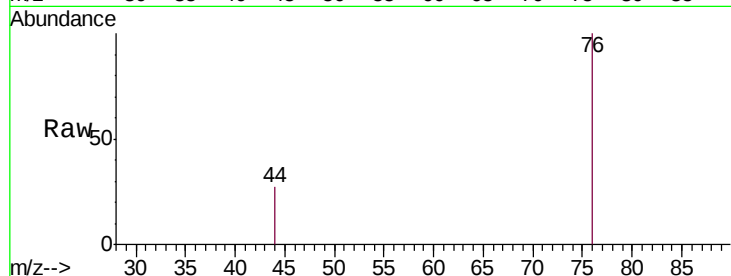

Abundance Ion 76.05 (75.75 to 76.75): VU041334.D (-442) (-)

Ion 78.00 (77.70 to 78.70): VU041334.D (-442) (-)

2.81

1200

1000

800

600

400



200

0

Time-->

2.80

2.85

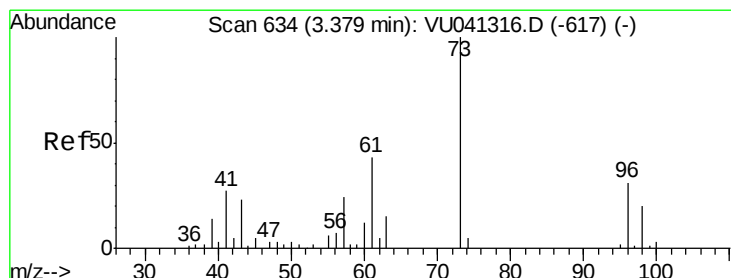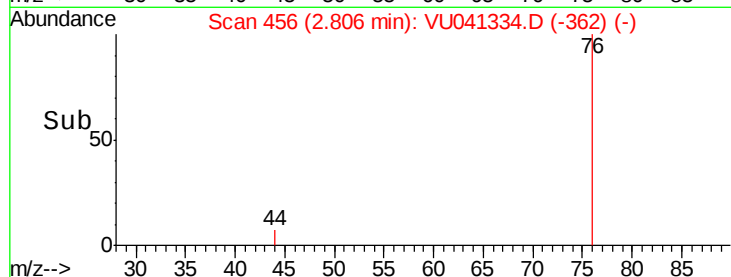

#17

Methyl tert-butyl Ether

Concen: 10.633 ug/L

RT: 3.38 min Scan# 634

Delta R.T. -0.00 min

Lab File: VU041334.D

Acq: 19 Nov 2020 00:10


Tgt Ion: 73 Resp: 120034

Ion Ratio Lower Upper

73 100

43 22.9 18.5 27.7

57 23.2 18.4 27.6

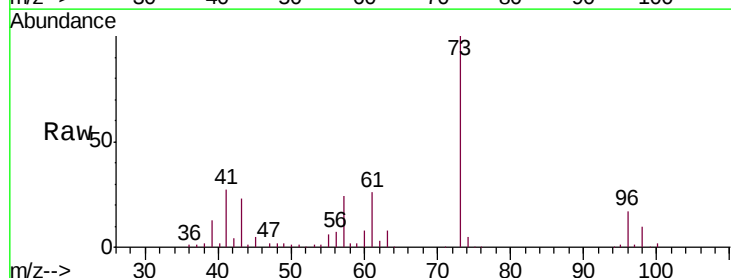

Abundance Ion 73.10 (72.80 to 73.80): VU041334.D (-617) (-)

Ion 43.05 (42.75 to 43.75): VU041334.D (-617) (-)

Ion 57.10 (56.80 to 57.80): VU041334.D (-617) (-)

3.38

60000

40000

20000


0


Time-->

3.30

3.40

3.50

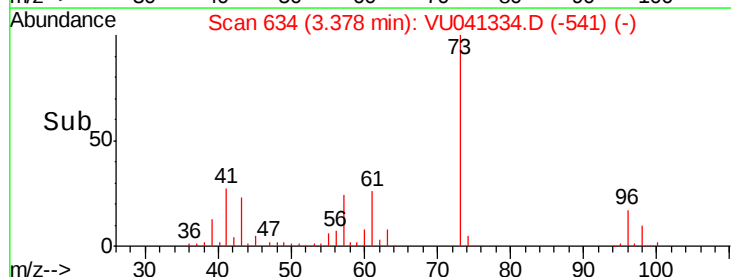

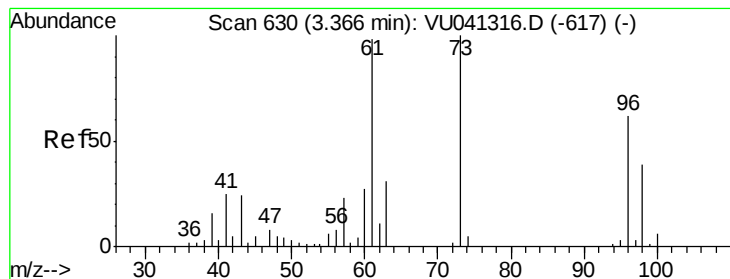

#18

trans-1,2-Dichloroethene

Concen: 5.407 ug/L

RT: 3.37 min Scan# 632

Delta R.T. 0.01 min

Lab File: VU041334.D

Acq: 19 Nov 2020 00:10

Instrument :

MSVOA\_U

ClientSampleId :

H4419


Tgt Ion: 96 Resp: 21716

Ion Ratio Lower Upper

96 100

61 153.1 110.9 205.9




98 61.5 45.4 84.2

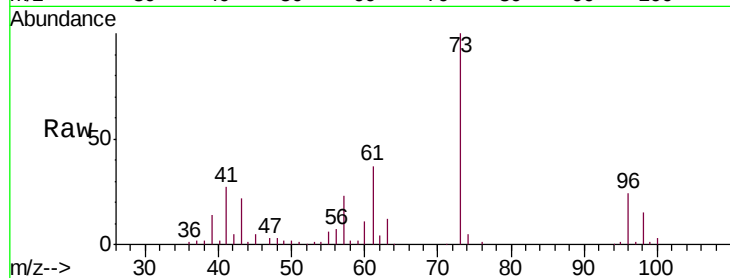

Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 61.05 (60.75 to 61.75): VU0

Ion 97.95 (97.65 to 98.65): VU0

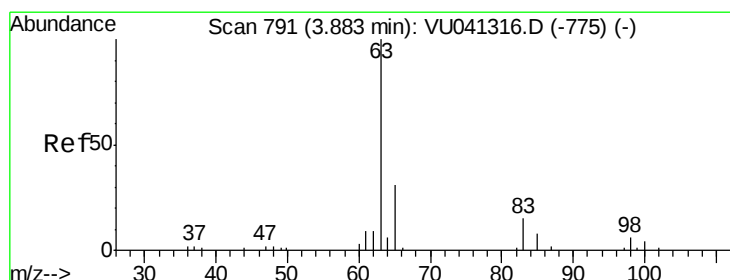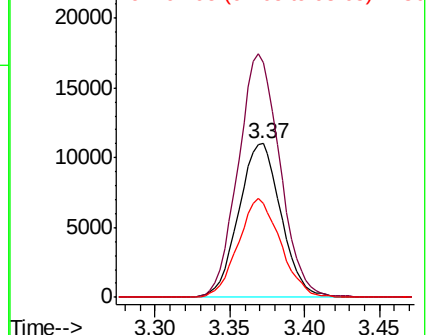

#19

1,1-Dichloroethane

Concen: 0.787 ug/L

RT: 3.89 min Scan# 792

Delta R.T. 0.00 min

Lab File: VU041334.D

Acq: 19 Nov 2020 00:10


Tgt Ion: 63 Resp: 7065

Ion Ratio Lower Upper

63 100

65 32.5 21.3 39.6



83 13.2 8.8 16.3

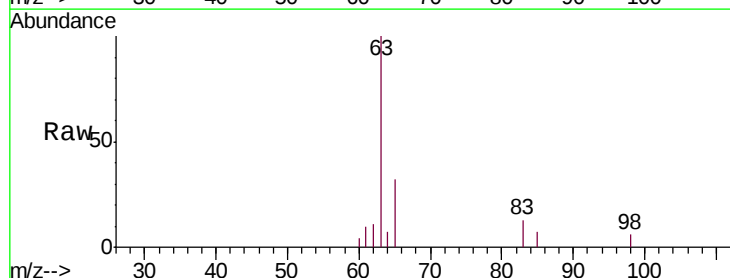


Abundance Ion 63.10 (62.80 to 63.80): VU0

Ion 65.10 (64.80 to 65.80): VU0

Ion 83.05 (82.75 to 83.75): VU0

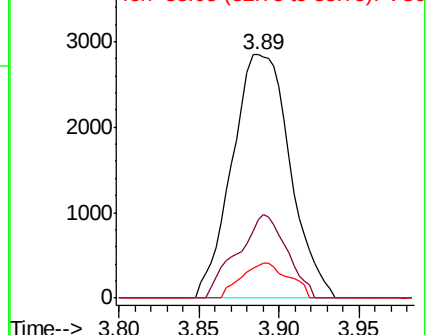


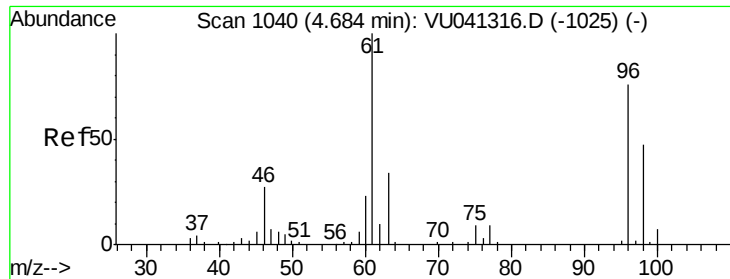




#22  
 cis-1,2-Dichloroethene  
 Concen: 1.397 ug/L  
 RT: 4.68 min Scan# 1040  
 Delta R.T. -0.00 min  
 Lab File: VU041334.D  
 Acq: 19 Nov 2020 00:10

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 H4419

Tgt Ion: 96 Resp: 6338  
 Ion Ratio Lower Upper  
 96 100  
 61 123.5 97.2 180.4  
 68 0.0 0.0 0.0

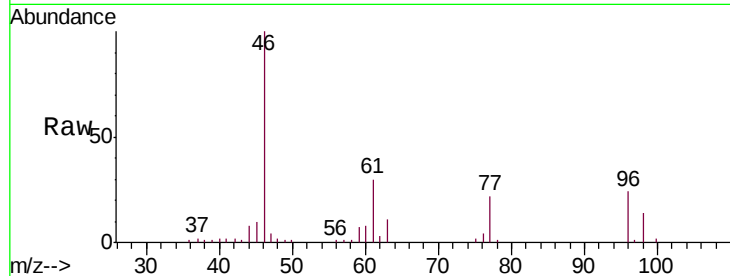


Abundance Ion 96.00 (95.70 to 96.70): VU0  
 Ion 61.05 (60.75 to 61.75): VU0  
 Ion 68.15 (67.85 to 68.85): VU0

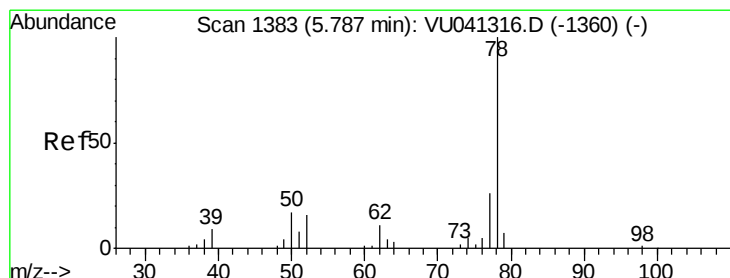
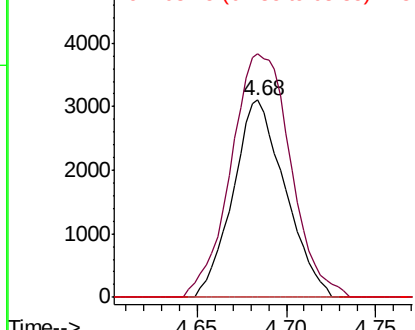



#33  
 Benzene  
 Concen: 0.374 ug/L  
 RT: 5.79 min Scan# 1385  
 Delta R.T. 0.01 min  
 Lab File: VU041334.D  
 Acq: 19 Nov 2020 00:10

Tgt Ion: 78 Resp: 6668

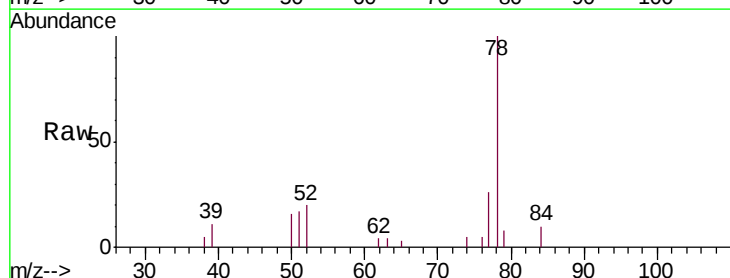

Abundance Ion 78.10 (77.80 to 78.80): VU0

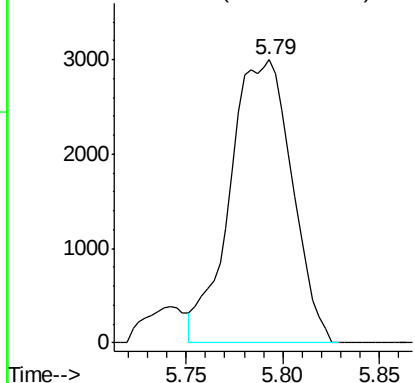



#34

Trichloroethene

Concen: 0.275 ug/L

RT: 6.55 min Scan# 1620

Delta R.T. -0.00 min

Lab File: VU041334.D

Acq: 19 Nov 2020 00:10

Instrument :

MSVOA\_U

ClientSampleId :

H4419

Tgt Ion: 95 Resp: 1328



Ion Ratio Lower Upper

95 100

97 51.9 45.6 84.6

132 58.0 64.8 120.4#

130 78.4 64.8 120.4


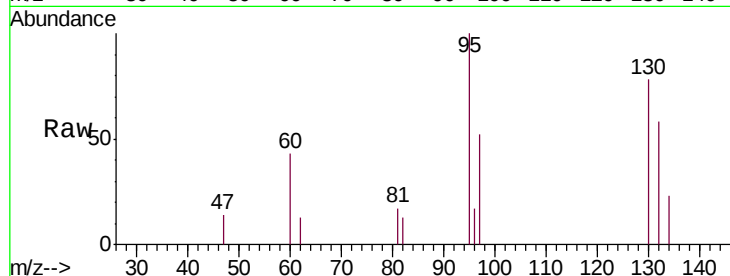


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

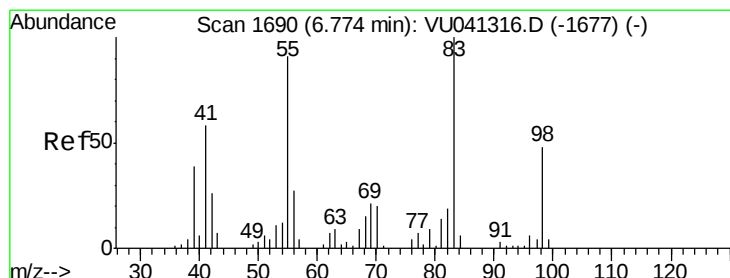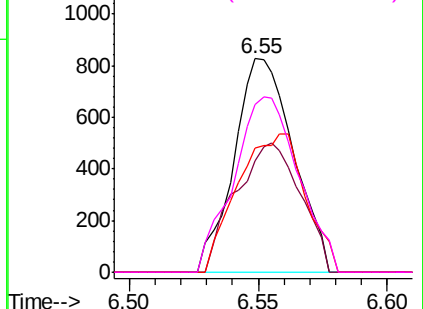

#35

Methylcyclohexane

Concen: 1.084 ug/L

RT: 6.70 min Scan# 1667

Delta R.T. -0.07 min

Lab File: VU041334.D

Acq: 19 Nov 2020 00:10



Tgt Ion: 83 Resp: 6946

Ion Ratio Lower Upper

83 100

55 0.0 72.0 108.0#


98 0.0 36.6 55.0#

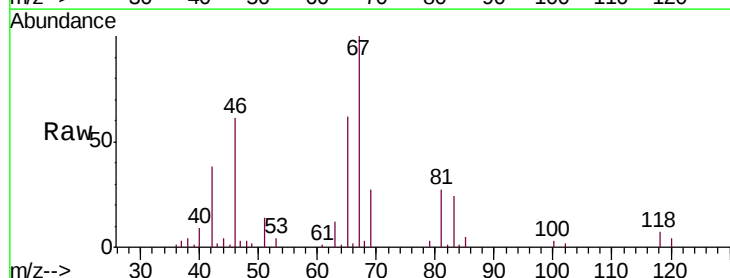


Abundance Ion 83.15 (82.85 to 83.85): VU0

Ion 55.10 (54.80 to 55.80): VU0

Ion 98.15 (97.85 to 98.85): VU0




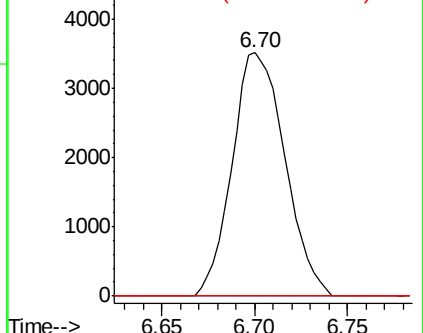


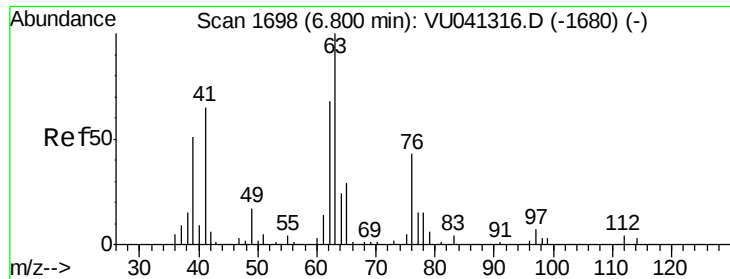

#37  
 1,2-Dichloropropane  
 Concen: 0.662 ug/L  
 RT: 6.70 min Scan# 1668  
 Delta R.T. -0.10 min  
 Lab File: VU041334.D  
 Acq: 19 Nov 2020 00:10




Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 H4419


Tgt Ion: 63 Resp: 3454  
 Ion Ratio Lower Upper  
 63 100  
 112 0.0 3.6 5.4#

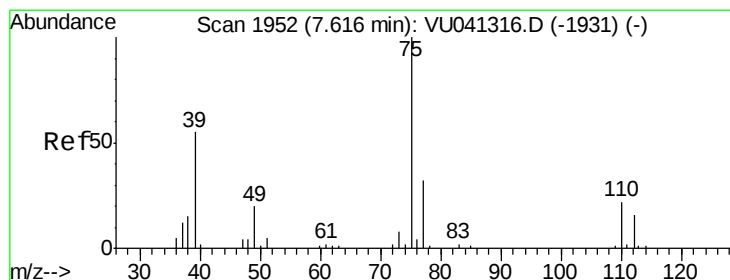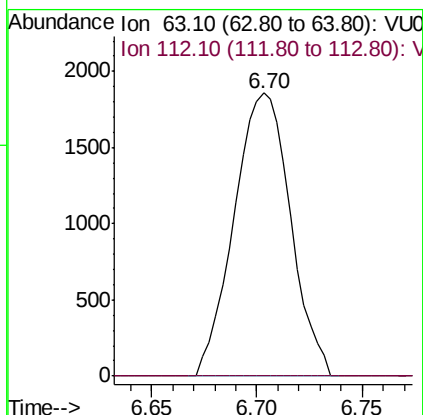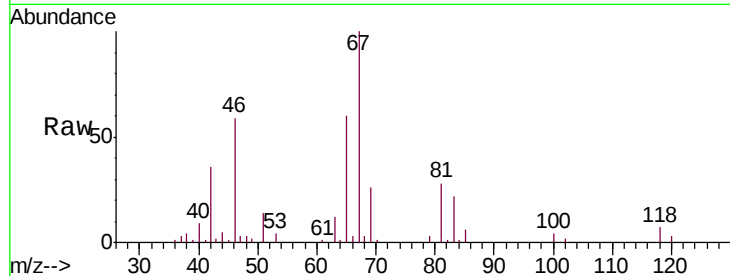

#39  
 cis-1,3-Dichloropropene  
 Concen: 0.119 ug/L  
 RT: 7.57 min Scan# 1938  
 Delta R.T. -0.05 min  
 Lab File: VU041334.D  
 Acq: 19 Nov 2020 00:10

Tgt Ion: 75 Resp: 865  
 Ion Ratio Lower Upper  
 75 100  
 77 43.1 22.7 42.3#

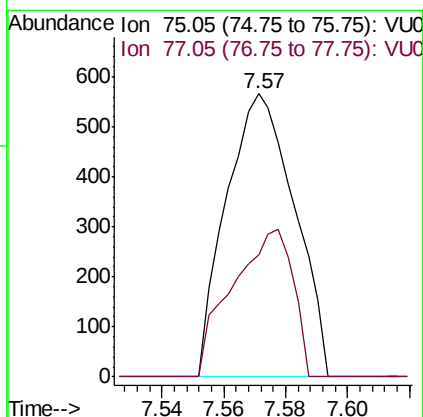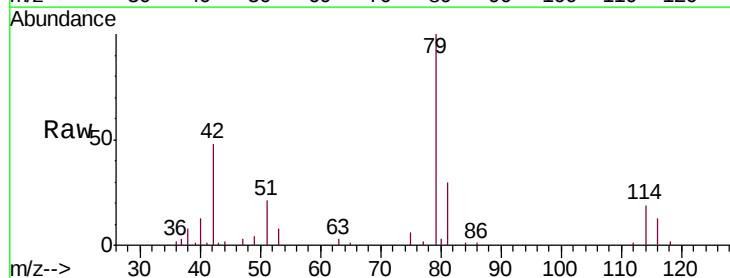

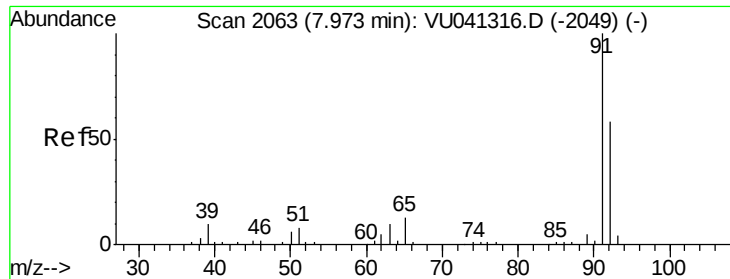

#42

Toluene

Concen: 0.236 ug/L

RT: 7.98 min Scan# 2064

Delta R.T. 0.00 min

Lab File: VU041334.D

Acq: 19 Nov 2020 00:10

Instrument :

MSVOA\_U

ClientSampleId :


H4419

Tgt Ion: 91 Resp: 4501

Ion Ratio Lower Upper




91 100

92 69.2 40.6 75.4

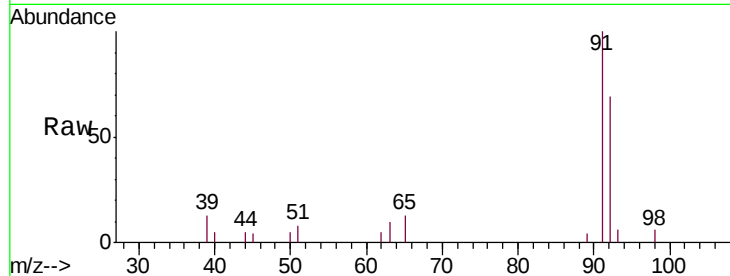

Abundance Ion 91.15 (90.85 to 91.85): VU041316.D (-2049) (-)

Ion 92.15 (91.85 to 92.85): VU041316.D (-2049) (-)

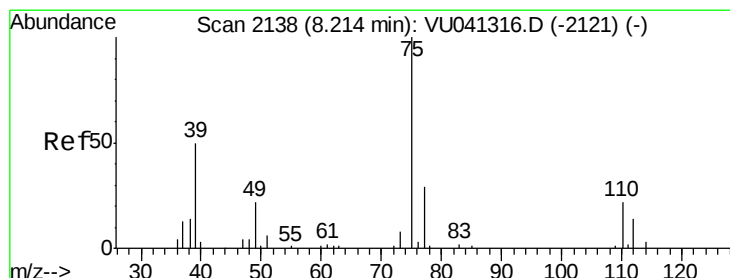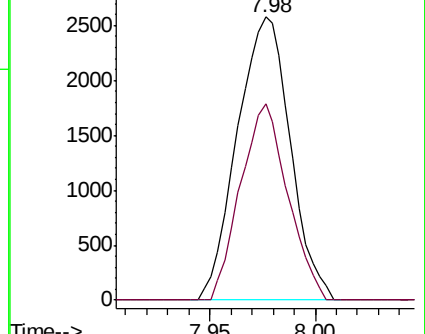

#44

trans-1,3-Dichloropropene

Concen: 0.063 ug/L

RT: 8.19 min Scan# 2130

Delta R.T. -0.03 min

Lab File: VU041334.D


Acq: 19 Nov 2020 00:10

Tgt Ion: 75 Resp: 433

Ion Ratio Lower Upper



75 100


77 65.5 23.3 43.3#

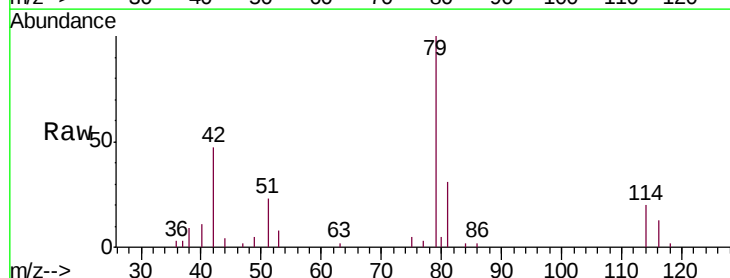

Abundance Ion 75.05 (74.75 to 75.75): VU041316.D (-2121) (-)

Ion 77.05 (76.75 to 77.75): VU041316.D (-2121) (-)




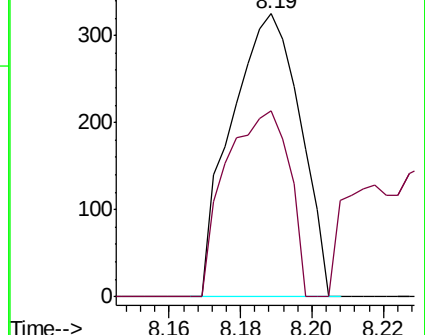


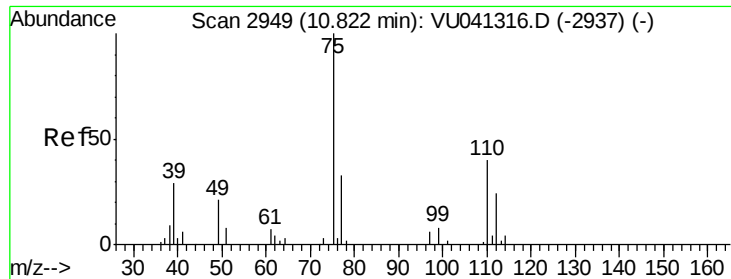

#59  
 1,2,3-Trichloropropane  
 Concen: 0.823 ug/L  
 RT: 11.81 min Scan# 3256  
 Delta R.T. 0.99 min  
 Lab File: VU041334.D  
 Acq: 19 Nov 2020 00:10

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 H4419

Tgt Ion: 75 Resp: 3387  
 Ion Ratio Lower Upper  
 75 100  
 77 37.3 25.7 38.5

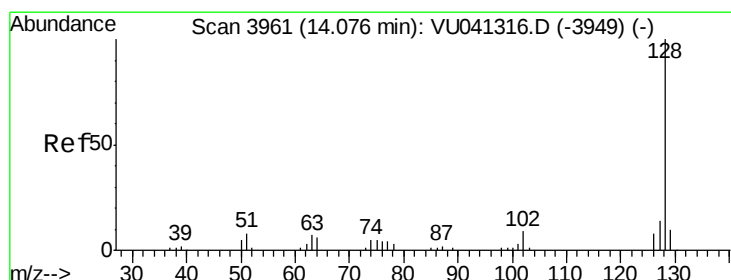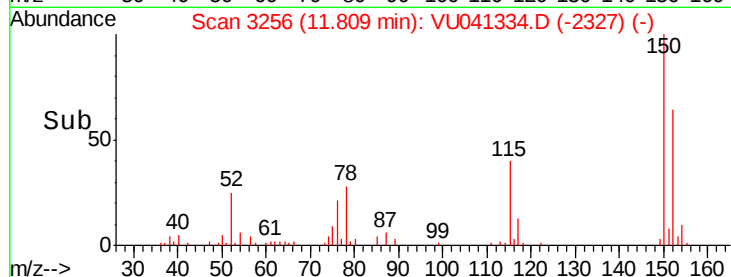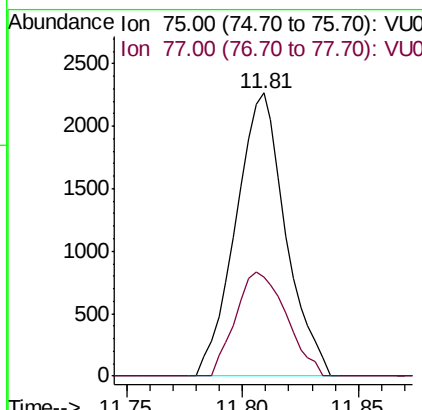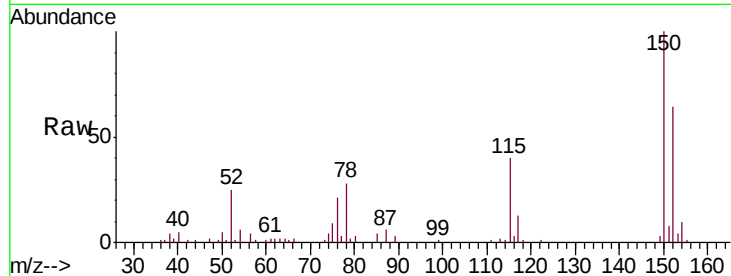

#69  
 Naphthalene  
 Concen: 0.088 ug/L  
 RT: 14.08 min Scan# 3961  
 Delta R.T. -0.00 min  
 Lab File: VU041334.D  
 Acq: 19 Nov 2020 00:10

Tgt Ion: 128 Resp: 683  
 Ion Ratio Lower Upper  
 128 100  
 129 11.6 8.7 13.1  
 127 0.0 10.8 16.2#

