

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU111920\
Quantitation Report (QT Reviewed)


Data File : VU041324.D
Acq On : 18 Nov 2020 20:13
Operator : SY/MD
Sample : L4790-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4420

Manual Integrations
APPROVED

MMDadoda
11/20/2020 2:21:16 PM

Quant Time: Nov 19 01:27:57 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Nov 19 00:50:13 2020
Response via : Initial Calibration

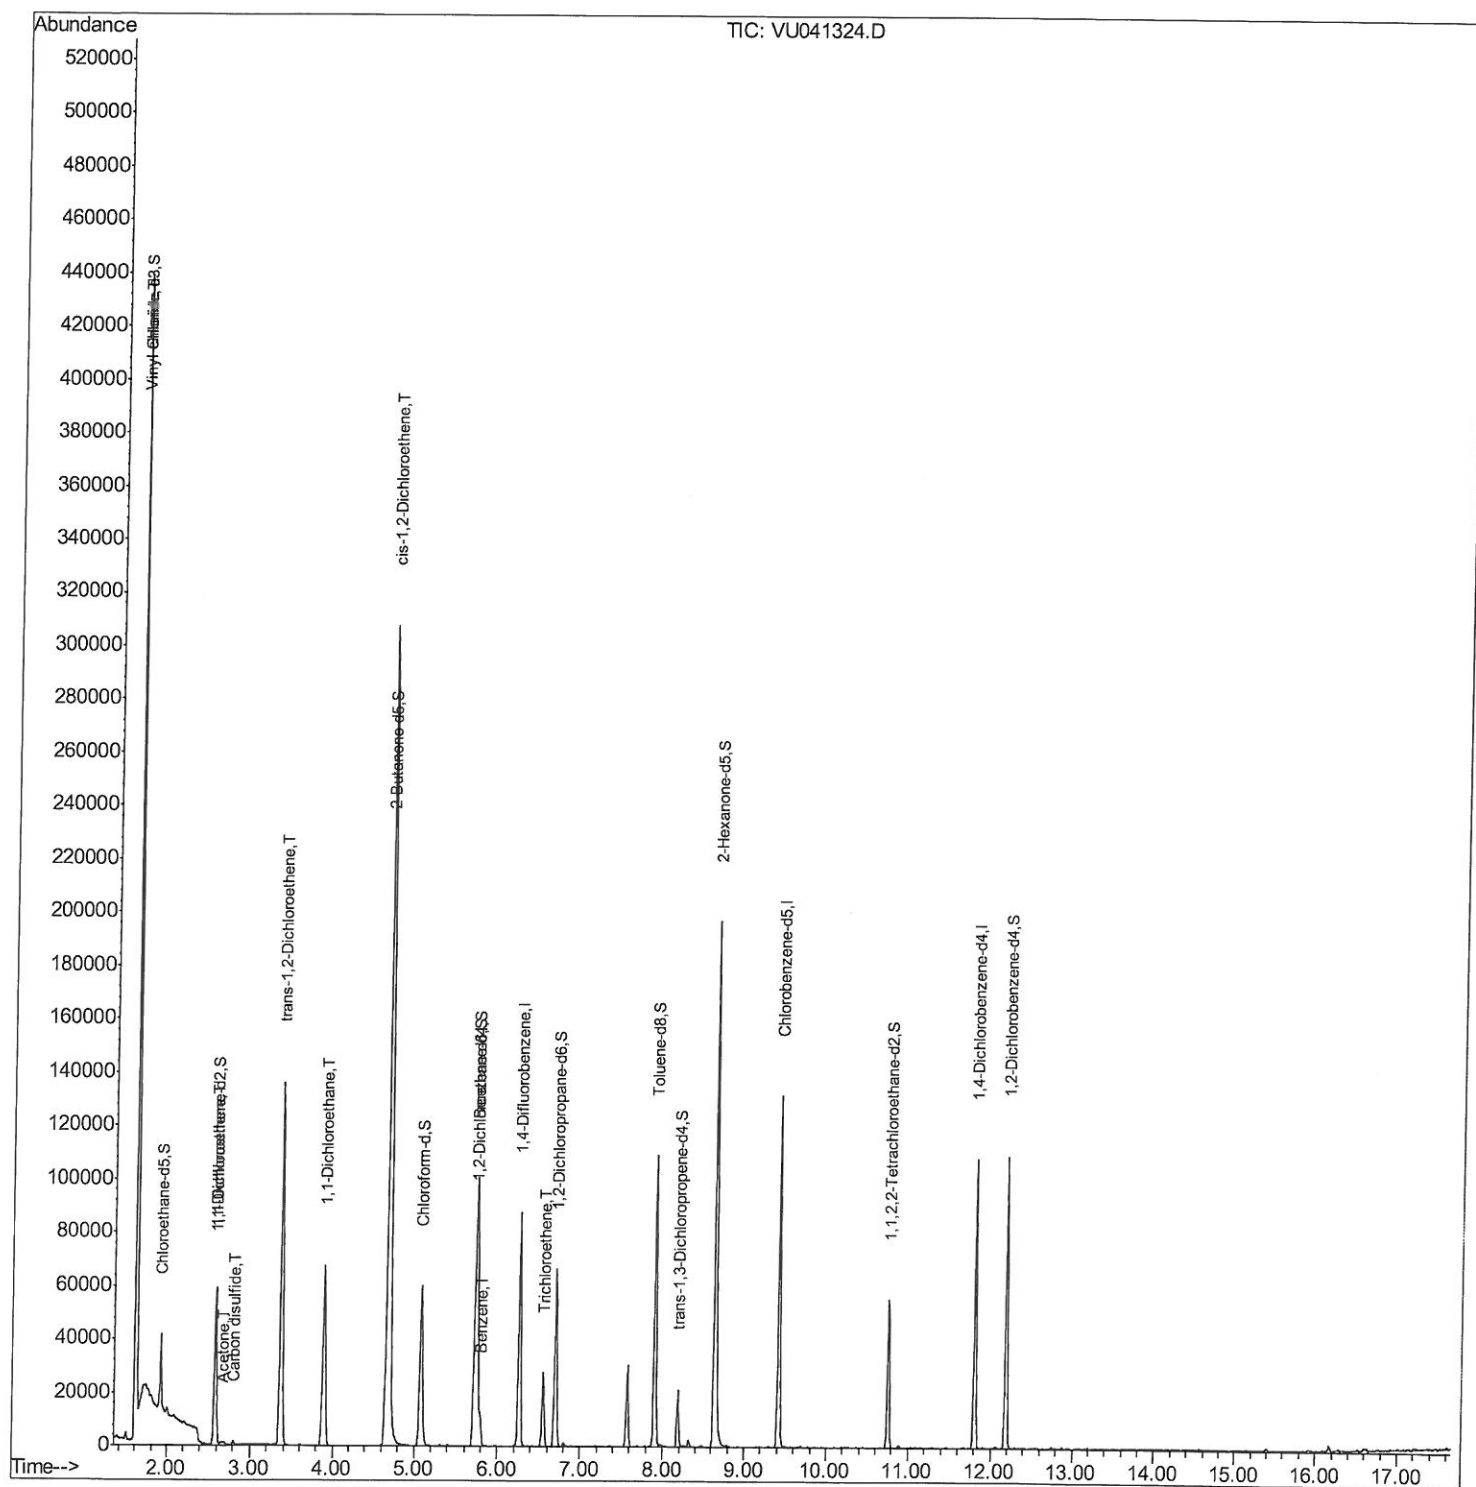

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU111920\
Quantitation Report (Qedit)




Data File : VU041324.D
Acq On : 18 Nov 2020 20:13
Operator : SY/MD
Sample : L4790-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4420

Manual Integrations
APPROVED

MMDadoda
11/20/2020 2:21:16 PM

Quant Time: Nov 19 00:52:42 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Nov 19 00:50:13 2020
Response via : Initial Calibration

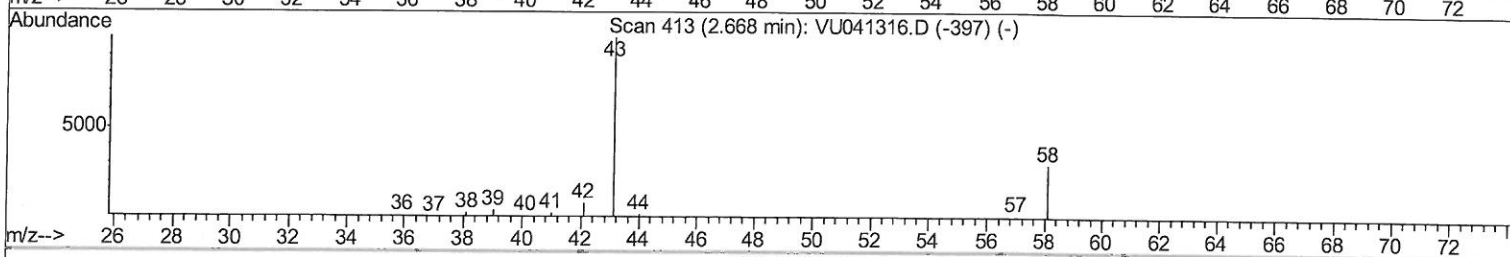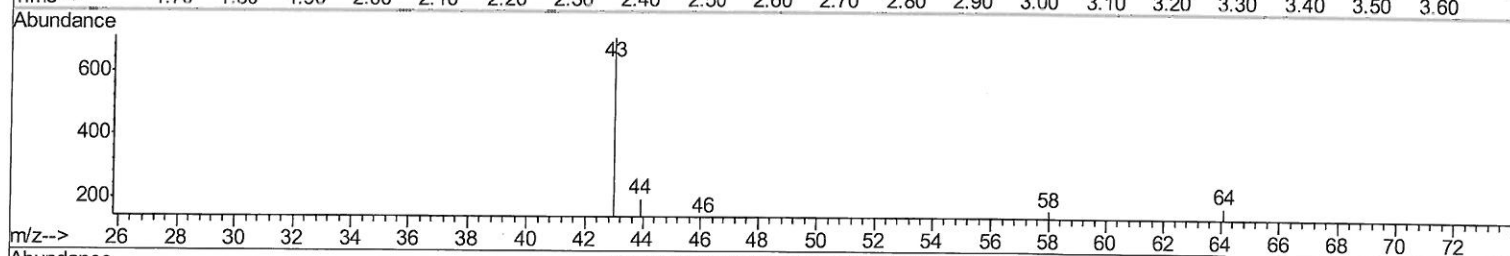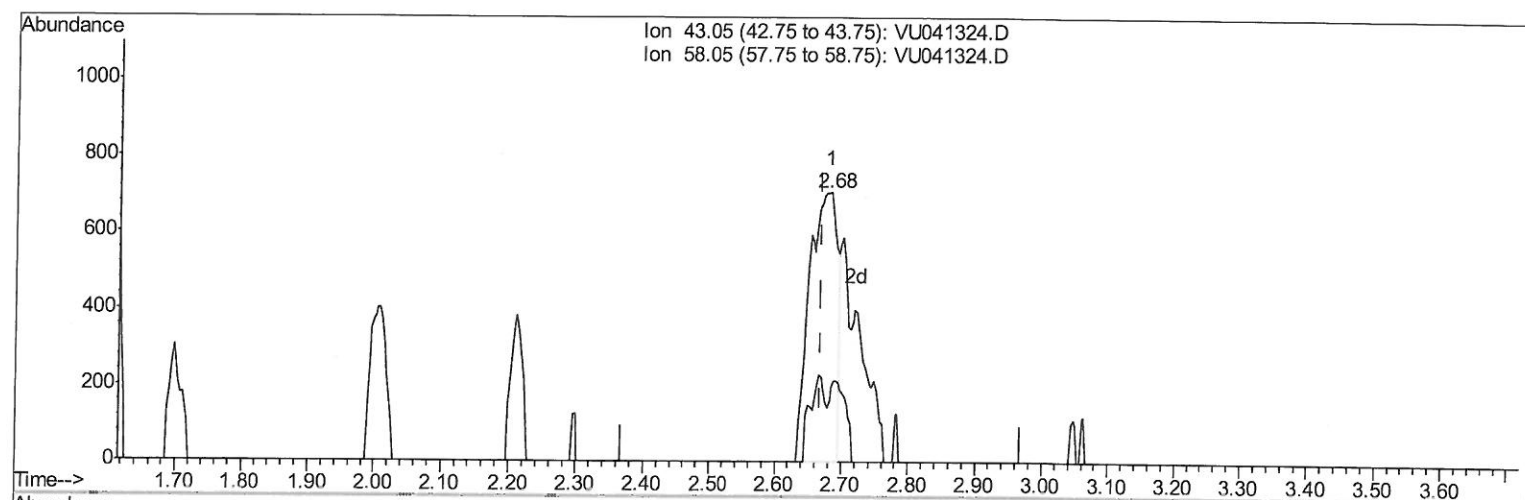

TIC: VU041324.D

(13) Acetone (T)

2.681min (+0.013) 1.51ug/L

response 2001

Ion	Exp%	Act%
43.05	100	100
58.05	12.70	18.29
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU111920\
Data File : VU041324.D
Acq On : 18 Nov 2020 20:13
Operator : SY/MD
Sample : L4790-08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4420

Manual Integrations
APPROVED

MMDadoda
11/20/2020 2:21:16 PM

Quant Time: Nov 19 01:27:57 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Nov 19 00:50:13 2020
Response via : Initial Calibration

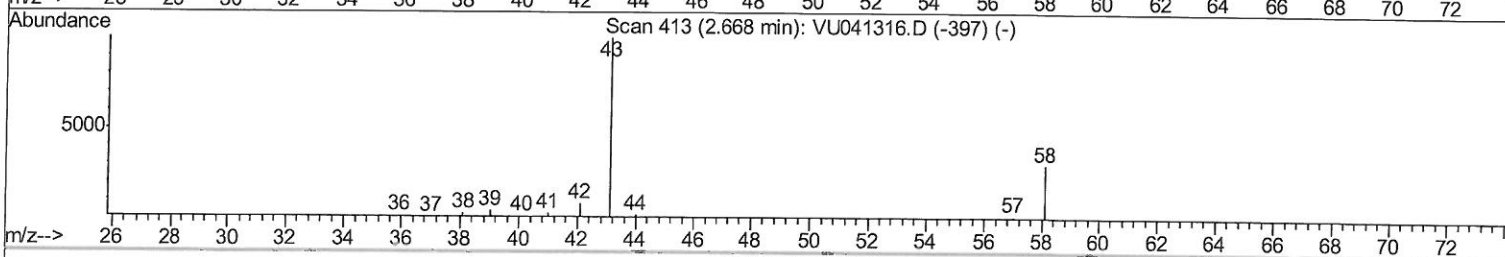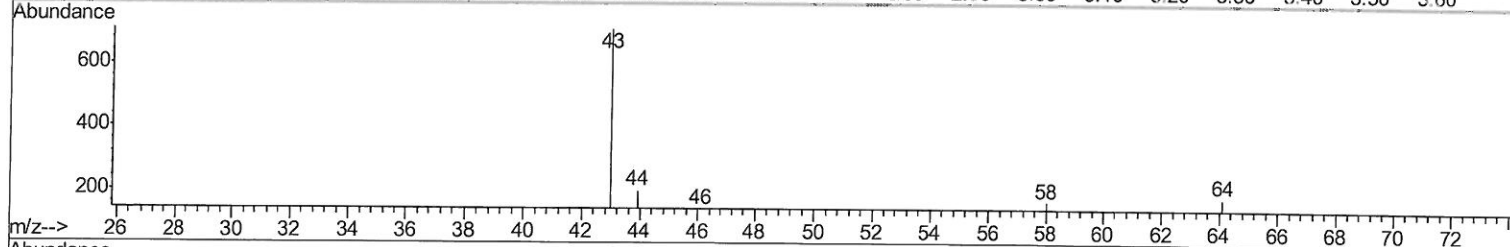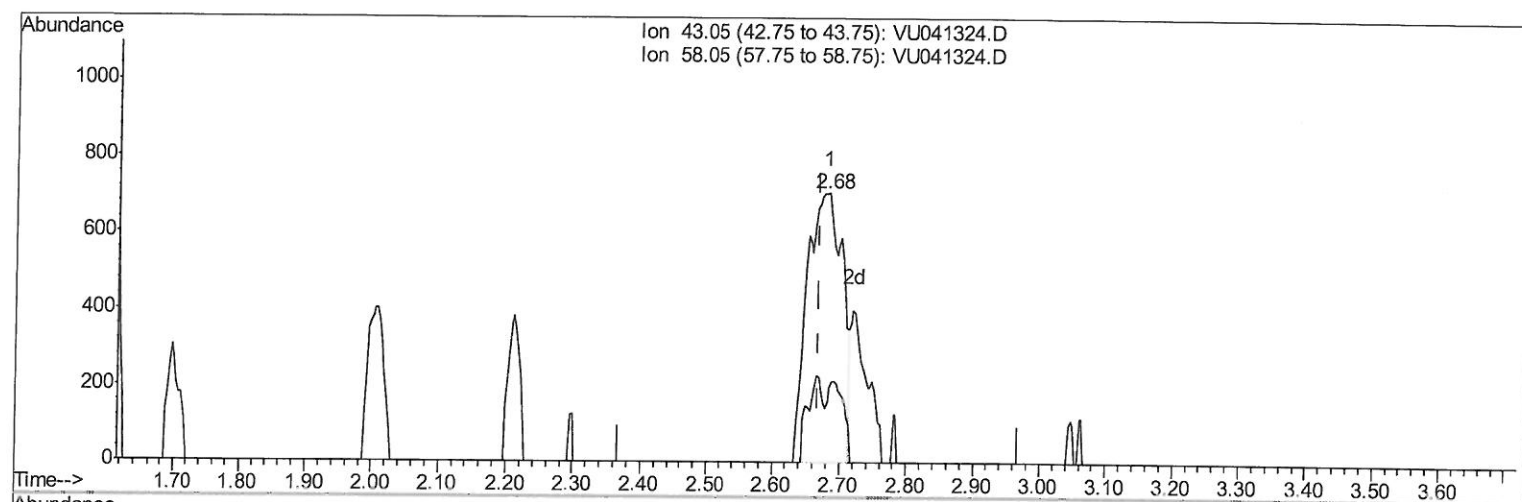

TIC: VU041324.D

(13) Acetone (T)

2.681min (+0.013) 1.92ug/L m

response 2541

MD
12/01/20

Ion	Exp%	Act%
43.05	100	100
58.05	12.70	14.40
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU111920\
Quantitation Report (Qedit)


Data File : VU041324.D
Acq On : 18 Nov 2020 20:13
Operator : SY/MD
Sample : L4790-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4420

Manual Integrations
APPROVED

MMDadoda
11/20/2020 2:21:16 PM

Quant Time: Nov 19 00:52:42 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Nov 19 00:50:13 2020
Response via : Initial Calibration

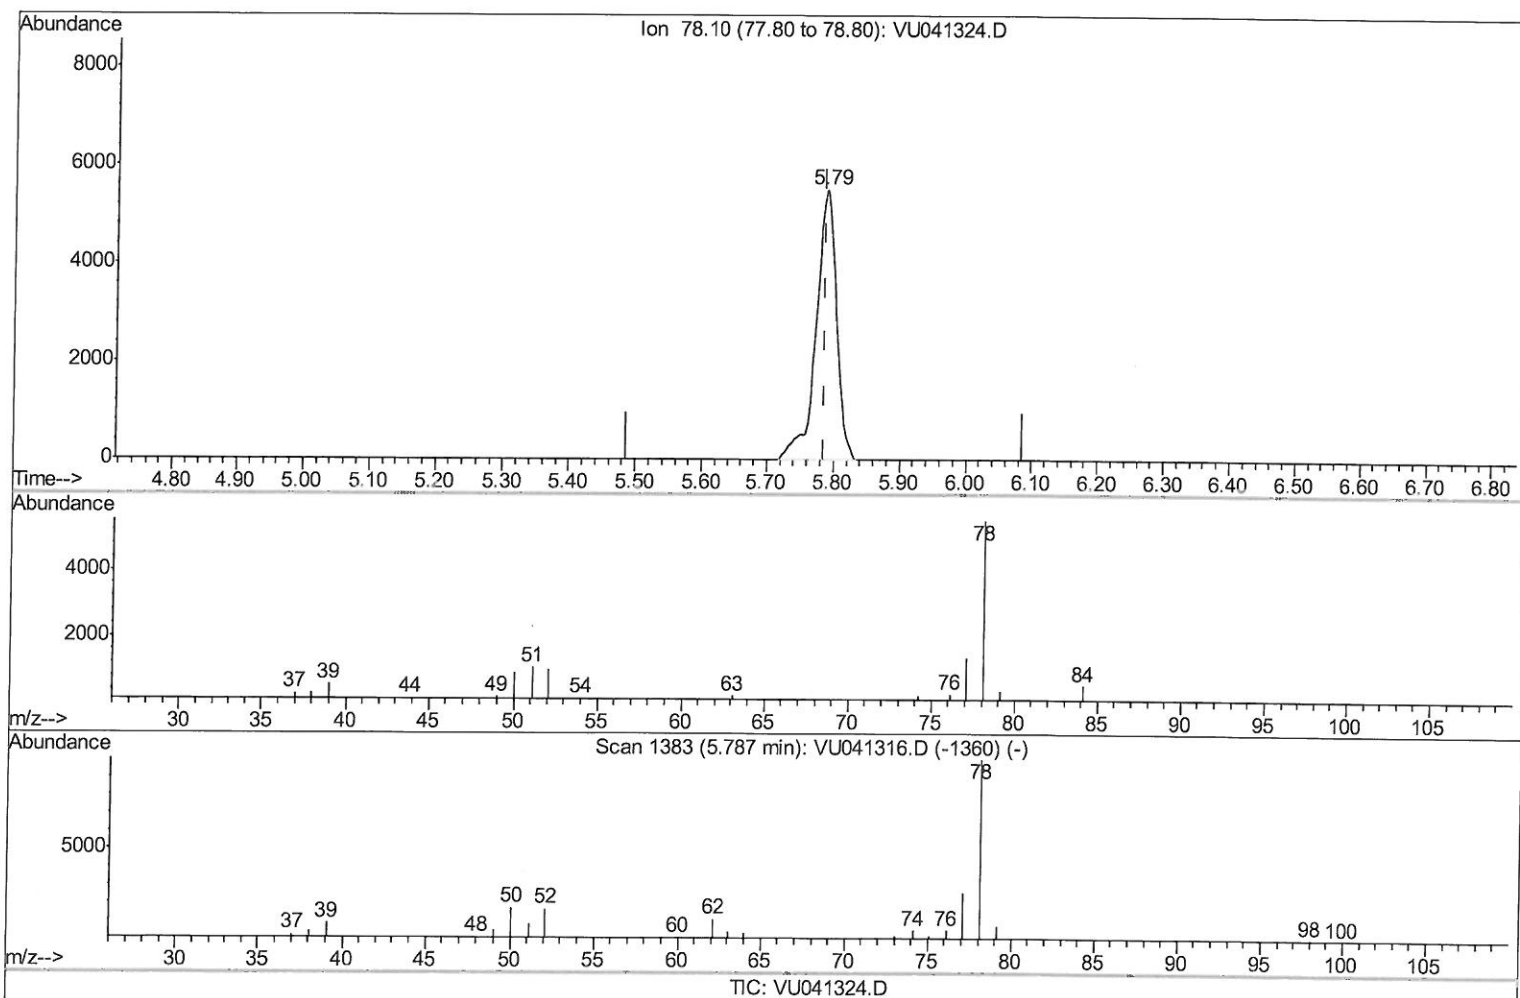

(33) Benzene (T)

5.787min (0.000) 0.67ug/L

response 11805

Ion	Exp%	Act%
78.10	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU111920\
Quantitation Report (Qedit)




Data File : VU041324.D
Acq On : 18 Nov 2020 20:13
Operator : SY/MD
Sample : L4790-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4420

Manual Integrations
APPROVED

MMDadoda
11/20/2020 2:21:16 PM

Quant Time: Nov 19 00:52:42 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Nov 19 00:50:13 2020
Response via : Initial Calibration

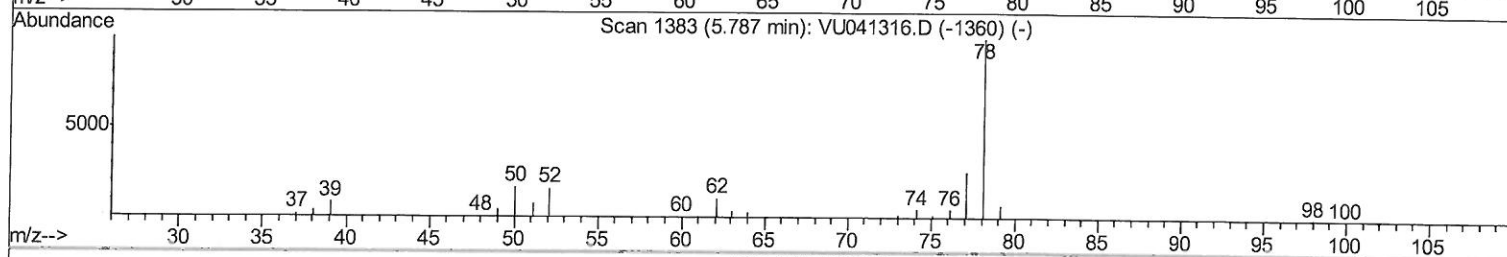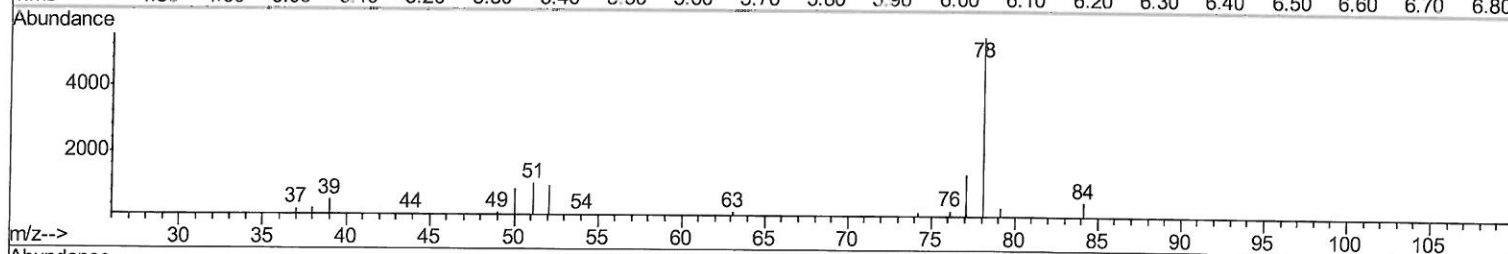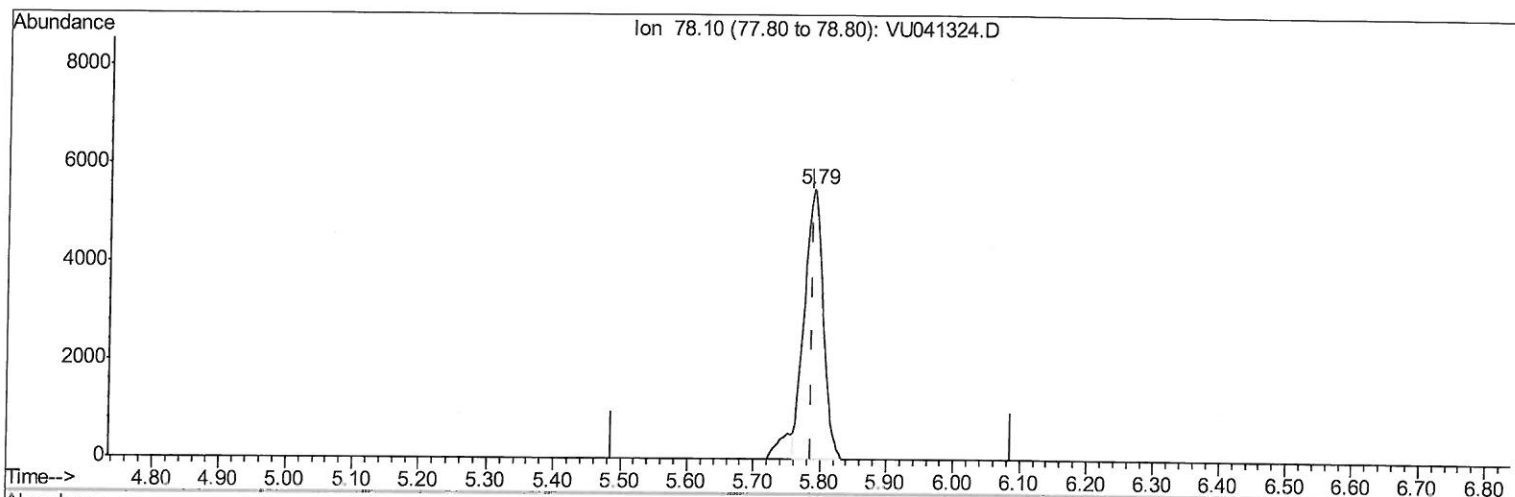

TIC: VU041324.D

(33) Benzene (T)

5.787min (0.000) 0.62ug/L m

response 10962

Ion	Exp%	Act%
78.10	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

7 mg
12/01/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU111920\

Quantitation Report (QT Reviewed)

Data File : VU041324.D

Acq On : 18 Nov 2020 20:13

Operator : SY/MD

Sample : L4790-08

Misc : 25.0mL/MSVOA_U/WATER

ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4420Manual Integrations
APPROVEDMMDadoda
11/20/2020 2:21:16 PM

Quant Time: Nov 19 01:27:57 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Thu Nov 19 00:50:13 2020

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	65650	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	65097	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	26292	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	22713	4.70	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	94.00%		
7) Chloroethane-d5	1.92	69	18657	4.52	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	90.40%		
11) 1,1-Dichloroethene-d2	2.58	63	35707	3.58	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	71.60%		
20) 2-Butanone-d5	4.66	46	94984	47.70	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	95.40%		
24) Chloroform-d	5.08	84	49962	4.78	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	95.60%		
26) 1,2-Dichloroethane-d4	5.72	65	30928	4.54	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	90.80%		
32) Benzene-d6	5.74	84	85759	4.89	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	97.80%		
36) 1,2-Dichloropropane-d6	6.70	67	29436	4.87	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	97.40%		
41) Toluene-d8	7.91	98	67715	4.10	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	82.00%		
43) trans-1,3-Dichloropropene-	8.19	79	11605	4.46	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	89.20%		
46) 2-Hexanone-d5	8.64	63	64656	46.51	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	93.02%		
57) 1,1,2,2-Tetrachloroethane-	10.75	84	26832	4.57	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	91.40%		
64) 1,2-Dichlorobenzene-d4	12.19	152	26288	5.12	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	102.40%		

Target Compounds

					Qvalue	
5) Vinyl chloride	1.61	62	266069	46.685	ug/L	99
12) 1,1-Dichloroethene	2.59	96	2950	0.690	ug/L #	1
13) Acetone	2.68	43	2541m	1.924	ug/L	
14) Carbon disulfide	2.81	76	1918	0.153	ug/L #	94
18) trans-1,2-Dichloroethene	3.37	96	53601	12.878	ug/L	99
19) 1,1-Dichloroethane	3.89	63	76988	8.273	ug/L	97
22) cis-1,2-Dichloroethene	4.68	96	138268	29.415	ug/L	96
33) Benzene	5.79	78	10962m	0.621	ug/L	
34) Trichloroethene	6.55	95	9133	1.916	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

MD
12/01/20