


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU111920\
 Data File : VU041338.D
 Acq On : 19 Nov 2020 09:14
 Operator : SY/MD
 Sample : BFB15
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB15

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR111620WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Dec 07 07:51:32 2020

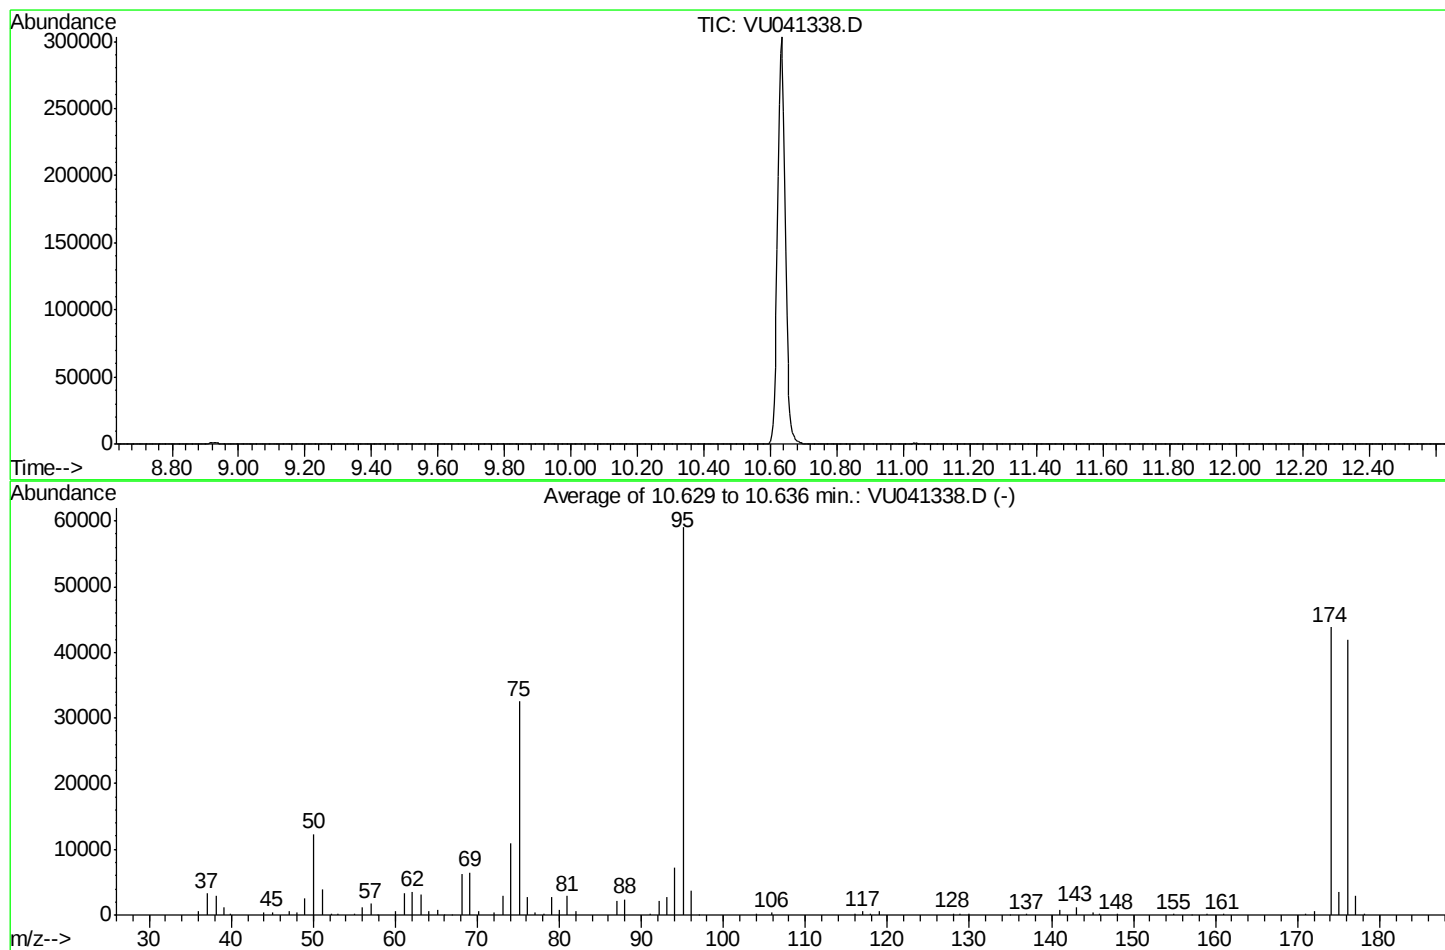

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	12288	PASS
75	95	30	80	55.0	32482	PASS
95	95	100	100	100.0	59037	PASS
96	95	5	9	6.3	3733	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.2	43826	PASS
175	174	5	9	8.0	3493	PASS
176	174	95	101	95.6	41909	PASS
177	176	5	9	6.9	2872	PASS

m/z	Abundance
44.00	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

m/z	Abundance
36.00	533.0
37.00	3282.0
38.10	3049.0
39.10	1279.0
40.00	141.0
44.10	486.0
45.00	469.0
47.10	602.0
47.90	472.0
49.00	2713.0
50.10	12104.0
51.10	3884.0
52.10	154.0
53.00	117.0
55.00	165.0
56.00	1118.0
57.00	1730.0
57.90	107.0
60.00	598.0
61.00	3299.0
62.10	3652.0
63.10	3296.0
64.10	694.0
65.10	681.0
66.00	118.0
66.90	132.0
68.10	6308.0
69.10	6466.0
70.10	472.0
72.00	326.0
73.10	3045.0
74.10	11000.0
75.10	32464.0
76.10	2726.0
77.10	346.0
78.00	161.0
79.00	2737.0
80.00	828.0
81.00	2876.0
82.00	641.0
87.00	2137.0
88.00	2406.0
91.00	253.0
92.10	1961.0
93.10	2610.0
94.10	7148.0
95.10	58896.0
96.10	3780.0
97.00	108.0
104.00	288.0
105.90	318.0
116.10	240.0
117.00	641.0
117.90	337.0
119.00	513.0
128.00	235.0
128.90	140.0
130.00	205.0
137.00	115.0
141.00	740.0
143.00	1125.0
145.00	553.0
145.80	128.0
148.00	115.0
155.00	158.0
157.00	132.0
158.90	104.0
160.90	115.0
171.00	192.0
172.10	543.0
174.10	42752.0
175.10	3306.0
176.10	40784.0
177.10	2817.0
178.10	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

m/z	Abundance
36.00	571.0
37.10	3313.0
38.10	3099.0
39.10	1306.0
40.00	135.0
44.00	451.0
45.00	471.0
47.00	547.0
47.90	460.0
49.00	2701.0
50.10	12739.0
51.10	3969.0
52.20	141.0
53.00	116.0
55.00	174.0
56.00	1170.0
57.10	1766.0
60.00	621.0
61.10	3491.0
62.10	3718.0
63.10	3223.0
64.10	641.0
65.10	750.0
66.00	103.0
66.90	132.0
68.10	6403.0
69.10	6658.0
70.10	594.0
72.00	388.0
73.10	2969.0
74.10	11409.0
75.10	33608.0
76.10	2855.0
77.10	381.0
78.10	193.0
79.00	2866.0
80.00	848.0
81.00	2968.0
82.00	691.0
87.00	2183.0
88.00	2469.0
91.00	218.0
92.10	2147.0
93.10	2741.0
94.10	7529.0
95.10	61056.0
96.10	3863.0
97.00	111.0
104.00	311.0
105.90	336.0
116.10	236.0
117.00	581.0
117.90	298.0
119.00	525.0
128.00	242.0
128.90	149.0
130.00	202.0
134.90	106.0
137.00	128.0
141.00	779.0
143.00	1242.0
145.10	499.0
145.90	131.0
148.00	151.0
154.90	172.0
157.10	117.0
159.00	121.0
161.00	109.0
171.00	212.0
172.10	600.0
174.10	45248.0
175.10	3590.0
176.10	43104.0
177.10	3006.0
178.20	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

m/z	Abundance
36.00	596.0
37.10	3183.0
38.10	2845.0
39.00	1232.0
39.90	133.0
44.00	417.0
45.00	467.0
47.00	481.0
48.00	398.0
49.00	2455.0
50.10	12023.0
51.10	3734.0
52.20	125.0
53.00	114.0
55.00	180.0
56.00	1028.0
57.10	1658.0
60.00	639.0
61.10	3357.0
62.10	3331.0
63.10	2909.0
64.10	562.0
65.10	748.0
68.10	5988.0
69.10	6267.0
70.10	601.0
72.00	400.0
73.10	2753.0
74.10	10609.0
75.10	31376.0
76.10	2689.0
77.10	376.0
78.10	214.0
79.00	2736.0
80.00	833.0
81.00	2803.0
82.00	710.0
87.00	2075.0
88.00	2280.0
91.00	198.0
92.10	2124.0
93.10	2703.0
94.10	7172.0
95.10	57160.0
96.10	3558.0
104.00	294.0
106.00	294.0
116.00	227.0
117.00	470.0
117.90	253.0
119.00	449.0
128.00	227.0
128.90	123.0
130.00	213.0
135.00	141.0
137.00	114.0
141.00	775.0
143.00	1189.0
145.10	429.0
145.90	120.0
148.00	158.0
155.00	176.0
159.00	125.0
161.00	100.0
171.00	202.0
172.10	574.0
174.10	43480.0
175.10	3585.0
176.10	41840.0
177.10	2795.0
178.20	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15