

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111921\
 Data File : VU045894.D
 Acq On : 19 Nov 2021 15:00
 Operator : SY/MD
 Sample : M4752-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG1W8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU045894.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.359	3	6	14	rVB4	7816	7191	1.83%	0.267%
2	1.601	71	81	94	rVB	39968	49571	12.64%	1.842%
3	1.916	171	179	193	rVB	30758	39736	10.14%	1.476%
4	2.572	371	383	396	rBV	59036	94187	24.02%	3.500%
5	4.649	1012	1029	1081	rBV2	39570	168242	42.91%	6.251%
6	5.067	1140	1159	1180	rBV	55599	124981	31.88%	4.644%
7	5.729	1345	1365	1386	rBV2	106399	281702	71.85%	10.467%
8	6.253	1514	1528	1545	rBV	108012	202393	51.63%	7.520%
9	6.694	1652	1665	1683	rVB	69513	132961	33.91%	4.940%
10	7.568	1925	1937	1952	rBV	34329	57832	14.75%	2.149%
11	7.899	2027	2040	2056	rBV	119983	212684	54.25%	7.902%
12	7.970	2056	2062	2083	rVB2	4346	8521	2.17%	0.317%
13	8.182	2116	2128	2143	rBV	21216	33875	8.64%	1.259%
14	8.472	2209	2218	2229	rBV	2675	4530	1.16%	0.168%
15	8.636	2256	2269	2310	rBV	191196	392044	100.00%	14.567%
16	9.420	2496	2513	2534	rBV	162036	272135	69.41%	10.111%
17	10.758	2918	2929	2945	rBV	63679	102318	26.10%	3.802%
18	10.896	2962	2972	2982	rBV2	6049	9443	2.41%	0.351%
19	11.812	3246	3257	3274	rVB	163070	259790	66.27%	9.653%
20	12.063	3325	3335	3350	rBV3	8916	19011	4.85%	0.706%
21	12.195	3364	3376	3392	rVB	135510	218209	55.66%	8.108%




Sum of corrected areas: 2691356

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111921\
Data File : VU045894.D
Acq On : 19 Nov 2021 15:00
Operator : SY/MD
Sample : M4752-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG1W8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

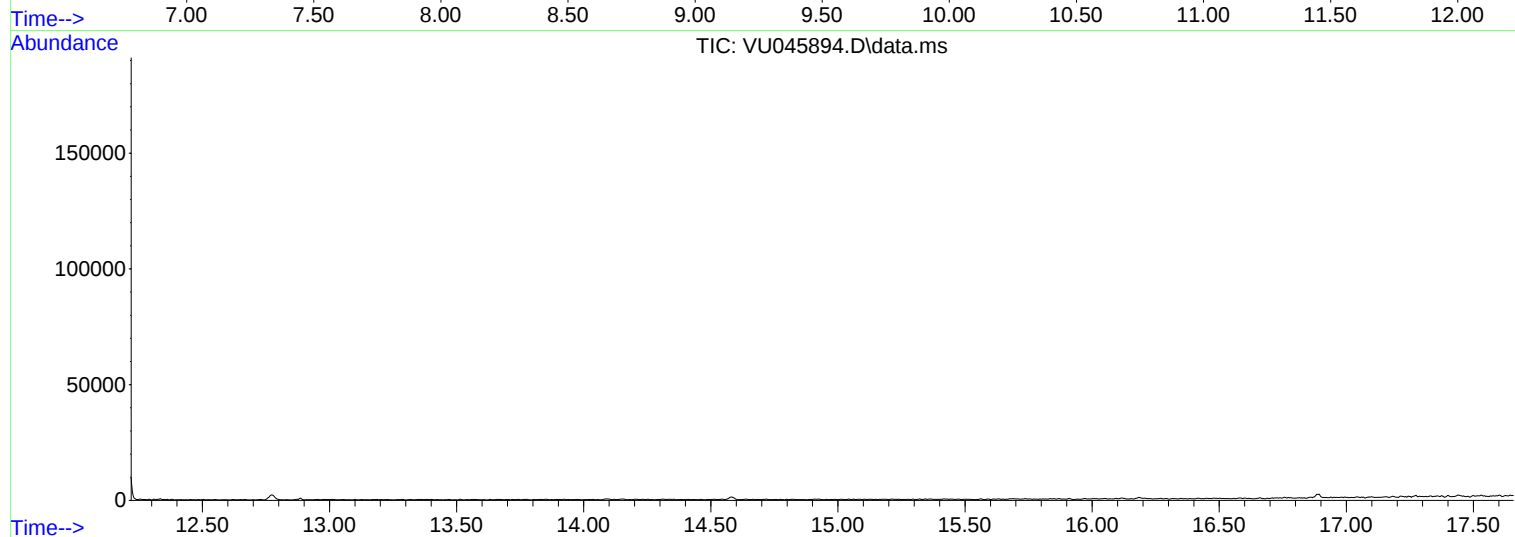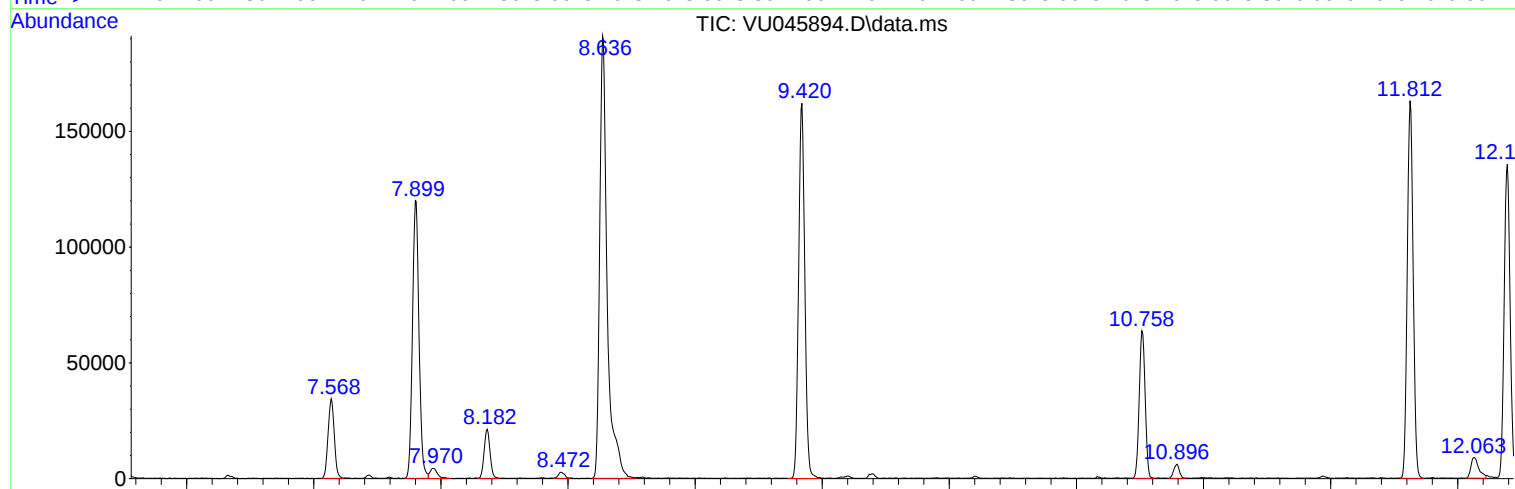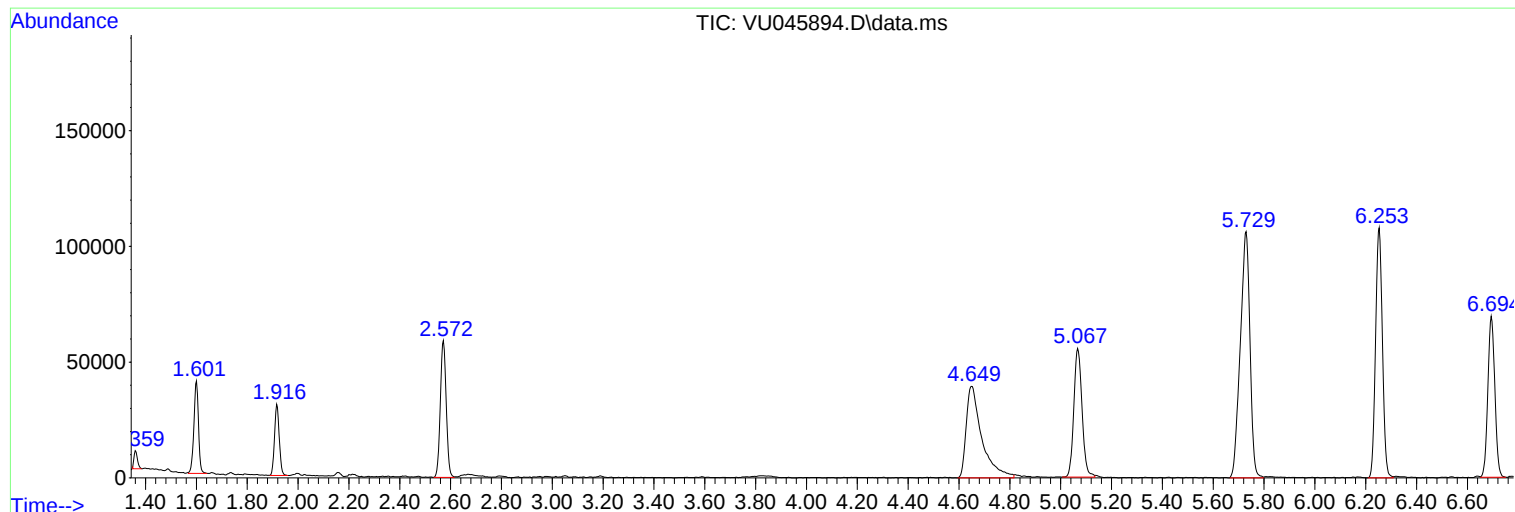

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111921\
Data File : VU045894.D
Acq On : 19 Nov 2021 15:00
Operator : SY/MD
Sample : M4752-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG1W8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111921\
Data File : VU045894.D
Acq On : 19 Nov 2021 15:00
Operator : SY/MD
Sample : M4752-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG1W8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc