
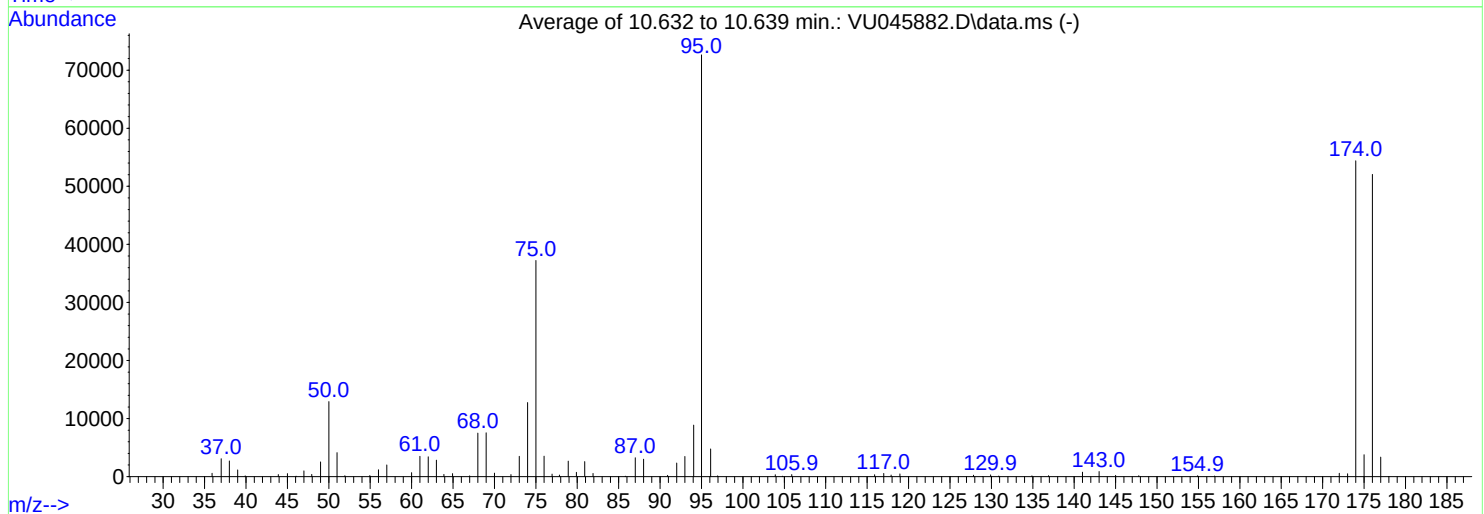


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111921\
Data File : VU045882.D
Acq On : 19 Nov 2021 09:18
Operator : SY/MD
Sample : BFB029
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB029

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Nov 26 23:26:55 2021

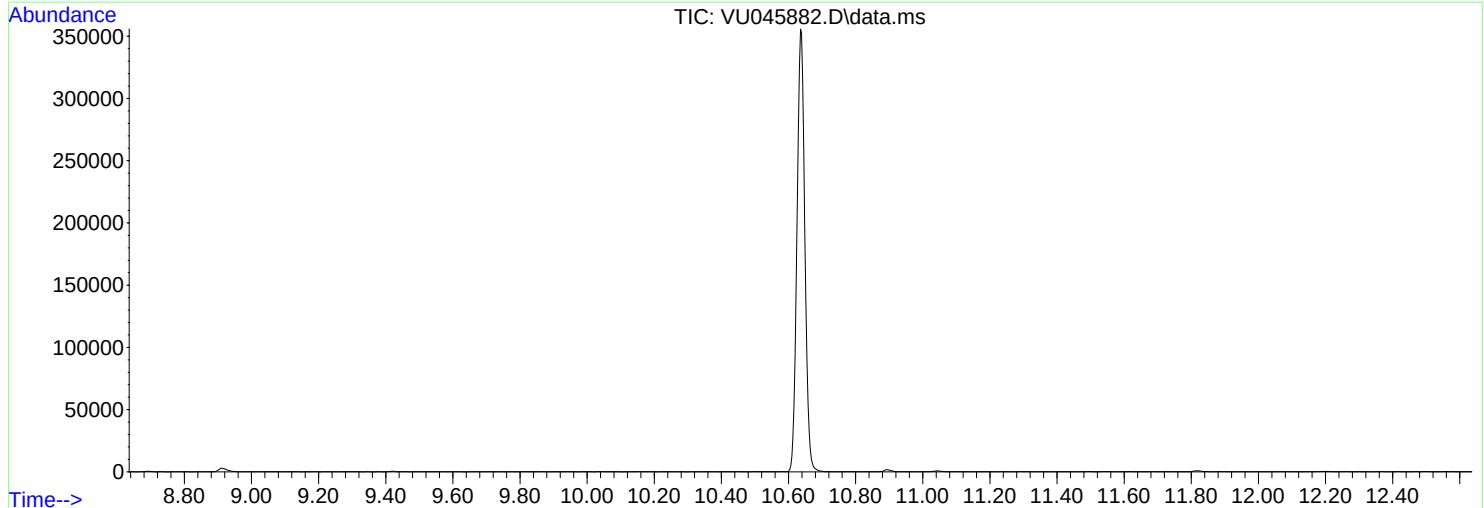

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	12930	PASS
75	95	30	80	51.3	37232	PASS
95	95	100	100	100.0	72643	PASS
96	95	5	9	6.6	4763	PASS
173	174	0.00	2	0.9	497	PASS
174	95	50	120	74.9	54389	PASS
175	174	5	9	7.0	3789	PASS
176	174	95	101	95.7	52051	PASS
177	176	5	9	6.4	3353	PASS

m/z	Abundance
35.90	636.0
37.00	3036.0
38.00	2797.0
39.00	1182.0
39.90	118.0
43.90	509.0
45.00	584.0
46.00	134.0
47.00	958.0
47.90	362.0
49.00	2674.0
50.00	12654.0
51.00	4159.0
52.00	152.0
54.90	172.0
56.00	1185.0
57.00	2013.0
60.00	721.0
61.00	3520.0
62.00	3531.0
63.00	3013.0
63.90	332.0
65.00	494.0
67.00	149.0
68.00	7671.0
69.00	7653.0
70.00	614.0
72.00	380.0
73.00	3556.0
74.00	12826.0
75.00	37928.0
76.00	3394.0
77.00	471.0
77.90	279.0
78.90	2686.0
79.90	803.0
80.90	2704.0
81.90	538.0
87.00	3369.0
88.00	3160.0
90.90	252.0
92.00	2471.0
93.00	3427.0
94.00	9263.0
95.00	74176.0
96.10	4741.0
96.90	116.0
103.90	353.0
104.80	114.0
105.90	345.0
115.90	322.0
117.00	538.0
117.90	275.0
119.00	487.0
127.90	258.0
129.90	327.0
130.90	114.0
134.90	150.0
136.90	150.0
141.00	727.0
143.00	925.0
145.00	223.0
147.80	171.0
154.90	173.0
157.00	107.0
172.00	595.0
173.00	535.0
174.00	56632.0
175.00	3871.0
176.00	53952.0
177.00	3380.0
178.00	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB029

m/z	Abundance
43.90	153.0

Instrument :
MSVOA_U
ClientSampleId :
BFB029

m/z	Abundance
35.90	523.0
37.00	3032.0
38.00	2580.0
39.00	1098.0
39.90	153.0
44.00	503.0
45.00	464.0
47.00	983.0
48.00	411.0
49.00	2317.0
50.00	12828.0
51.00	3978.0
51.90	192.0
54.90	212.0
56.00	1165.0
57.00	1933.0
60.00	648.0
61.00	3394.0
62.00	3221.0
63.00	2564.0
63.90	455.0
64.90	547.0
67.00	150.0
68.00	7058.0
69.00	7257.0
70.00	564.0
72.00	345.0
73.00	3319.0
74.00	12304.0
75.00	35456.0
76.00	3530.0
76.90	397.0
77.80	239.0
78.90	2574.0
79.90	666.0
80.90	2421.0
81.90	559.0
85.80	138.0
87.00	3029.0
88.00	2757.0
90.90	208.0
92.00	2130.0
93.00	3366.0
94.10	8201.0
95.00	68680.0
96.10	4608.0
97.00	167.0
103.90	313.0
105.90	340.0
115.90	303.0
117.00	520.0
117.90	263.0
118.90	459.0
127.80	227.0
129.90	292.0
130.90	118.0
134.90	146.0
136.90	156.0
141.00	777.0
143.00	804.0
145.00	230.0
147.80	151.0
154.90	137.0
156.90	108.0
172.00	554.0
173.00	439.0
174.00	50376.0
175.00	3572.0
176.00	48408.0
177.00	3210.0

Instrument :
MSVOA_U
ClientSampleId :
BFB029

m/z	Abundance
35.90	618.0
37.00	3225.0
38.00	2756.0
39.00	1182.0
39.90	146.0
43.90	505.0
45.00	524.0
46.10	128.0
47.00	1064.0
47.90	389.0
49.00	2631.0
50.00	13307.0
51.00	4305.0
52.00	185.0
55.00	216.0
56.00	1228.0
57.00	2083.0
60.00	730.0
61.00	3631.0
62.00	3500.0
63.00	2944.0
63.90	393.0
65.00	524.0
67.00	147.0
68.00	7727.0
69.00	7756.0
70.00	618.0
72.00	367.0
73.00	3648.0
74.00	13129.0
75.00	38312.0
76.00	3681.0
76.90	448.0
77.90	275.0
78.90	2723.0
79.90	767.0
80.90	2635.0
81.90	568.0
85.80	134.0
87.00	3373.0
88.00	3085.0
90.90	223.0
92.00	2471.0
93.00	3629.0
94.00	9152.0
95.00	75072.0
96.10	4939.0
96.90	140.0
103.90	352.0
104.80	109.0
105.90	364.0
115.90	337.0
117.00	564.0
117.90	281.0
118.90	493.0
127.80	267.0
128.90	104.0
129.90	334.0
130.90	134.0
134.90	150.0
136.90	169.0
141.00	794.0
143.00	943.0
145.00	240.0
147.80	177.0
154.90	157.0
157.00	105.0
172.00	603.0
173.00	517.0
174.00	56160.0
175.00	3924.0
176.00	53792.0
177.00	3468.0

Instrument :
MSVOA_U
ClientSampleId :
BFB029