

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU111922\
 Data File : VU051950.D
 Acq On : 19 Nov 2022 13:00
 Operator : JC/MD
 Sample : N5693-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBN88


Quant Time: Nov 19 21:43:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 19 21:39:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	223280	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	228285	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	87306	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	104923	4.831	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.600%
7) Chloroethane-d5	1.906	69	85544	5.071	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.400%
11) 1,1-Dichloroethene-d2	2.565	65	36555	4.696	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	94.000%
20) 2-Butanone-d5	4.616	46	198825	50.505	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.000%
24) Chloroform-d	5.060	84	160377	5.026	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.600%
26) 1,2-Dichloroethane-d4	5.700	65	81560	5.060	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.200%
32) Benzene-d6	5.726	84	333058	4.914	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%
36) 1,2-Dichloropropane-d6	6.687	67	109142	5.204	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.000%
41) Toluene-d8	7.896	98	262385	4.279	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.600%
43) trans-1,3-Dichloroprop...	8.179	79	33578	4.393	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.800%
46) 2-Hexanone-d5	8.629	63	150116	46.345	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.680%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	90952	5.001	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.000%
66) 1,2-Dichlorobenzene-d4	12.192	152	91501	5.474	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.400%
Target Compounds						Qvalue
5) Vinyl chloride	1.604	62	3226	0.133	ug/L #	1
10) 1,1,2-Trichloro-1,2,2-...	2.565	101	1174	0.072	ug/L #	1
13) Acetone	2.620	43	315268	117.933	ug/L	98
15) Methyl Acetate	3.038	43	1130	0.163	ug/L #	48
16) Methylene chloride	3.044	84	67457	3.078	ug/L	99
17) Methyl tert-butyl Ether	3.359	73	3945	0.109	ug/L #	91
18) trans-1,2-Dichloroethene	3.350	96	2065	0.119	ug/L	94
22) cis-1,2-Dichloroethene	4.665	96	136655	7.499	ug/L	99
27) 1,2-Dichloroethane	5.793	62	15427	0.794	ug/L #	91
33) Benzene	5.774	78	28173	0.379	ug/L	100
34) Trichloroethene	6.539	95	172803	9.325	ug/L	97
35) Methylcyclohexane	6.687	83	23605	0.886	ug/L #	20
37) 1,2-Dichloropropane	6.687	63	10888	0.566	ug/L #	88
39) cis-1,3-Dichloropropene	7.565	75	2377	0.096	ug/L #	52
49) Dibromochloromethane	8.555	129	1400	0.086	ug/L #	12
61) 1,2,3-Trichloropropane	11.809	75	9870	0.988	ug/L #	68

(#) = qualifier out of range (m) = manual integration (+) = signals summed





Instrument :
MSVOA_U
ClientSampleId :
GBN88

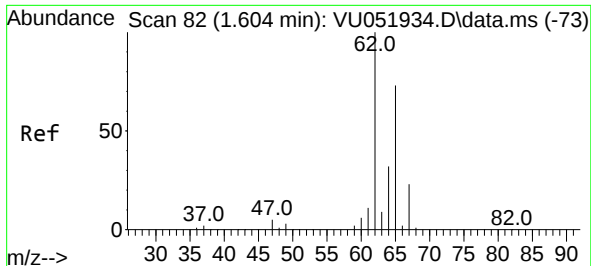

#5
 Vinyl chloride
 Concen: 0.133 ug/L
 RT: 1.604 min Scan# 81
 Delta R.T. -0.000 min
 Lab File: VU051950.D
 Acq: 19 Nov 2022 13:00




Instrument :
 MSVOA_U
 ClientSampleId :
 GBN88


Tgt Ion: 62 Resp: 3226
 Ion Ratio Lower Upper
 62 100
 64 142.1 23.5 43.7#

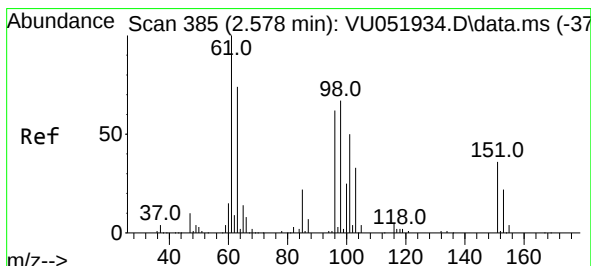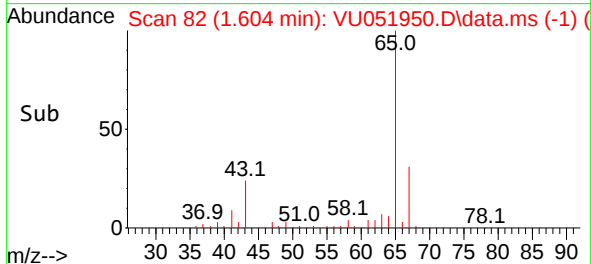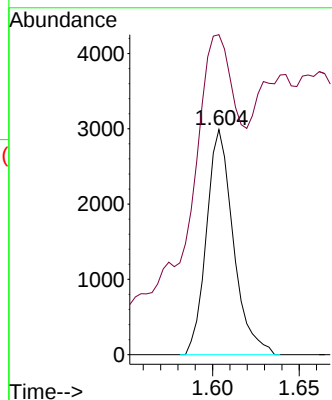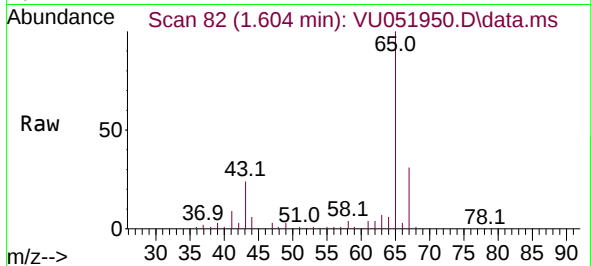

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.072 ug/L
 RT: 2.565 min Scan# 381
 Delta R.T. -0.013 min
 Lab File: VU051950.D
 Acq: 19 Nov 2022 13:00

Tgt Ion: 101 Resp: 1174
 Ion Ratio Lower Upper
 101 100
 85 597.4 33.8 50.6#
 151 0.0 58.6 88.0#

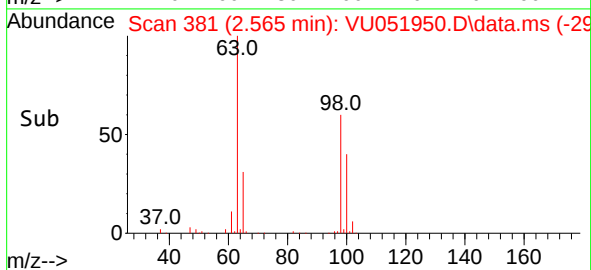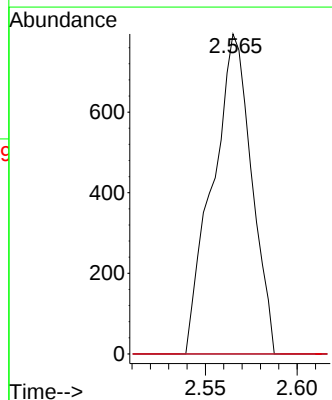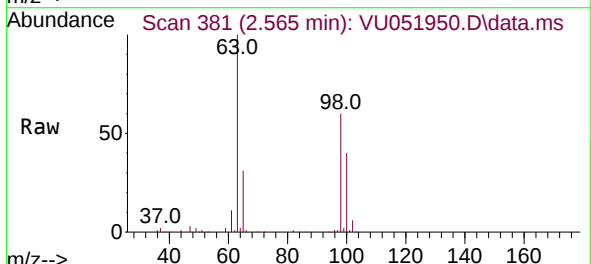

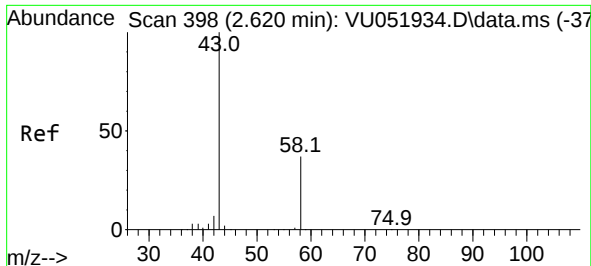

#13

Acetone

Concen: 117.933 ug/L

RT: 2.620 min Scan# 398

Delta R.T. -0.000 min

Lab File: VU051950.D

Acq: 19 Nov 2022 13:00

Instrument :

MSVOA_U

ClientSampleId :





GBN88

Tgt Ion: 43 Resp: 315268

Ion Ratio Lower Upper

43 100

58 36.8 0.0 76.0

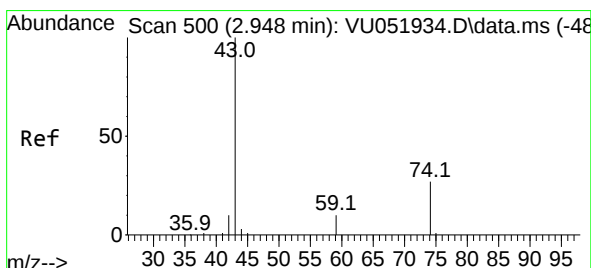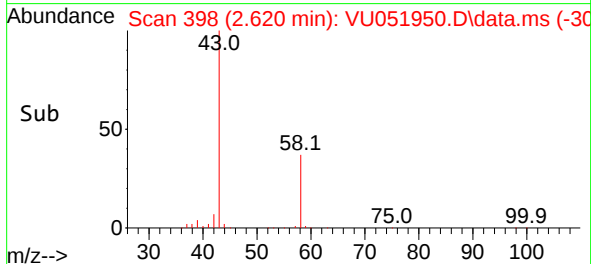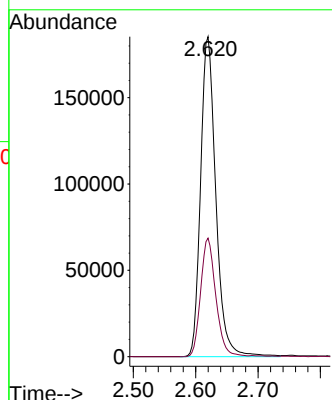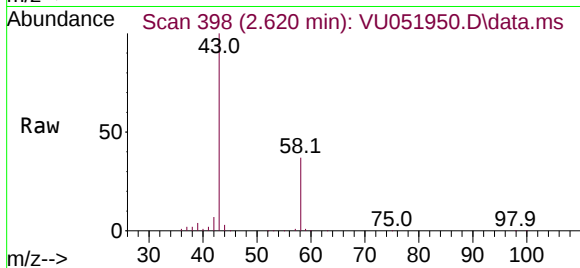

#15

Methyl Acetate

Concen: 0.163 ug/L

RT: 3.038 min Scan# 528

Delta R.T. 0.090 min

Lab File: VU051950.D




Acq: 19 Nov 2022 13:00


Tgt Ion: 43 Resp: 1130

Ion Ratio Lower Upper

43 100

74 0.0 21.3 31.9#


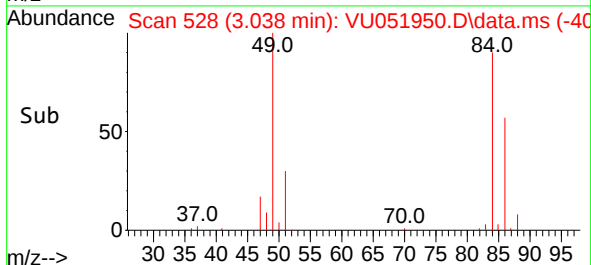
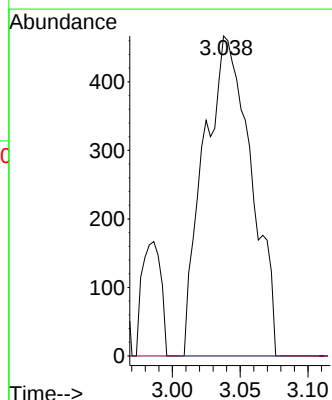
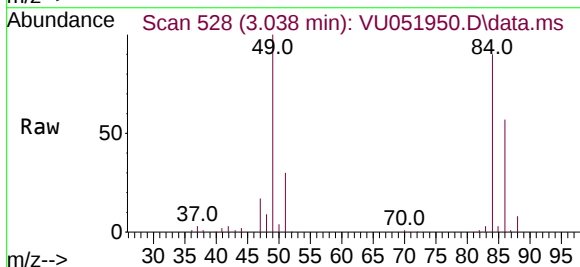




#16
Methylene chloride
Concen: 3.078 ug/L
RT: 3.044 min Scan# 51
Delta R.T. -0.000 min
Lab File: VU051950.D
Acq: 19 Nov 2022 13:00




Instrument :
MSVOA_U
ClientSampleId :
GBN88


Tgt Ion: 84 Resp: 67457
Ion Ratio Lower Upper
84 100
86 63.1 43.8 81.4
49 110.1 75.9 141.1

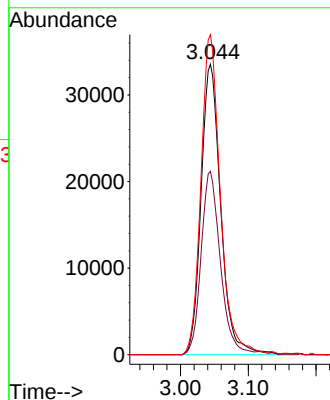

#17
Methyl tert-butyl Ether
Concen: 0.109 ug/L
RT: 3.359 min Scan# 628
Delta R.T. -0.000 min
Lab File: VU051950.D
Acq: 19 Nov 2022 13:00

Tgt Ion: 73 Resp: 3945
Ion Ratio Lower Upper
73 100
43 19.1 13.2 19.8
57 16.8 17.8 26.8#

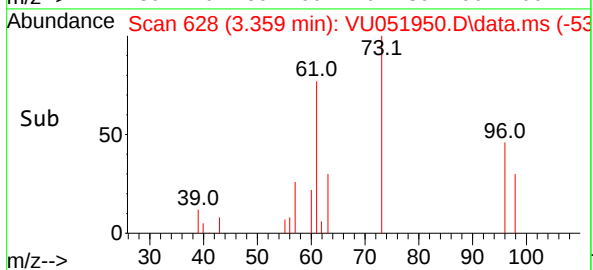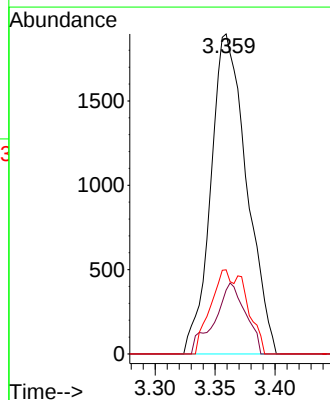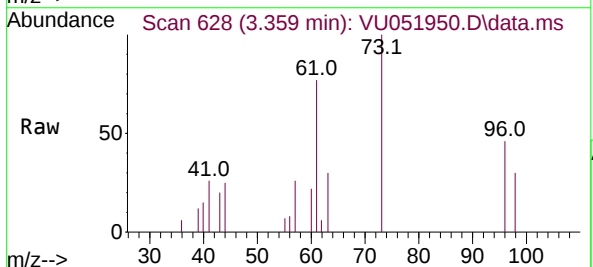



#18

trans-1,2-Dichloroethene

Concen: 0.119 ug/L

RT: 3.350 min Scan# 61

Delta R.T. -0.003 min

Lab File: VU051950.D

Acq: 19 Nov 2022 13:00

Instrument :

MSVOA_U

ClientSampleId :

GBN88





Tgt Ion: 96 Resp: 2065

Ion Ratio Lower Upper

96 100

61 139.7 97.9 181.7

98 48.2 43.8 81.3

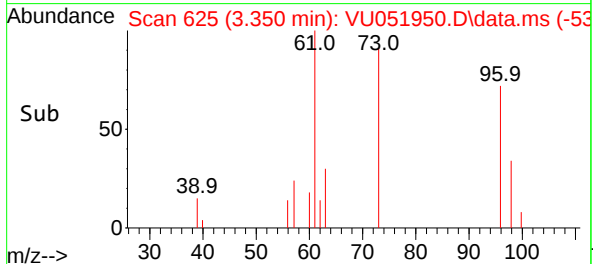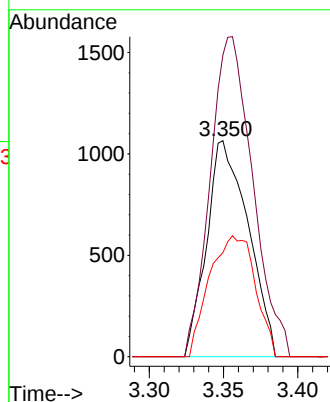

#22

cis-1,2-Dichloroethene

Concen: 7.499 ug/L

RT: 4.665 min Scan# 1034

Delta R.T. -0.000 min

Lab File: VU051950.D

Acq: 19 Nov 2022 13:00




Tgt Ion: 96 Resp: 136655


Ion Ratio Lower Upper

96 100

61 121.8 85.1 158.1

98 64.2 42.8 79.6

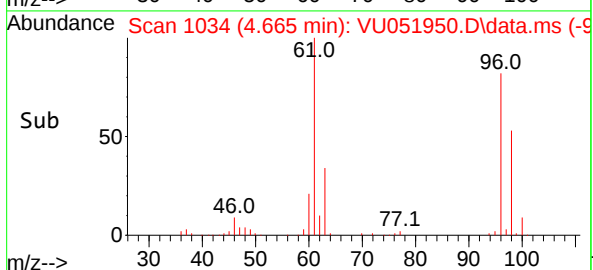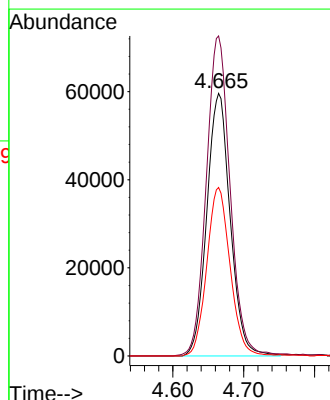



#27

1,2-Dichloroethane

Concen: 0.794 ug/L

RT: 5.793 min Scan# 1

Delta R.T. 0.003 min

Lab File: VU051950.D

Acq: 19 Nov 2022 13:00

Instrument :

MSVOA_U

ClientSampleId :





GBN88

Tgt Ion: 62 Resp: 15427

Ion Ratio Lower Upper

62 100

98 7.0 8.4 12.6#

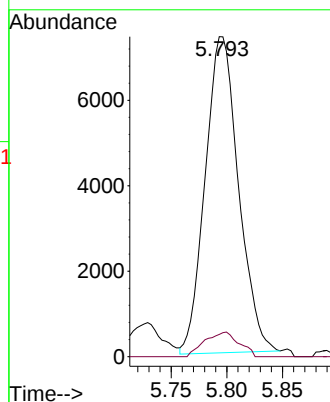

#33

Benzene

Concen: 0.379 ug/L




RT: 5.774 min Scan# 1379


Delta R.T. 0.003 min

Lab File: VU051950.D

Acq: 19 Nov 2022 13:00

Tgt Ion: 78 Resp: 28173


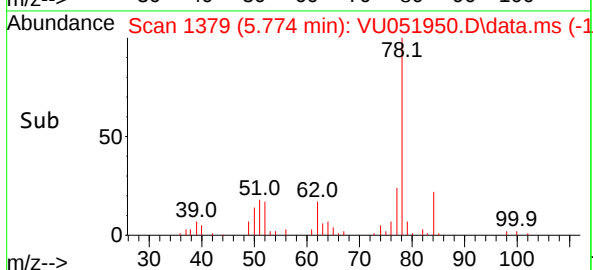
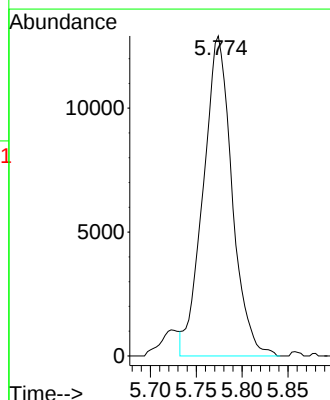





#34
Trichloroethene
Concen: 9.325 ug/L
RT: 6.539 min Scan# 1617
Delta R.T. -0.000 min
Lab File: VU051950.D
Acq: 19 Nov 2022 13:00




Instrument :
MSVOA_U
ClientSampleId :
GBN88


Tgt Ion: 95 Resp: 172803
Ion Ratio Lower Upper
95 100
97 64.5 43.7 81.1
132 95.8 64.3 119.3
130 97.9 67.3 124.9

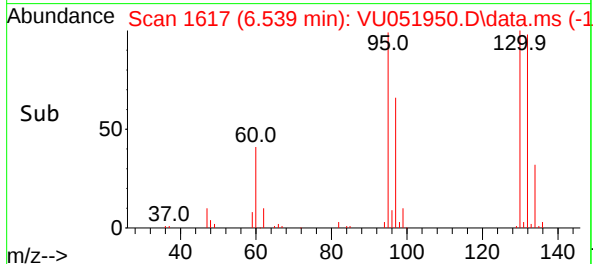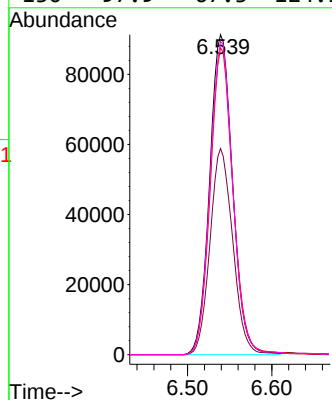

#35
Methylcyclohexane
Concen: 0.886 ug/L
RT: 6.687 min Scan# 1663
Delta R.T. -0.074 min
Lab File: VU051950.D
Acq: 19 Nov 2022 13:00

Tgt Ion: 83 Resp: 23605
Ion Ratio Lower Upper
83 100
55 0.0 60.8 91.2#
98 1.0 35.1 52.7#

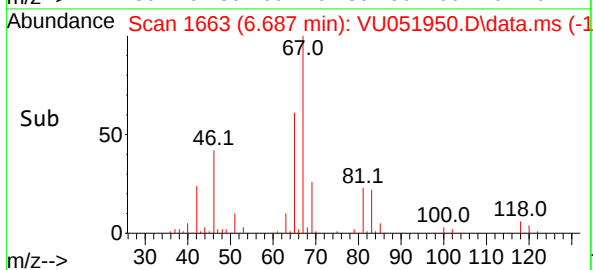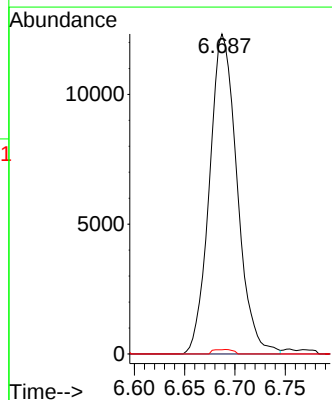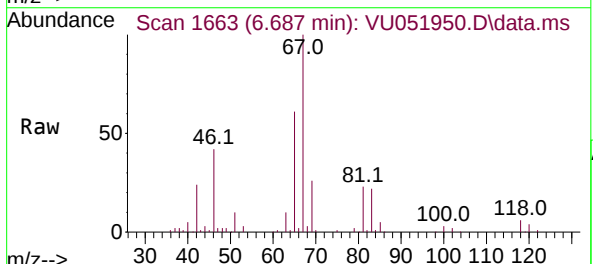



#37

1,2-Dichloropropane

Concen: 0.566 ug/L

RT: 6.687 min Scan# 1

Delta R.T. -0.100 min

Lab File: VU051950.D

Acq: 19 Nov 2022 13:00

Instrument :

MSVOA_U

ClientSampleId :





GBN88

Tgt Ion: 63 Resp: 10888

Ion Ratio Lower Upper

63 100

112 0.0 3.3 4.9#

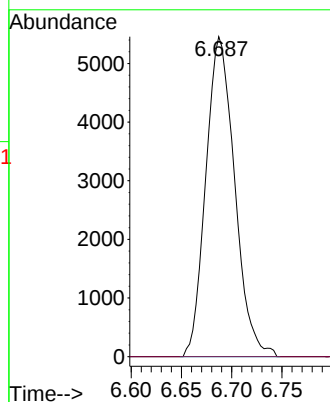

#39

cis-1,3-Dichloropropene

Concen: 0.096 ug/L

RT: 7.565 min Scan# 1936

Delta R.T. -0.039 min

Lab File: VU051950.D




Acq: 19 Nov 2022 13:00


Tgt Ion: 75 Resp: 2377

Ion Ratio Lower Upper

75 100

77 57.8 22.0 40.8#

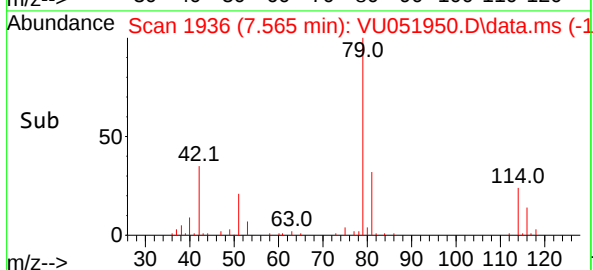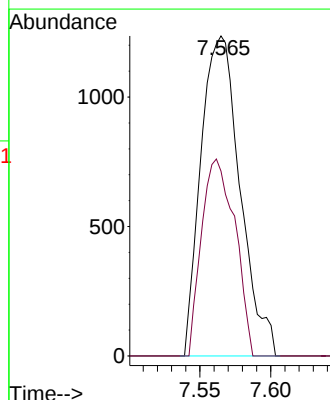



#49

Dibromochloromethane

Concen: 0.086 ug/L

RT: 8.555 min Scan# 21

Delta R.T. -0.251 min

Lab File: VU051950.D

Acq: 19 Nov 2022 13:00

Instrument :

MSVOA_U

ClientSampleId :





GBN88

Tgt Ion:129 Resp: 1400

Ion Ratio Lower Upper

129 100

127 0.0 52.8 98.2#

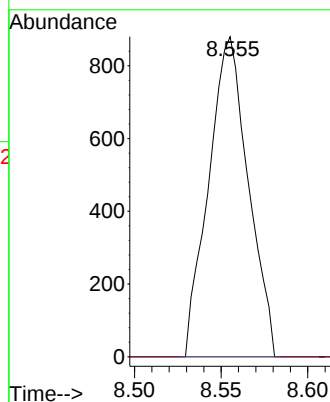

#61

1,2,3-Trichloropropane

Concen: 0.988 ug/L

RT: 11.809 min Scan# 3256

Delta R.T. 0.990 min

Lab File: VU051950.D

Acq: 19 Nov 2022 13:00

Tgt Ion: 75 Resp: 9870

Ion Ratio Lower Upper

75 100

110 1.8 28.3 42.5#

77 35.0 26.2 39.2

